

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD040723AL\
Data File : FD045456.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2023 11:22
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:18:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 05:57:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.554	52008	0.399 ug/ml
21) T	n-Octatriacontane (C38)	20.595	61018	0.556 ug/ml
22) T	n-Tetracontane (C40)	21.429	78578	0.732 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD040723AL\
Data File : FD045456.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2023 11:22
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:18:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 05:57:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

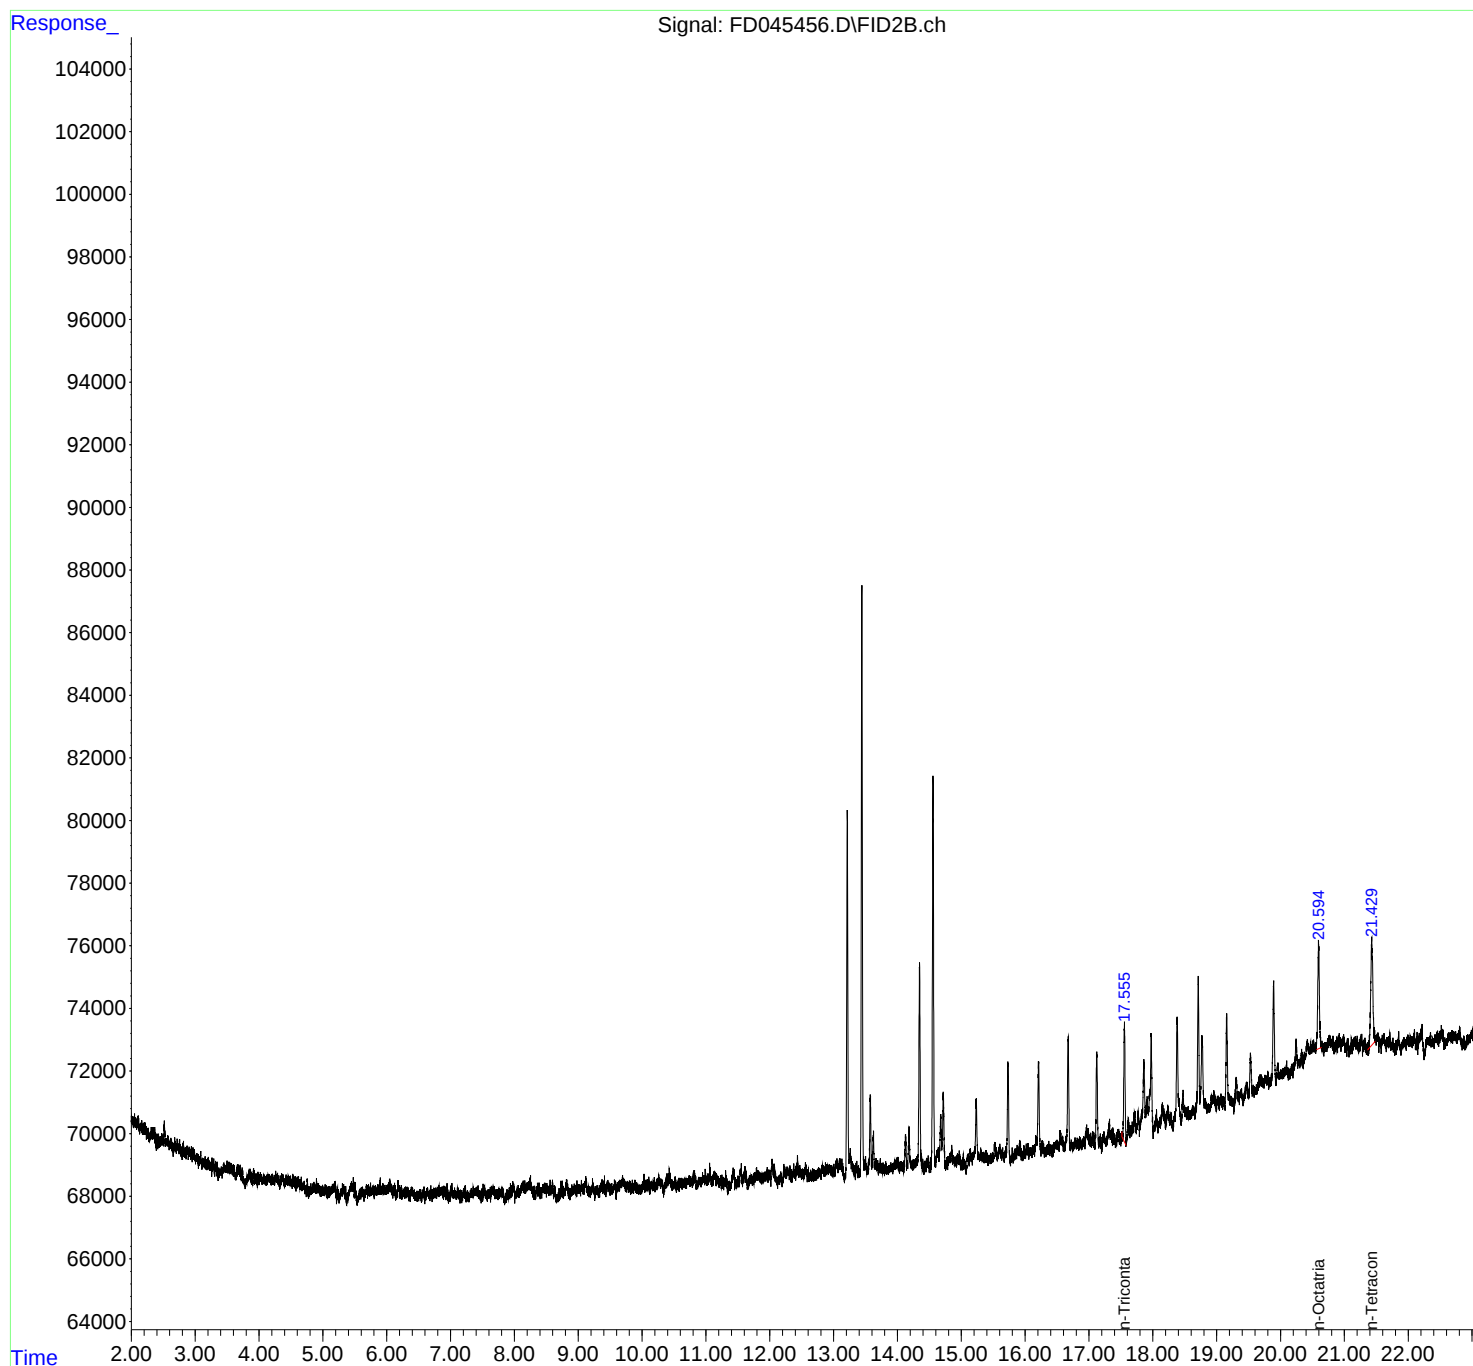


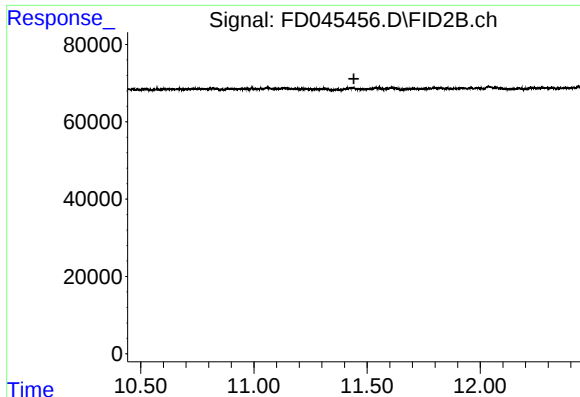

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.442 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

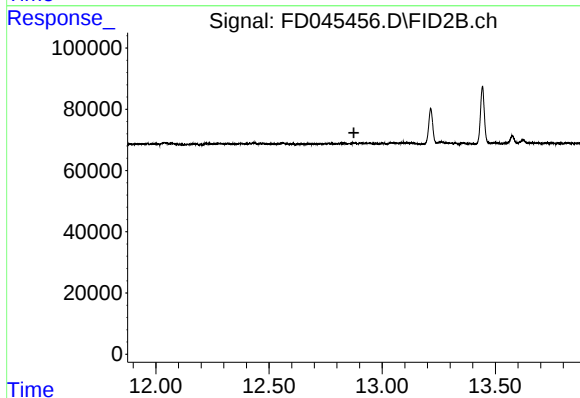


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.875 min
Response: 0
Conc: N.D.

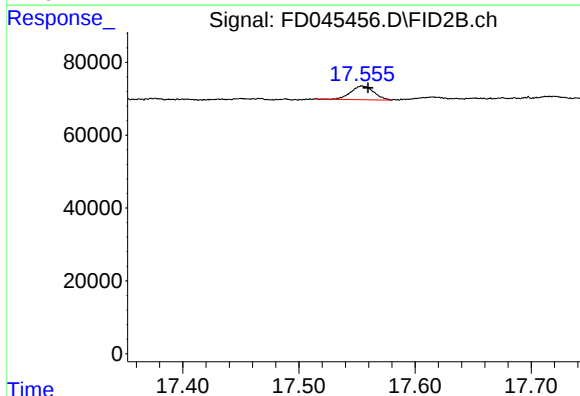


#17 n-Tricontane (C30)

R.T.: 17.554 min
Delta R.T.: -0.005 min
Response: 52008
Conc: 0.40 ug/ml

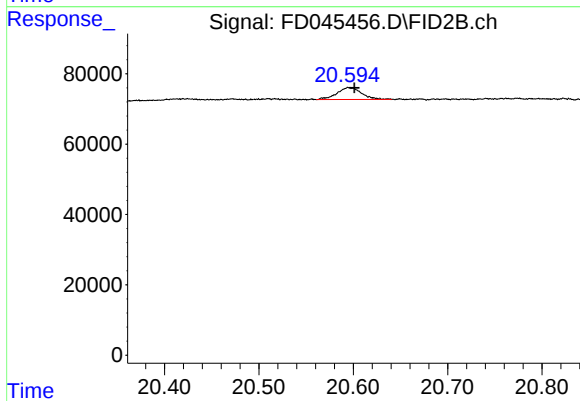

#21 n-Octatriacontane (C38)

R.T.: 20.595 min
Delta R.T.: -0.006 min
Response: 61018
Conc: 0.56 ug/ml

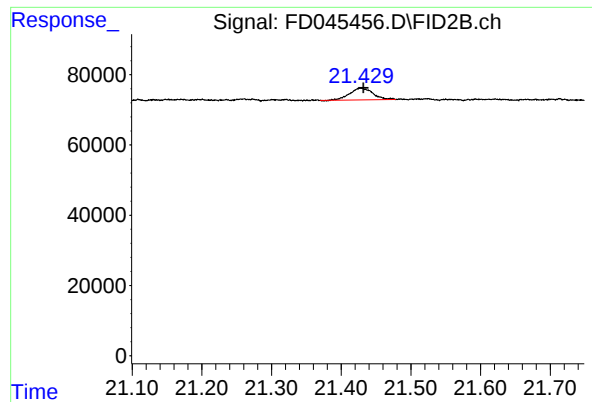

#22 n-Tetracontane (C40)

R.T.: 21.429 min
Delta R.T.: -0.003 min
Response: 78578
Conc: 0.73 ug/ml

Instrument :

FID_D

ClientSampleId :