

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD040723AR\
Data File : FD045434.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2023 08:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:40:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 0302823.M
Quant Title : GC Extractables
QLast Update : Tue Mar 28 05:56:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T Indeno[1,2,3-cd]pyren...	17.946	69874	0.590 ug/ml
20) T Dibenz[a,h]anthracene...	17.946	69874	0.587 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD040723AR\
Data File : FD045434.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2023 08:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:40:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 0302823.M
Quant Title : GC Extractables
QLast Update : Tue Mar 28 05:56:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

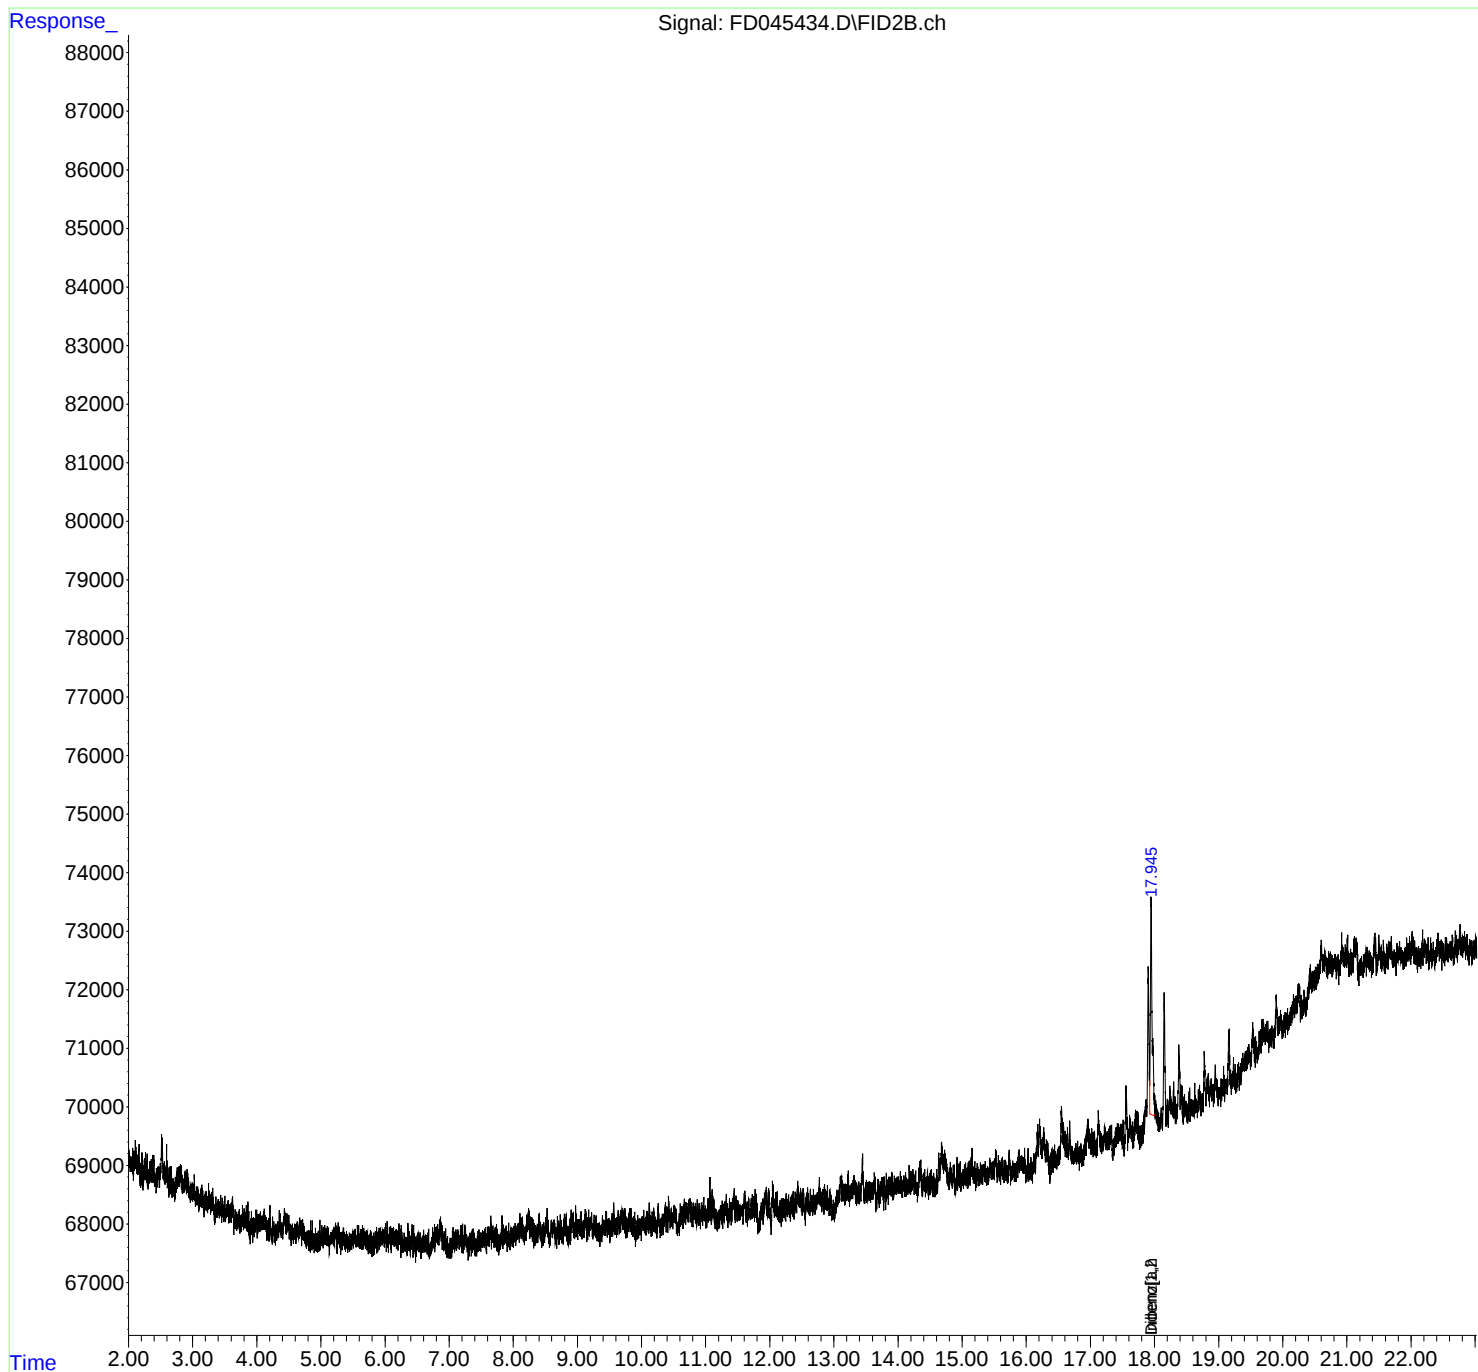


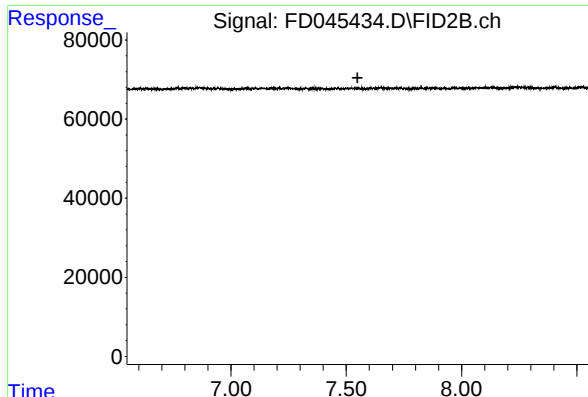

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T.: 7.549 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

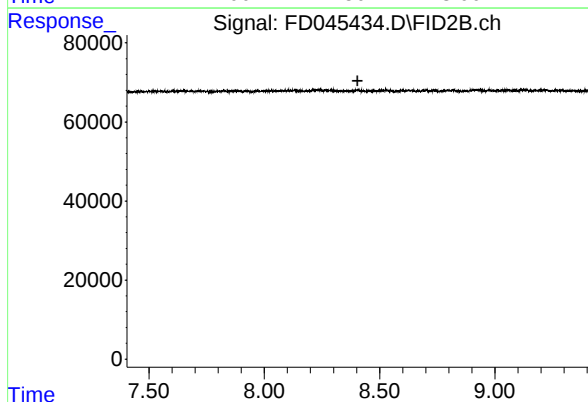


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 8.404 min
Response: 0
Conc: N.D.

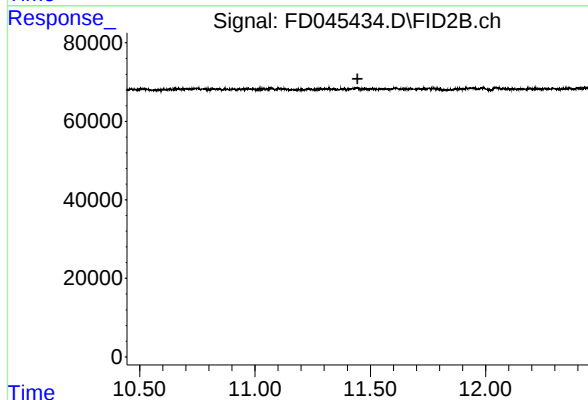


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.444 min
Response: 0
Conc: N.D.

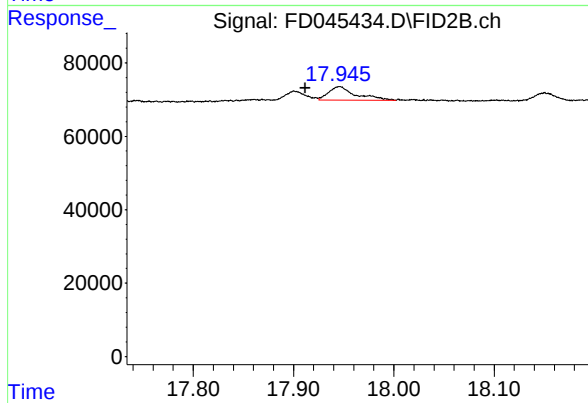

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.946 min
Delta R.T.: 0.034 min
Response: 69874
Conc: 0.59 ug/ml

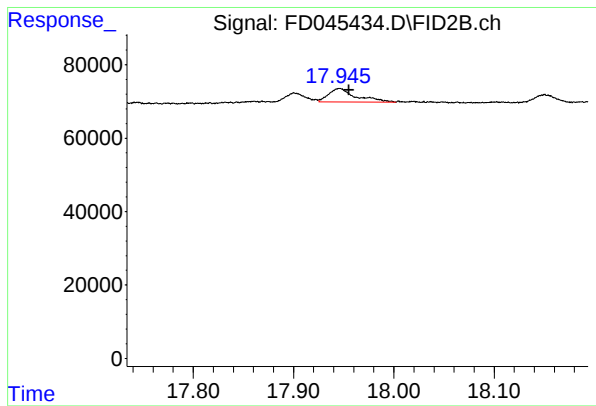

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.946 min

Delta R.T.: -0.010 min

Response: 69874

Conc: 0.59 ug/ml

Instrument :

FID_D

ClientSampleId :