

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD041122AL\
 Data File : FD041940.D
 Signal(s) : FID2B.CH
 Acq On : 11 Apr 2022 20:13
 Operator : UA/NP
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 02:39:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 032222.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 23 05:05:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

15) T	n-Hexacosane (C26)	15.527	621384	3.847 ug/ml
16) T	n-Octacosane (C28)	16.460	439827	2.732 ug/ml
17) T	n-Tricontane (C30)	17.358	702913	4.460 ug/ml
18) T	n-Dotriacontane (C32)	18.177	290199	1.956 ug/ml
19) T	n-Tetratriacontane (C34)	18.953	537140	4.009 ug/ml
20) T	n-Hexatriacontane (C36)	19.700	1281764	10.704 ug/ml
21) T	n-Octatriacontane (C38)	20.412	818418	7.394 ug/ml
22) T	n-Tetracontane (C40)	21.176	748108	6.949 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD041122AL\
Data File : FD041940.D
Signal(s) : FID2B.CH
Acq On : 11 Apr 2022 20:13
Operator : UA/NP
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:39:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 032222.M
Quant Title : GC Extractables
QLast Update : Wed Mar 23 05:05:55 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

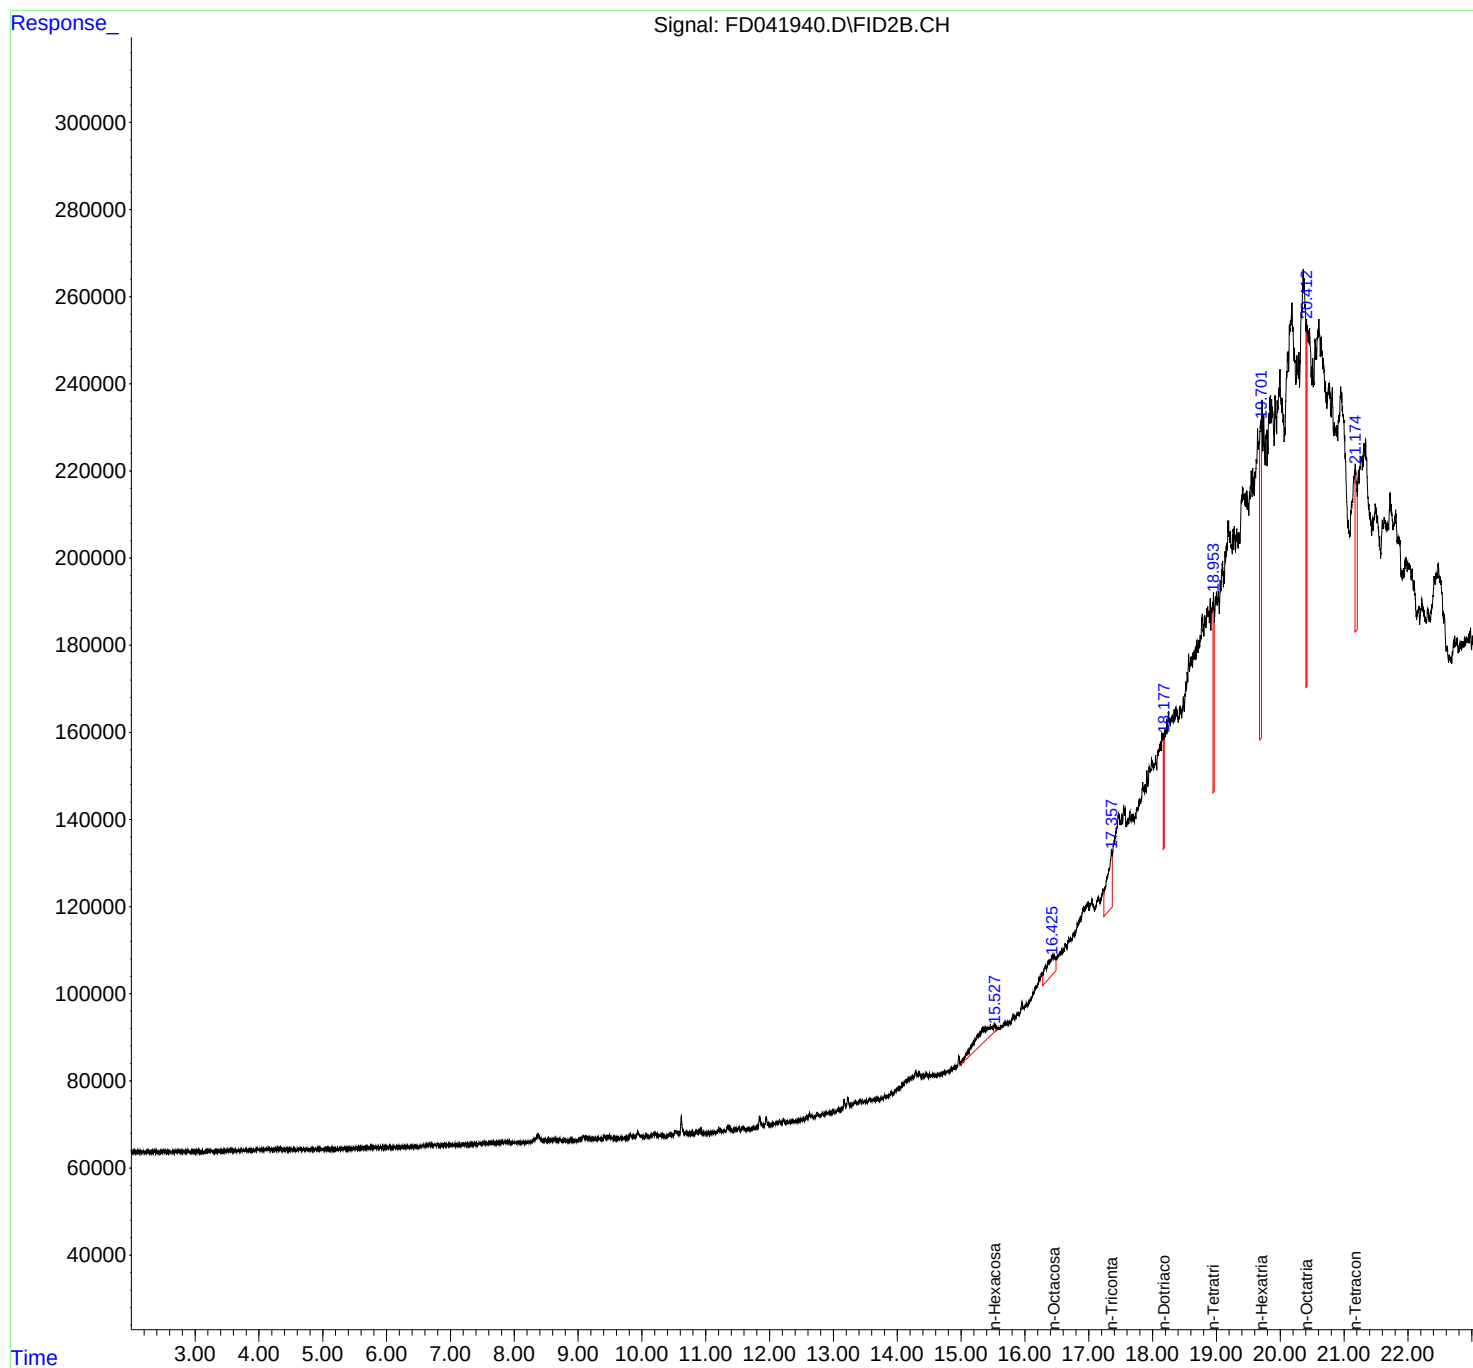


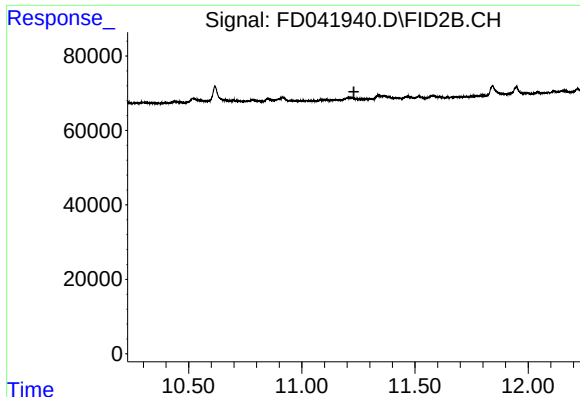

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.230 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

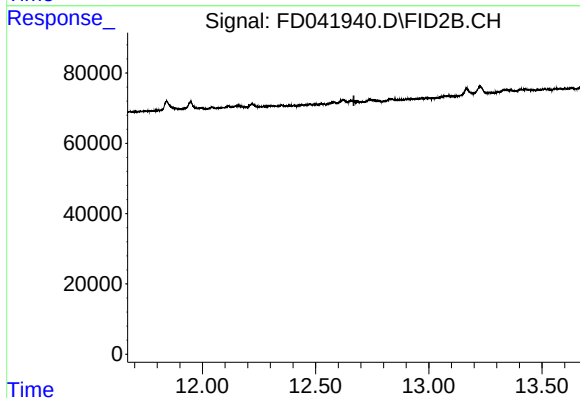


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.669 min
Response: 0
Conc: N.D.

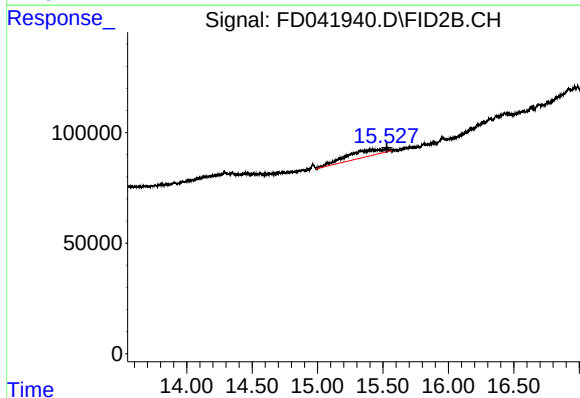


#15 n-Hexacosane (C26)

R.T.: 15.527 min
Delta R.T.: -0.003 min
Response: 621384
Conc: 3.85 ug/ml

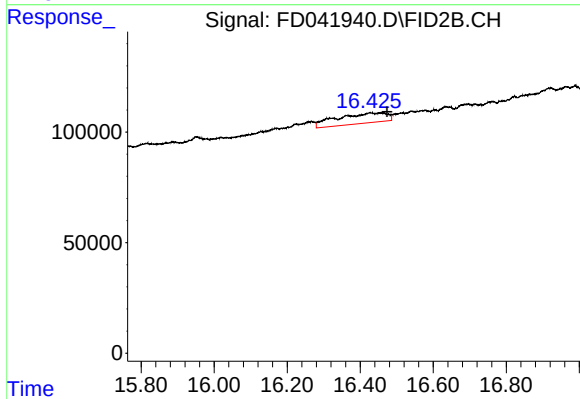

#16 n-Octacosane (C28)


R.T.: 16.460 min
Delta R.T.: -0.014 min
Response: 439827
Conc: 2.73 ug/ml

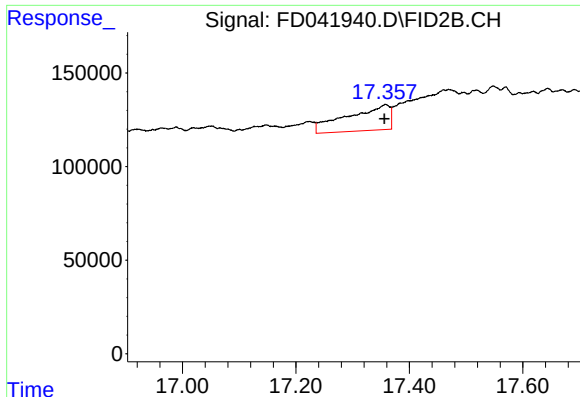

#17 n-Tricontane (C30)


R.T.: 17.358 min
Delta R.T.: 0.003 min
Response: 702913
Conc: 4.46 ug/ml

Instrument :
FID_D
ClientSampleId :

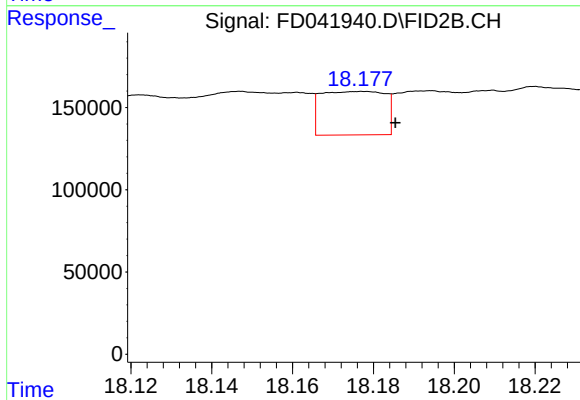


#18 n-Dotriacontane (C32)

R.T.: 18.177 min
Delta R.T.: -0.008 min
Response: 290199
Conc: 1.96 ug/ml

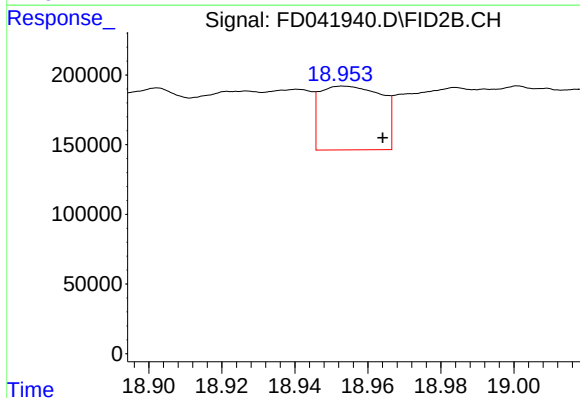


#19 n-Tetratriacontane (C34)

R.T.: 18.953 min
Delta R.T.: -0.011 min
Response: 537140
Conc: 4.01 ug/ml

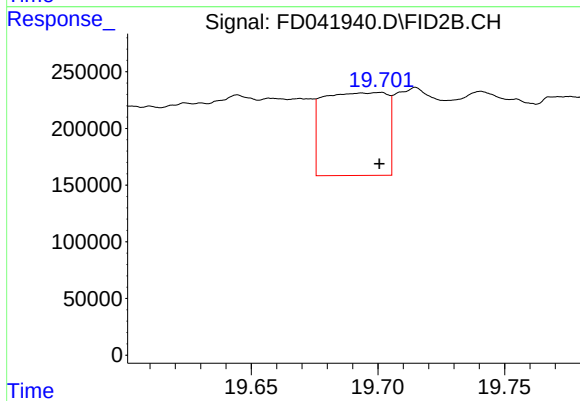

#20 n-Hexatriacontane (C36)

R.T.: 19.700 min
Delta R.T.: 0.000 min
Response: 1281764
Conc: 10.70 ug/ml

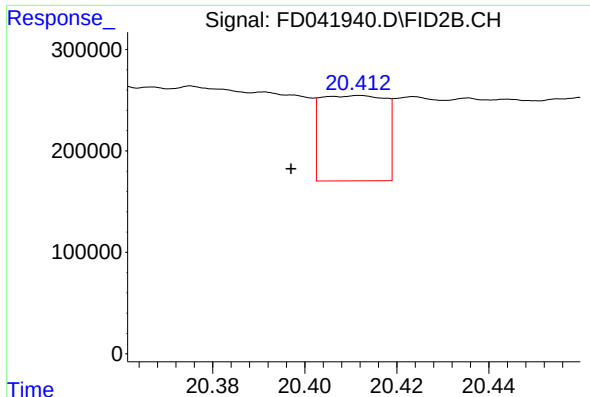


#21 n-Octatriacontane (C38)

R.T.: 20.412 min
Delta R.T.: 0.015 min
Response: 818418
Conc: 7.39 ug/ml

Instrument :

FID_D

ClientSampleId :

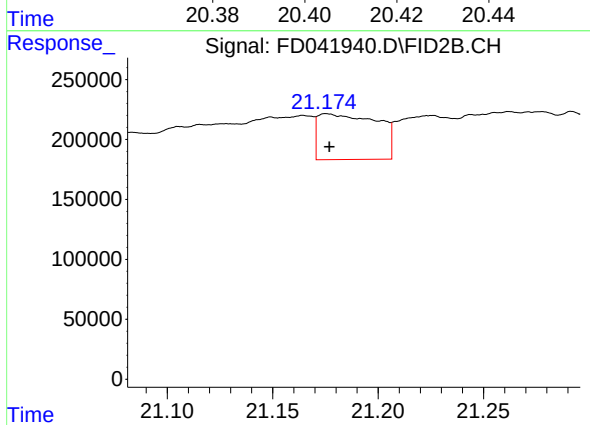

#22 n-Tetracontane (C40)

R.T.: 21.176 min
Delta R.T.: -0.001 min
Response: 748108
Conc: 6.95 ug/ml