

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD042821AL\
 Data File : FD037216.D
 Signal(s) : FID2B.CH
 Acq On : 28 Apr 2021 17:14
 Operator : DD\AJ
 Sample : M2170-15DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 29 02:42:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 042121.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 22 03:31:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.472	2001023	17.137 ug/ml
Spiked Amount 50.000		Recovery =	34.27%
12) S 1-chlorooctadecane (S...	12.907	1566866	18.521 ug/ml
Spiked Amount 50.000		Recovery =	37.04%
Target Compounds			
10) T n-Eicosane (C20)	12.514	852339	8.035 ug/ml
14) T n-Tetracosane (C24)	14.720	396238	3.912 ug/ml
16) T n-Octacosane (C28)	16.707	166800	1.735 ug/ml
18) T n-Dotriacontane (C32)	18.394	114838	1.168 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD042821AL\
Data File : FD037216.D
Signal(s) : FID2B.CH
Acq On : 28 Apr 2021 17:14
Operator : DD\AJ
Sample : M2170-15DL 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 29 02:42:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 042121.M
Quant Title : GC Extractables
QLast Update : Thu Apr 22 03:31:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

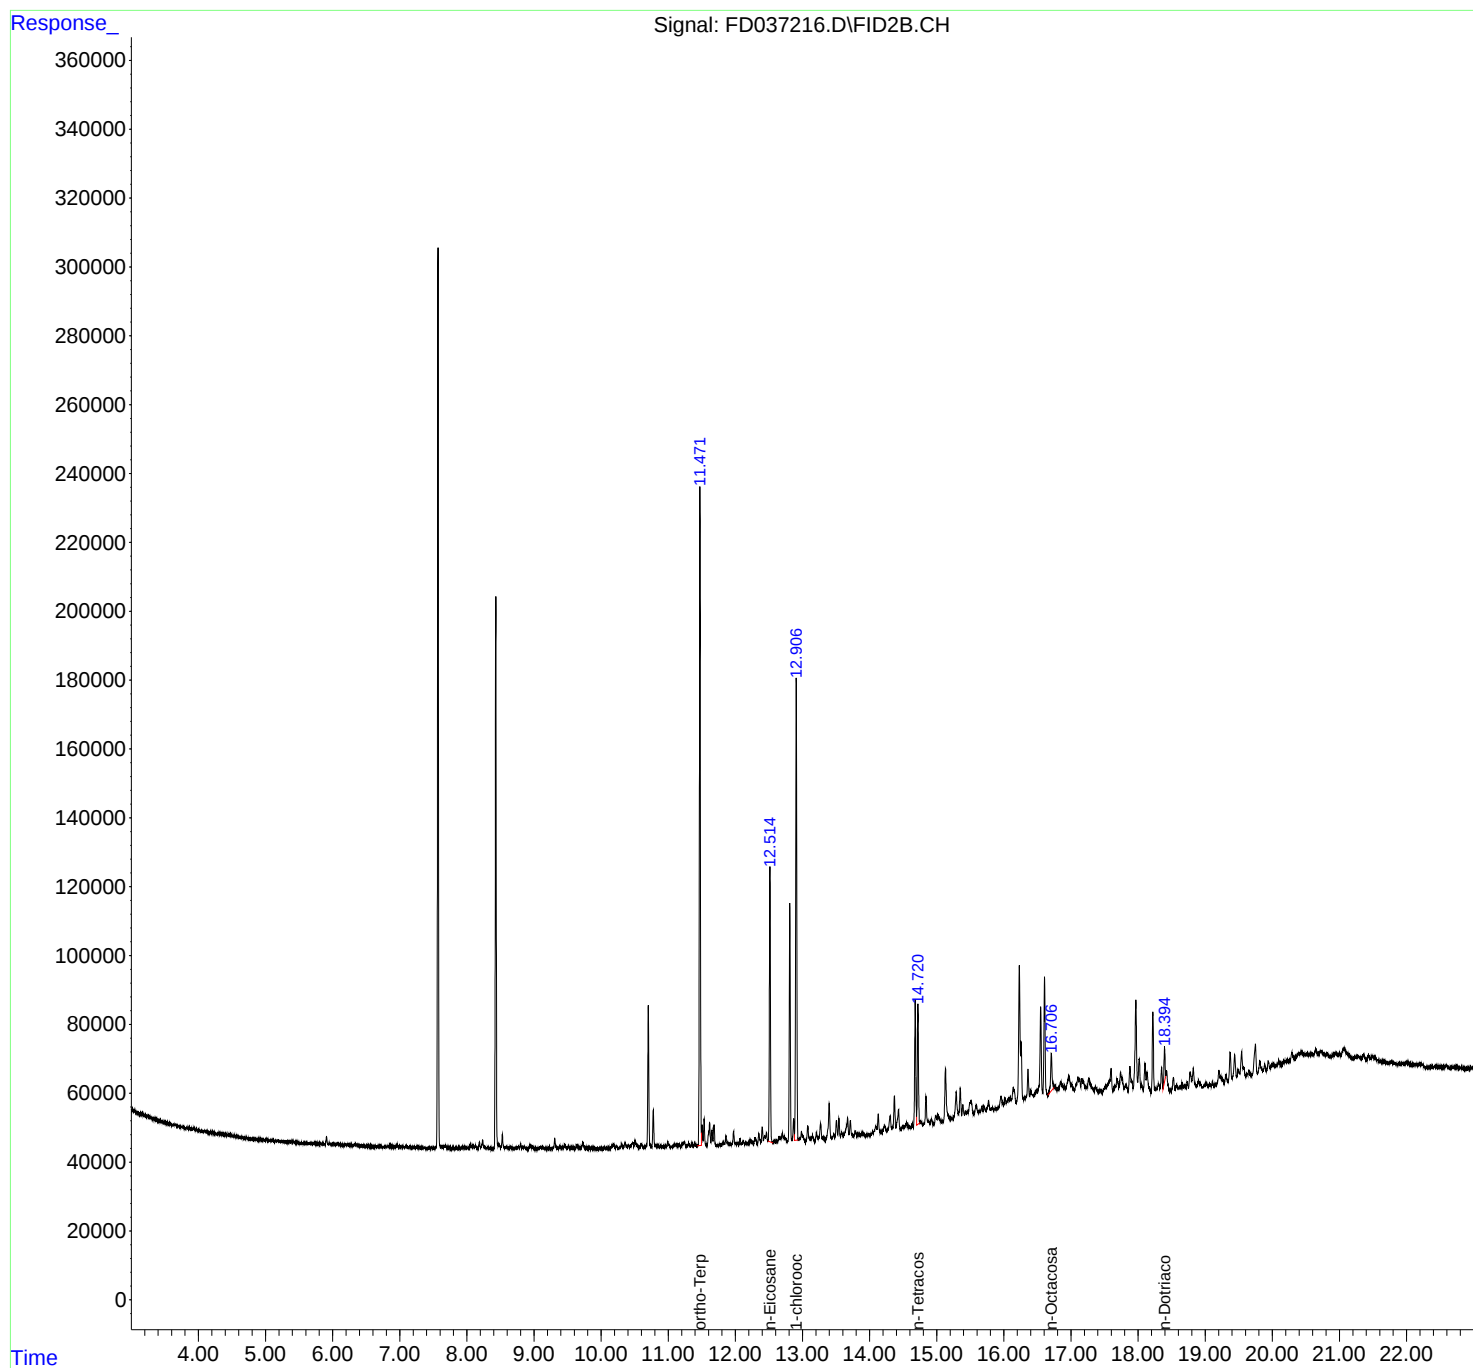


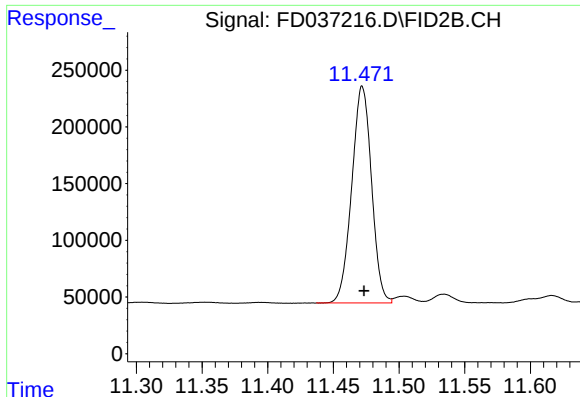

#9 ortho-Terphenyl (SURR)


R.T.: 11.472 min
Delta R.T.: -0.001 min
Response: 2001023
Conc: 17.14 ug/ml

Instrument :
FID_D
ClientSampleId :

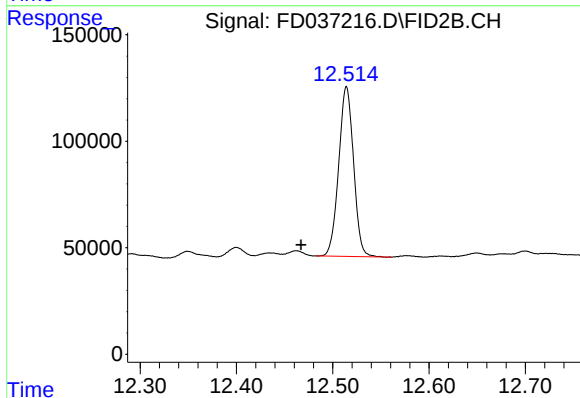


#10 n-Eicosane (C20)

R.T.: 12.514 min
Delta R.T.: 0.047 min
Response: 852339
Conc: 8.04 ug/ml

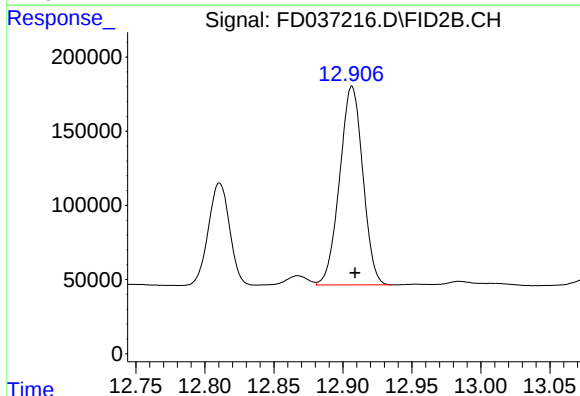


#12 1-chlorooctadecane (SURR)

R.T.: 12.907 min
Delta R.T.: -0.002 min
Response: 1566866
Conc: 18.52 ug/ml

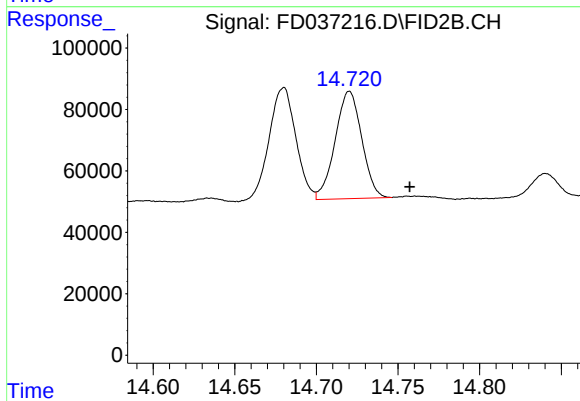

#14 n-Tetracosane (C24)


R.T.: 14.720 min
Delta R.T.: -0.037 min
Response: 396238
Conc: 3.91 ug/ml

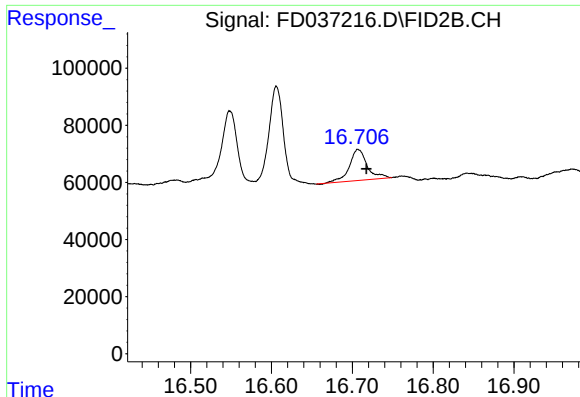

#16 n-Octacosane (C28)

R.T.: 16.707 min
Delta R.T.: -0.010 min
Response: 166800
Conc: 1.74 ug/ml

Instrument :
FID_D
ClientSampleId :

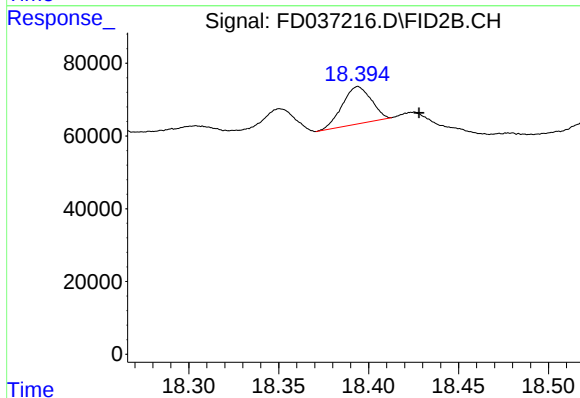

#18 n-Dotriacontane (C32)

R.T.: 18.394 min
Delta R.T.: -0.034 min
Response: 114838
Conc: 1.17 ug/ml