

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD050622AL\
 Data File : FD042347.D
 Signal(s) : FID2B.CH
 Acq On : 06 May 2022 15:59
 Operator : UA/NP
 Sample : N2691-05
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 SHALLOW-WC-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/09/2022
 Supervised By :mohammad ahmed 05/10/2022

Integration File: autoint1.e
 Quant Time: May 09 00:47:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 042122.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 22 01:55:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.213	3835130	22.868 ug/ml
Spiked Amount 50.000		Recovery =	45.74%
12) S 1-chlorooctadecane (S...	12.652	3064453	23.223 ug/mlm
Spiked Amount 50.000		Recovery =	46.45%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD050622AL\
Data File : FD042347.D
Signal(s) : FID2B.CH
Acq On : 06 May 2022 15:59
Operator : UA/NP
Sample : N2691-05
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
SHALLOW-WC-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/10/2022

Integration File: autoint1.e
Quant Time: May 09 00:47:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 042122.M
Quant Title : GC Extractables
QLast Update : Fri Apr 22 01:55:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

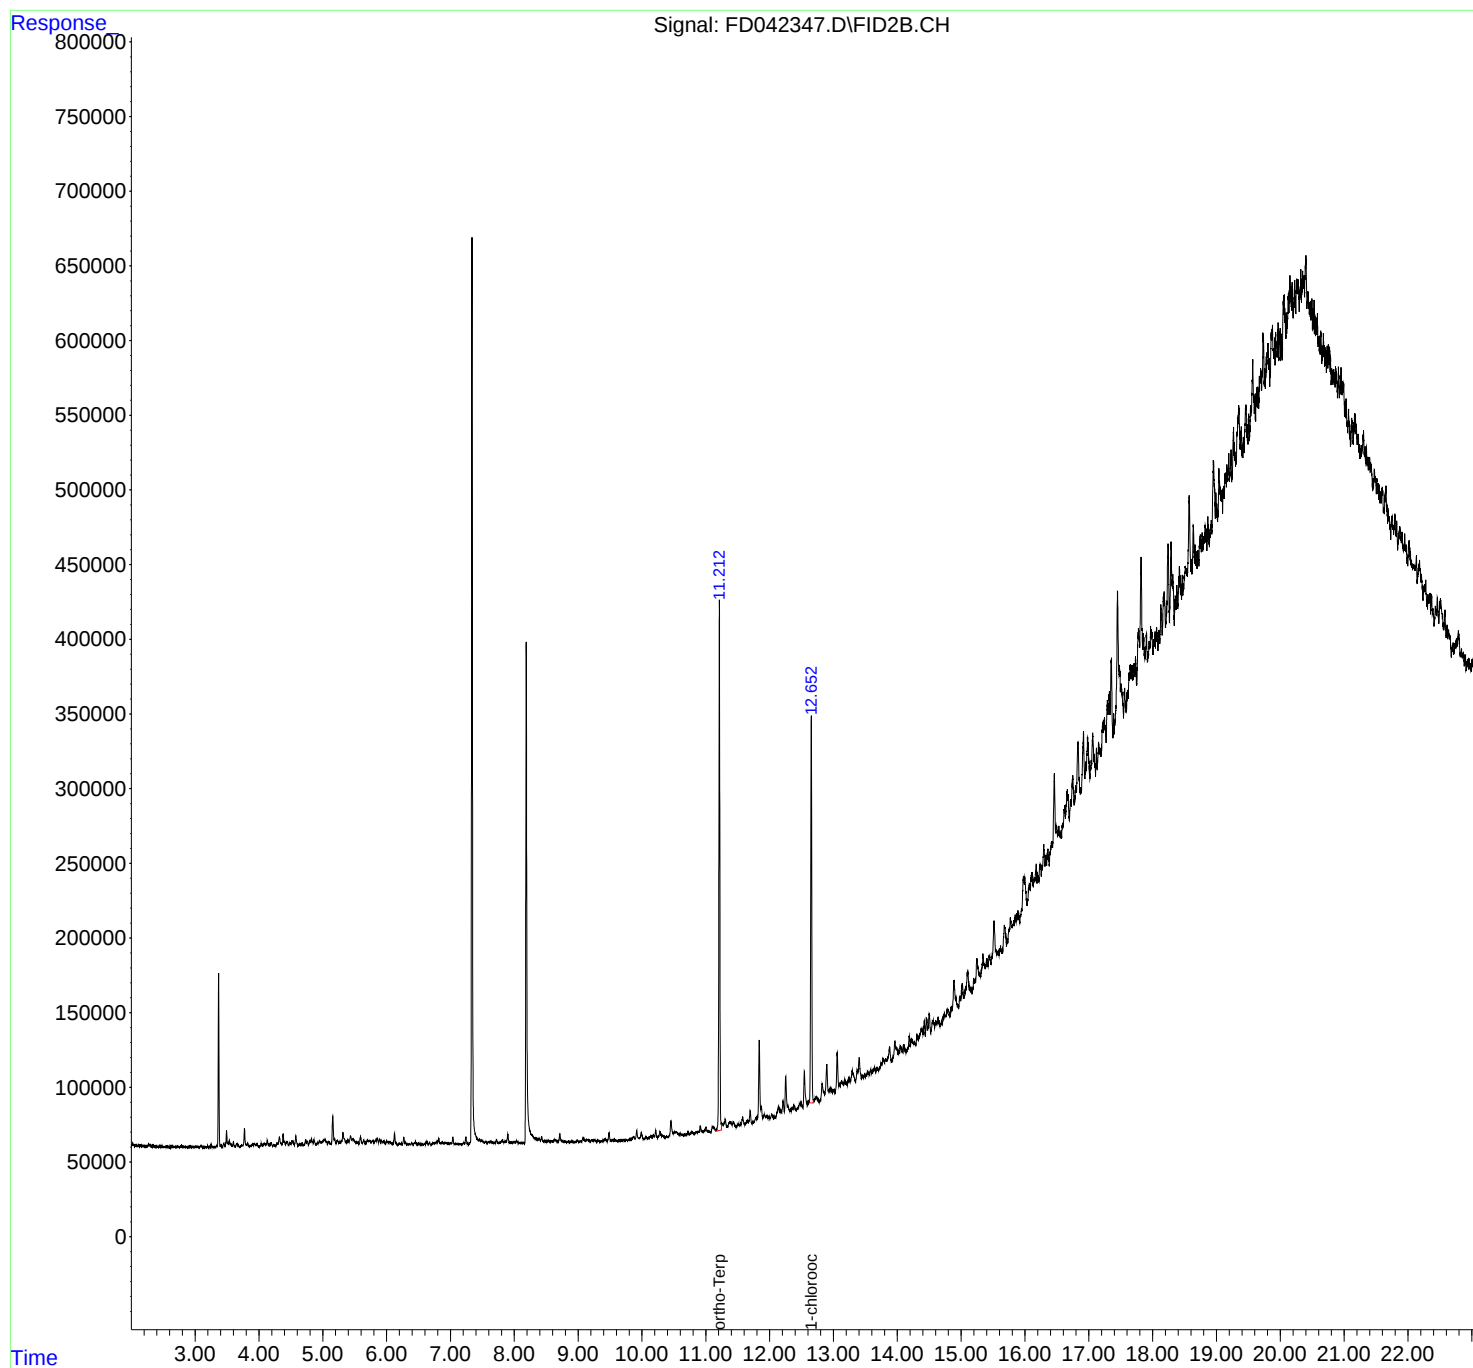

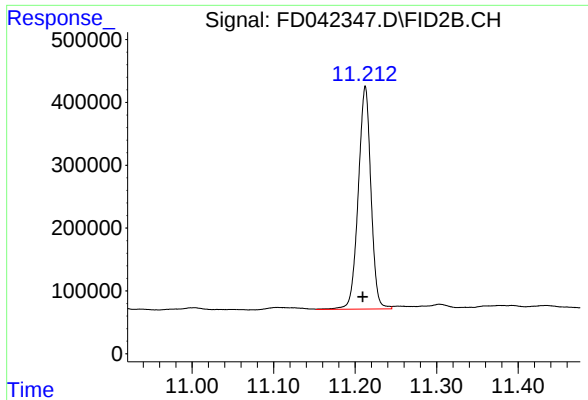


#9 ortho-Terphenyl (SURR)

R.T.: 11.213 min
Delta R.T.: 0.003 min
Response: 3835130
Conc: 22.87 ug/ml

Instrument :
FID_D
ClientSampleId :
SHALLOW-WC-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/10/2022

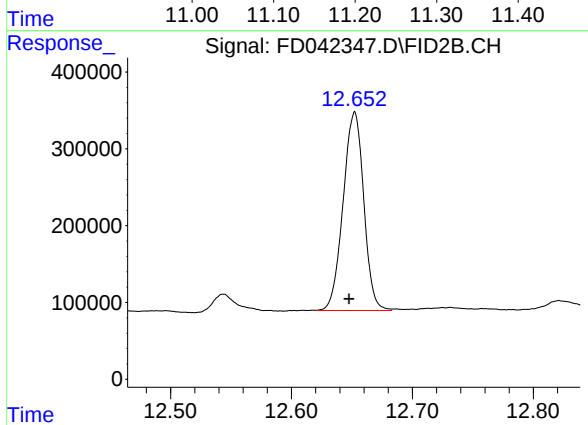

#12 1-chlorooctadecane (SURR)

R.T.: 12.652 min
Delta R.T.: 0.005 min
Response: 3064453
Conc: 23.22 ug/ml m