

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD051021AL\  
 Data File : FD037445.D  
 Signal(s) : FID2B.CH  
 Acq On : 10 May 2021 23:20  
 Operator : DD\AJ  
 Sample : PB136196BL  
 Misc : LOD-WATER-BL  
 ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e  
 Quant Time: May 11 04:27:02 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Alaphatic EPH 042121.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Apr 22 03:31:40 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 12.901 | 3676799    | 43.460 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 86.92%       |
| Target Compounds               |        |            |              |
| 4) T n-Dodecane (C12)          | 6.335  | 116907     | 0.984 ug/ml  |
| 17) T n-Tricontane (C30)       | 17.589 | 139258     | 1.448 ug/ml  |
| 18) T n-Dotriacontane (C32)    | 18.417 | 172197     | 1.751 ug/ml  |
| 19) T n-Tetratriacontane (C34) | 19.196 | 125966     | 1.327 ug/ml  |
| -----                          |        |            |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD051021AL\  
Data File : FD037445.D  
Signal(s) : FID2B.CH  
Acq On : 10 May 2021 23:20  
Operator : DD\AJ  
Sample : PB136196BL  
Misc : LOD-WATER-BL  
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 11 04:27:02 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Alaphatic EPH 042121.M  
Quant Title : GC Extractables  
QLast Update : Thu Apr 22 03:31:40 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

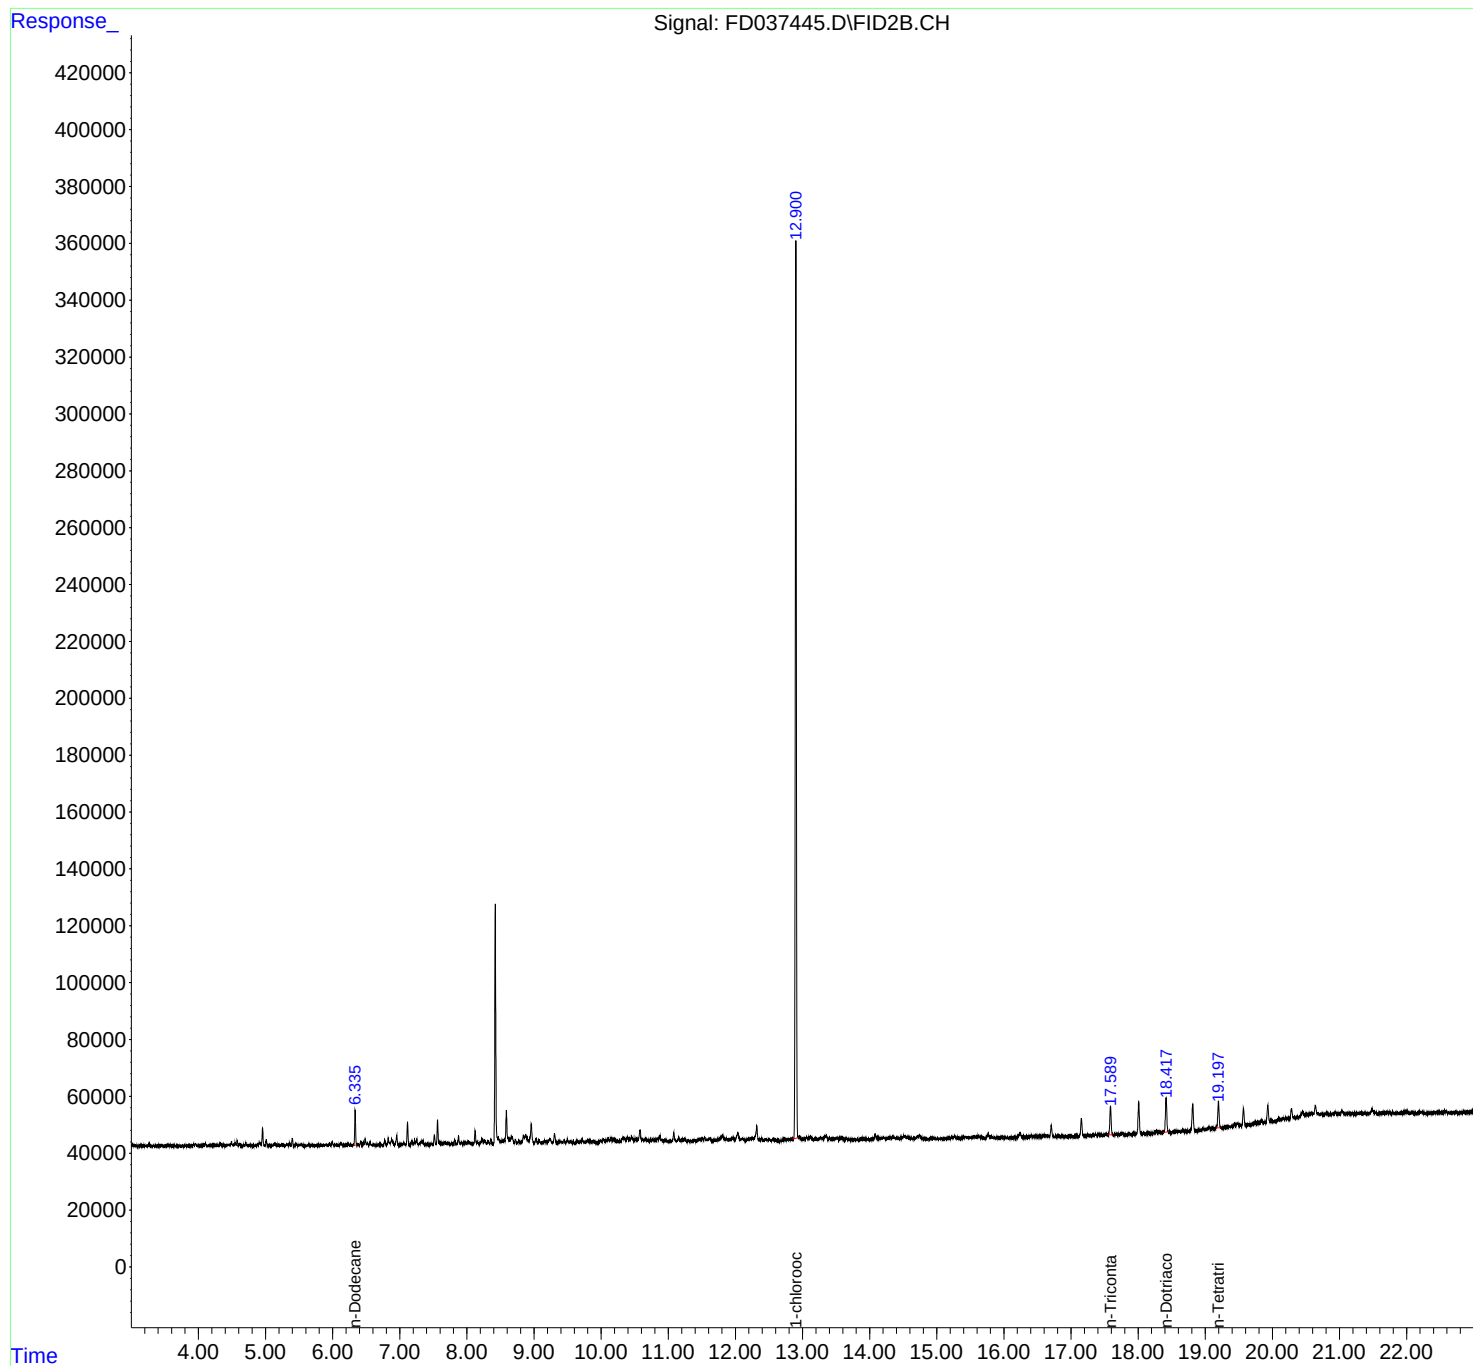

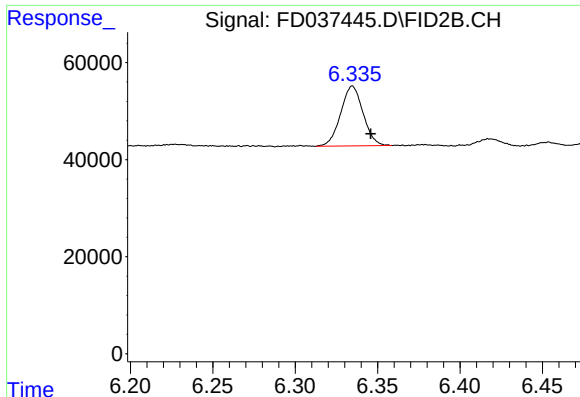


#4 n-Dodecane (C12)

R.T.: 6.335 min  
Delta R.T.: -0.011 min  
Response: 116907  
Conc: 0.98 ug/ml

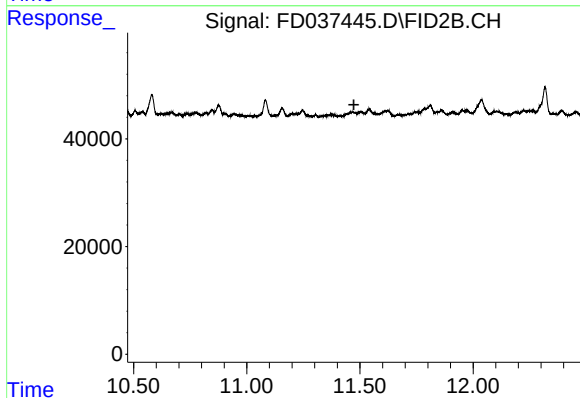


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T. : 11.473 min  
Response: 0  
Conc: N.D.

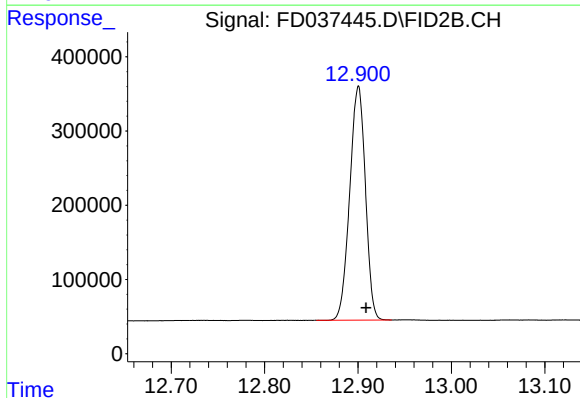


#12 1-chlorooctadecane (SURR)

R.T.: 12.901 min  
Delta R.T.: -0.008 min  
Response: 3676799  
Conc: 43.46 ug/ml

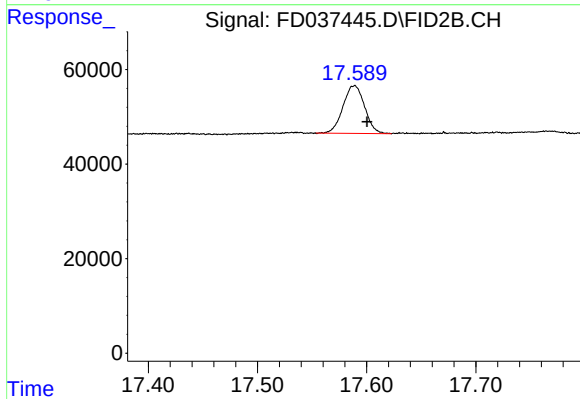


#17 n-Tricontane (C30)

R.T.: 17.589 min  
Delta R.T.: -0.011 min  
Response: 139258  
Conc: 1.45 ug/ml

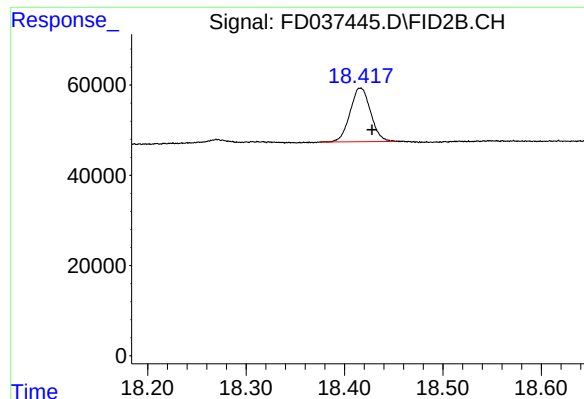

#18 n-Dotriacontane (C32)

R.T.: 18.417 min  
Delta R.T.: -0.011 min  
Response: 172197  
Conc: 1.75 ug/ml

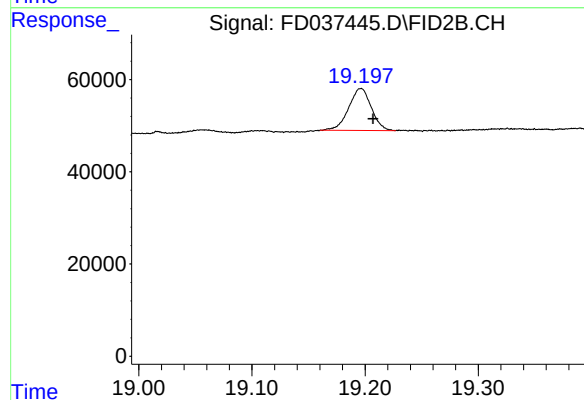

#19 n-Tetratriacontane (C34)

R.T.: 19.196 min  
Delta R.T.: -0.011 min  
Response: 125966  
Conc: 1.33 ug/ml