

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD051424AL\
Data File : FD047748.D
Signal(s) : FID2B.ch
Acq On : 14 May 2024 07:37
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 15 05:28:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 13:08:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.344	57493	0.338 ug/ml
19) T	n-Tetratriacontane (C34)	19.050	45707	0.283 ug/ml
20) T	n-Hexatriacontane (C36)	19.890f	75753	0.496 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD051424AL\
Data File : FD047748.D
Signal(s) : FID2B.ch
Acq On : 14 May 2024 07:37
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 15 05:28:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 13:08:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

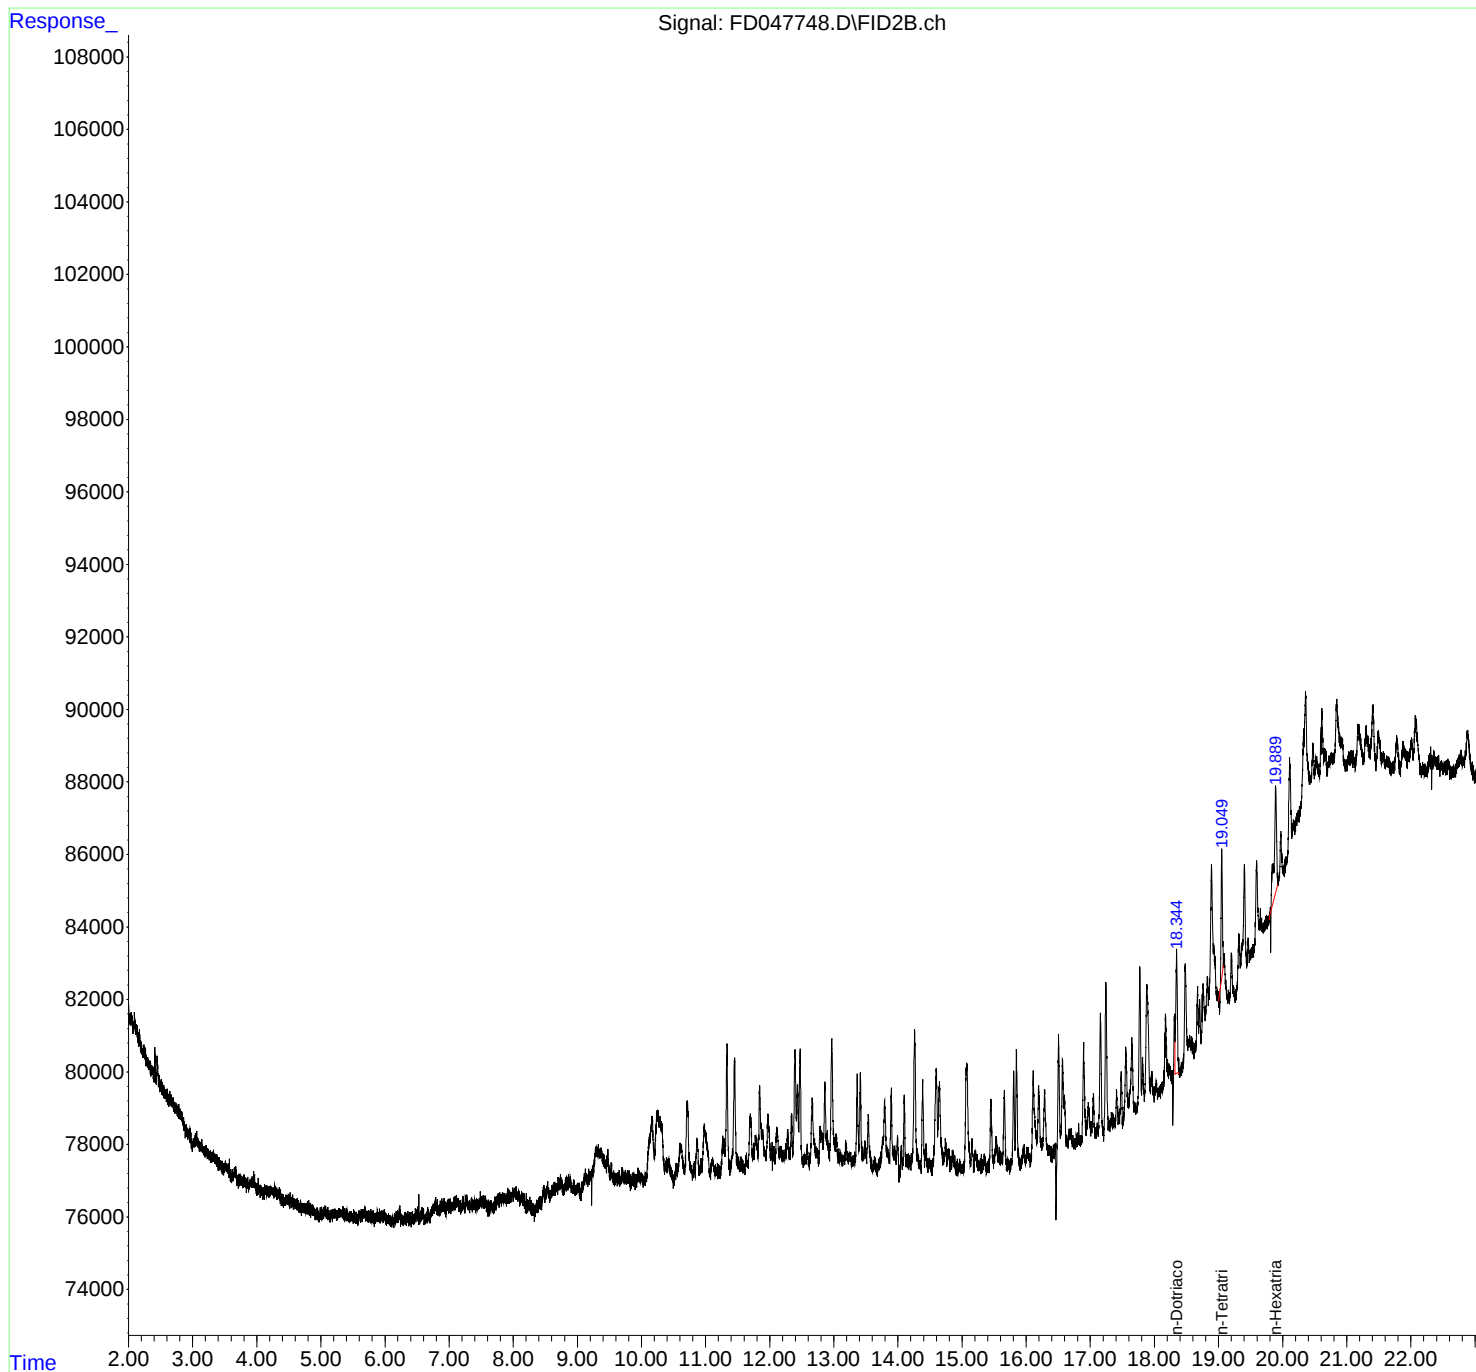


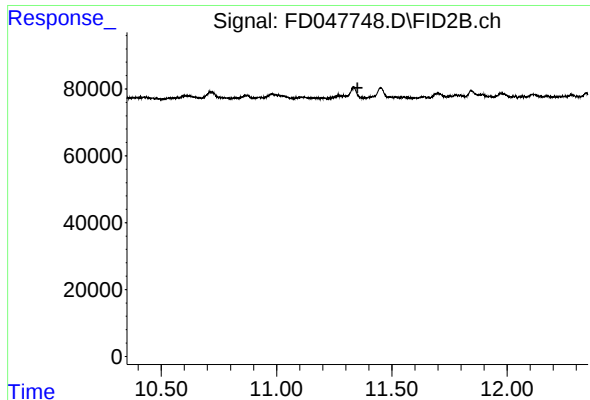

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.351 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

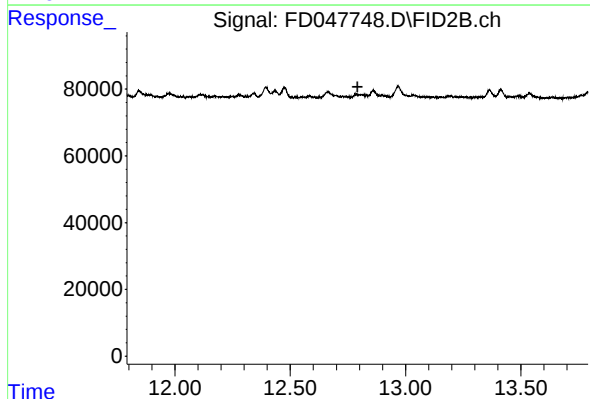


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.791 min
Response: 0
Conc: N.D.

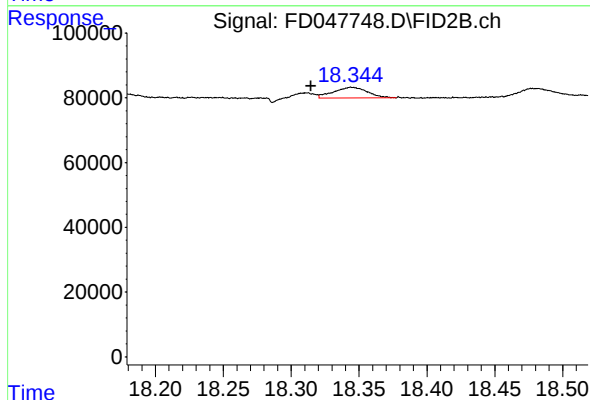


#18 n-Dotriacontane (C32)

R.T.: 18.344 min
Delta R.T.: 0.030 min
Response: 57493
Conc: 0.34 ug/ml

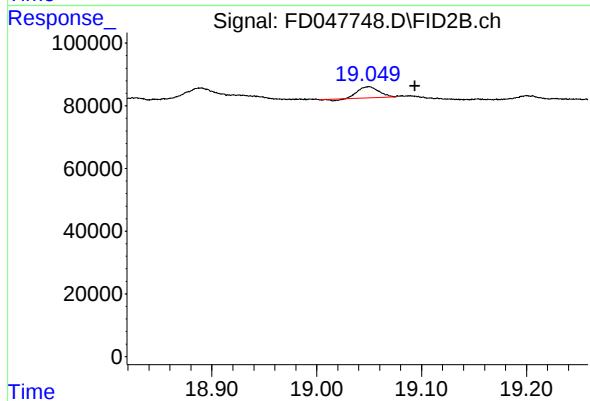

#19 n-Tetratriacontane (C34)

R.T.: 19.050 min
Delta R.T.: -0.044 min
Response: 45707
Conc: 0.28 ug/ml

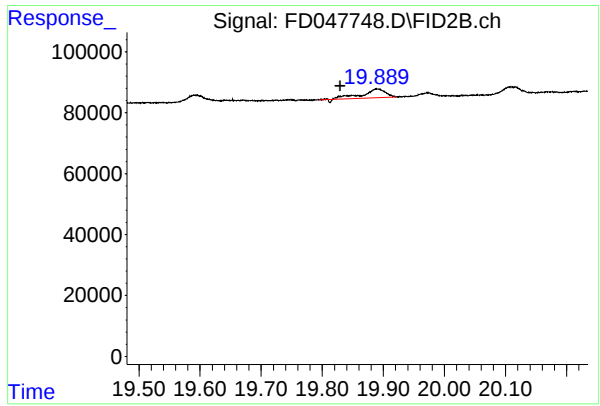

#20 n-Hexatriacontane (C36)

R.T.: 19.890 min
Delta R.T.: 0.061 min
Response: 75753
Conc: 0.50 ug/ml

Instrument :
FID_D
ClientSampleId :