

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051622\
 Data File : FB027219.D
 Signal(s) : FID2B.CH
 Acq On : 16 May 2022 23:39
 Operator : AJ/MA
 Sample : BSF0516S3
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 17 01:09:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	250421	23.856 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	467822	29.398 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	544263	33.734 ng/ml
3) t n-Heptane	7.753	139200	8.518 ng/ml
4) t Benzene	7.890	184172	9.932 ng/ml
6) t Toluene	10.623	541697	30.511 ng/ml
7) t Ethylbenzene	13.060	178067	10.783 ng/ml
8) t m-Xylene	13.192	354567	21.549 ng/ml
9) t O-Xylene	13.919	361462	22.037 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	379032	22.703 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051622\
Data File : FB027219.D
Signal(s) : FID2B.CH
Acq On : 16 May 2022 23:39
Operator : AJ/MA
Sample : BSF0516S3
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 17 01:09:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

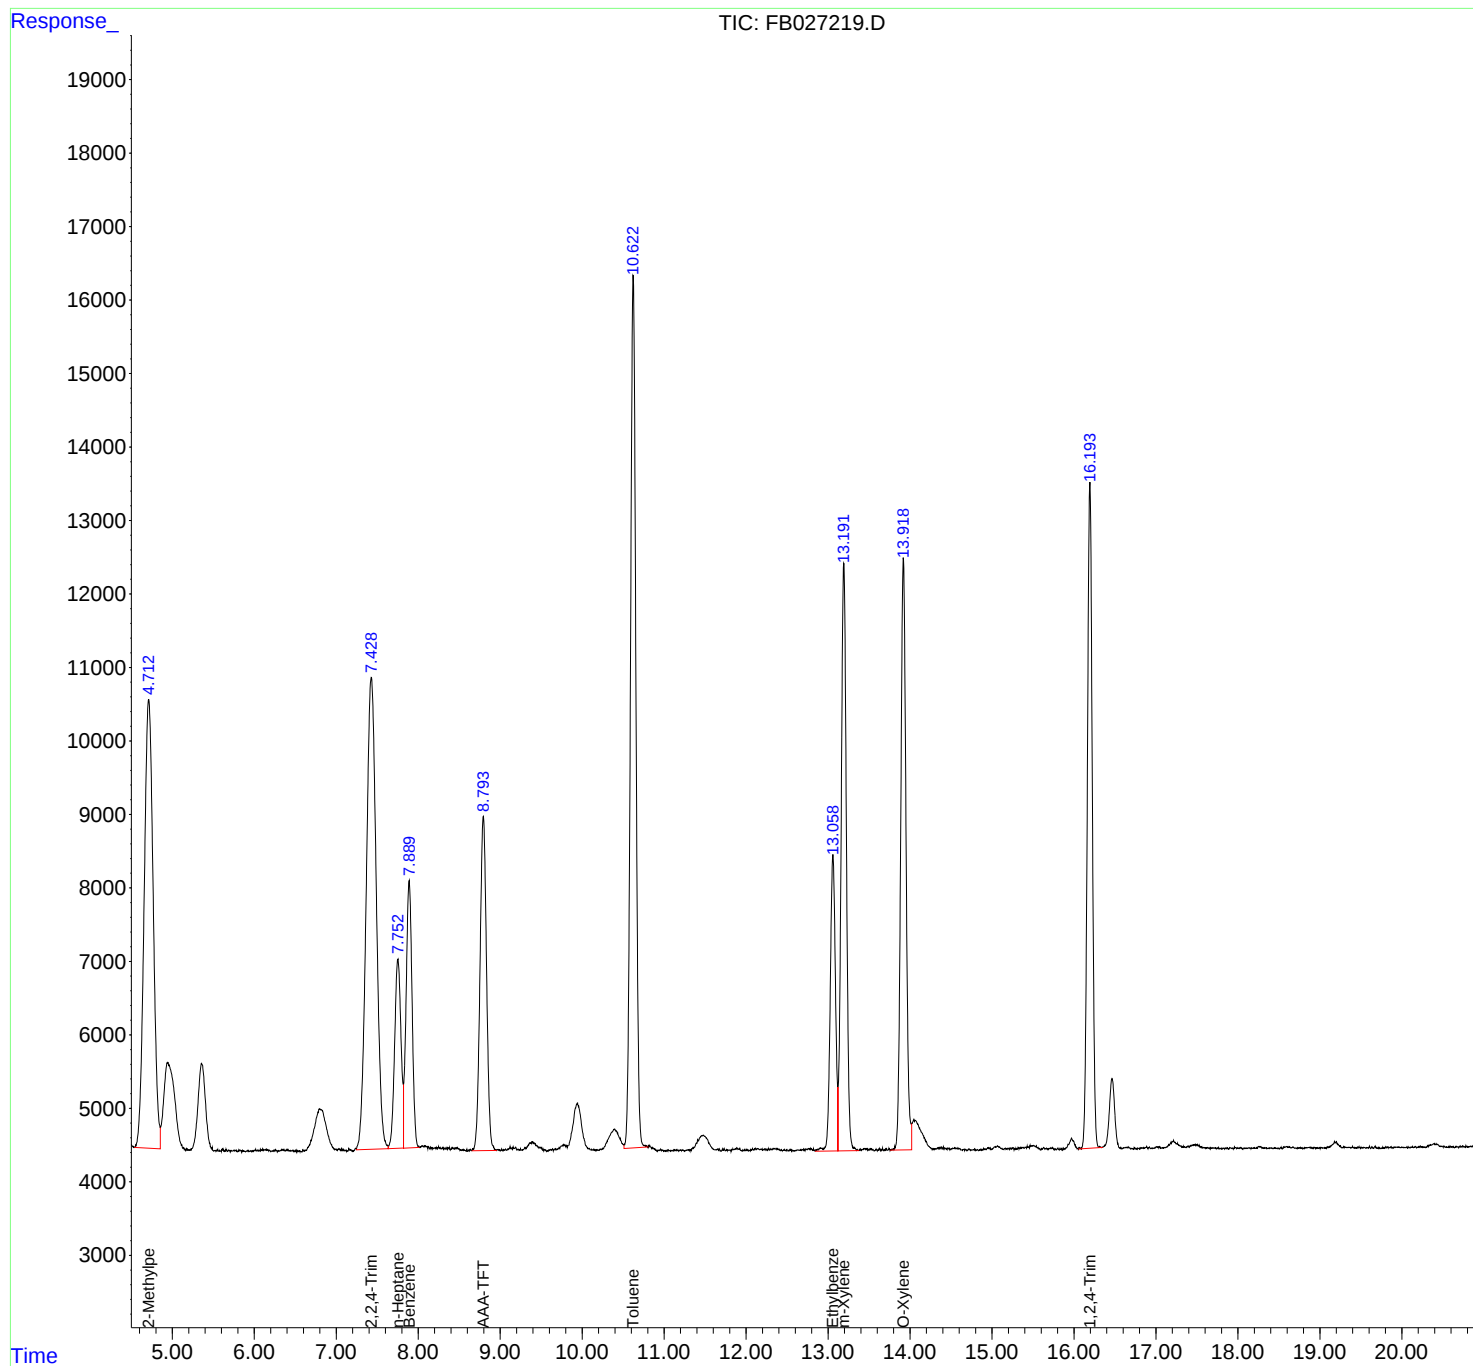


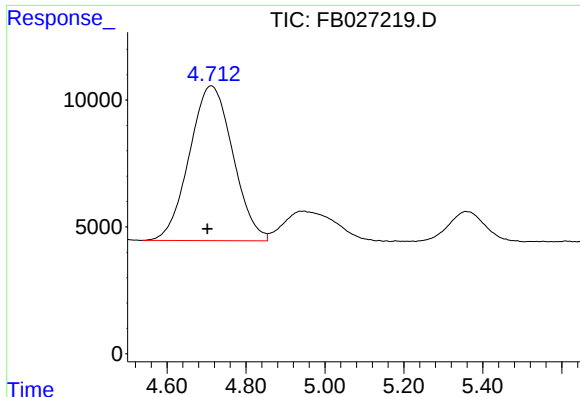

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.011 min
Response: 467822
Conc: 29.40 ng/ml

Instrument :
FID_D
ClientSampleId :

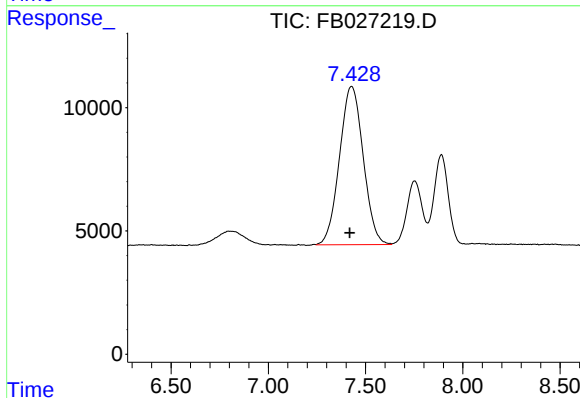


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.009 min
Response: 544263
Conc: 33.73 ng/ml

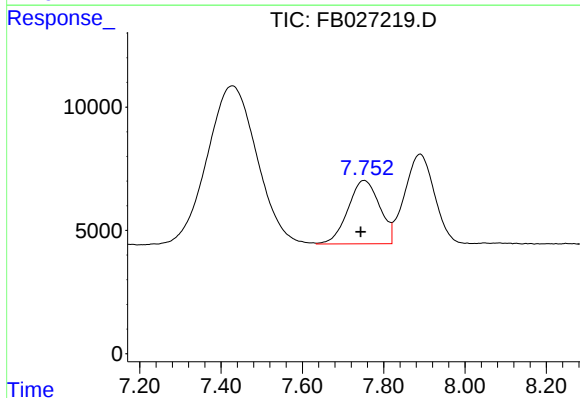


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.010 min
Response: 139200
Conc: 8.52 ng/ml

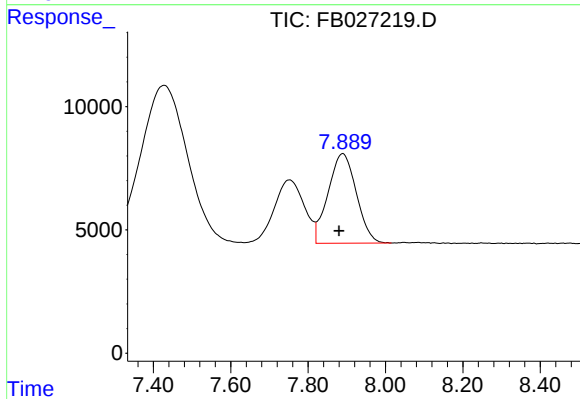

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.010 min
Response: 184172
Conc: 9.93 ng/ml

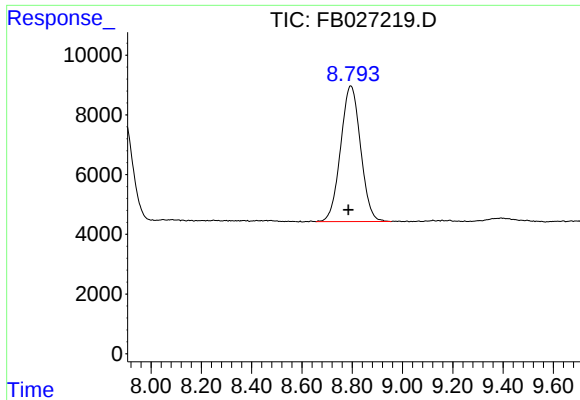

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.010 min
Response: 250421
Conc: 23.86 ng/ml

Instrument :
FID_D
ClientSampleId :

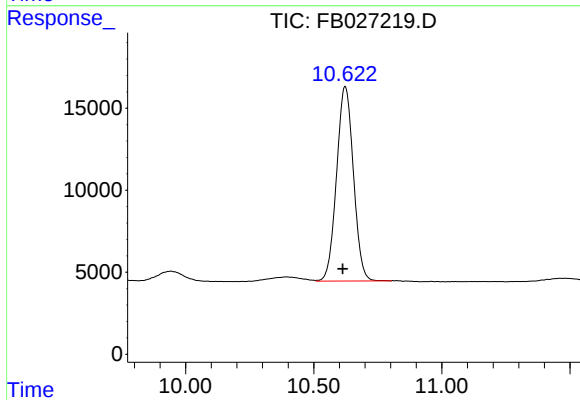


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.010 min
Response: 541697
Conc: 30.51 ng/ml

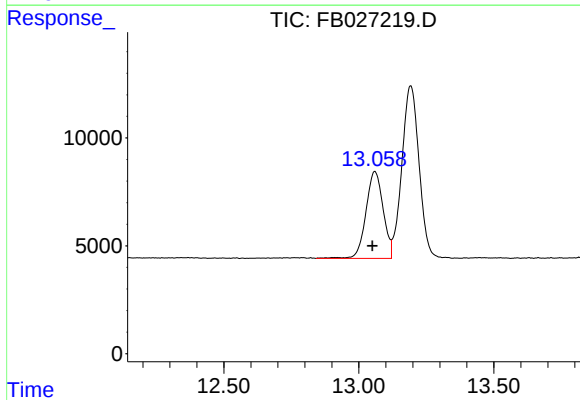


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.010 min
Response: 178067
Conc: 10.78 ng/ml

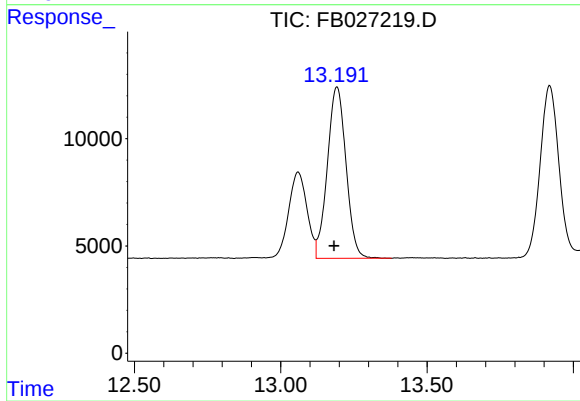

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.010 min
Response: 354567
Conc: 21.55 ng/ml

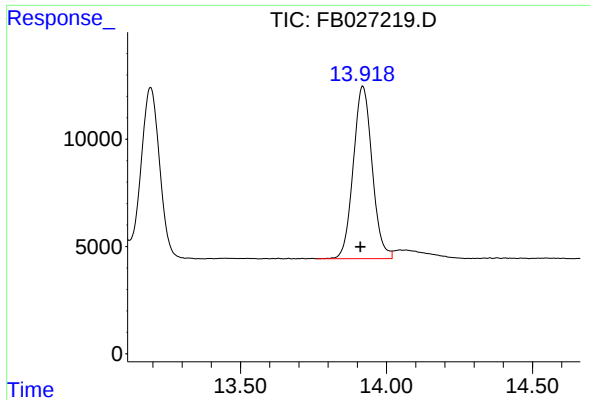

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.009 min
Response: 361462
Conc: 22.04 ng/ml

Instrument :
FID_D
ClientSampleId :

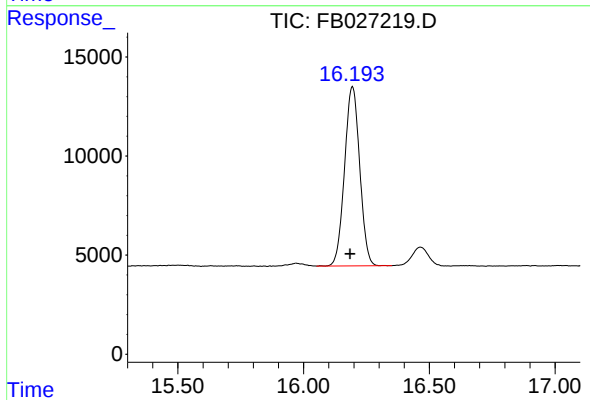

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.009 min
Response: 379032
Conc: 22.70 ng/ml