

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD051923AR\
 Data File : FD045699.D
 Signal(s) : FID2B.ch
 Acq On : 19 May 2023 22:41
 Operator : YP/AJ
 Sample : 02837-01MS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 WASTE-1MS

Integration File: autoint1.e
 Quant Time: May 20 00:36:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 050523.M
 Quant Title : GC Extractables
 QLast Update : Fri May 05 18:09:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T Benzo[a]anthracene (C...	14.678	130157	0.818 ug/ml
15) T Chrysene (C27.41)	14.678	130157	0.802 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD051923AR\
Data File : FD045699.D
Signal(s) : FID2B.ch
Acq On : 19 May 2023 22:41
Operator : YP/AJ
Sample : 02837-01MS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
WASTE-1MS

Integration File: autoint1.e
Quant Time: May 20 00:36:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 050523.M
Quant Title : GC Extractables
QLast Update : Fri May 05 18:09:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

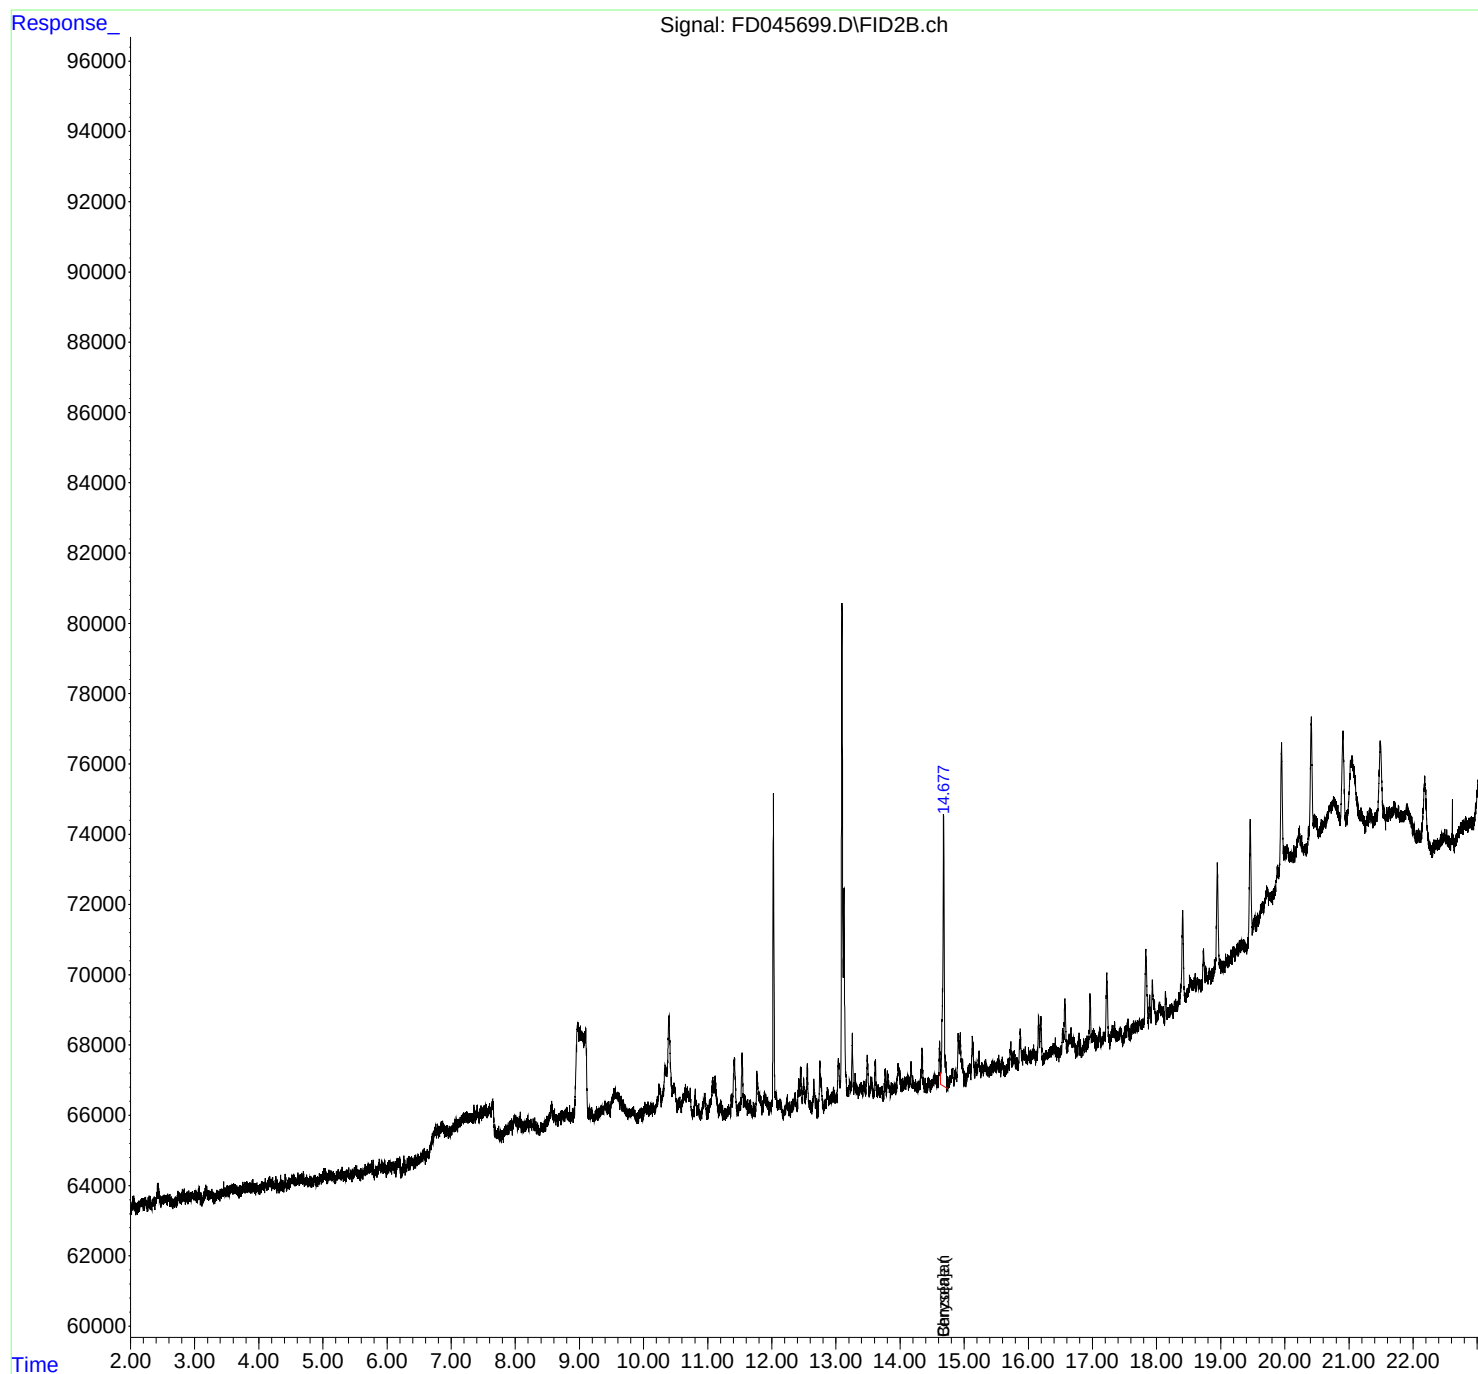


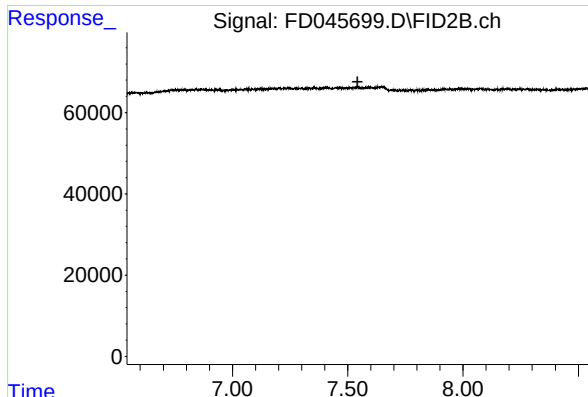

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.542 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
WASTE-1MS

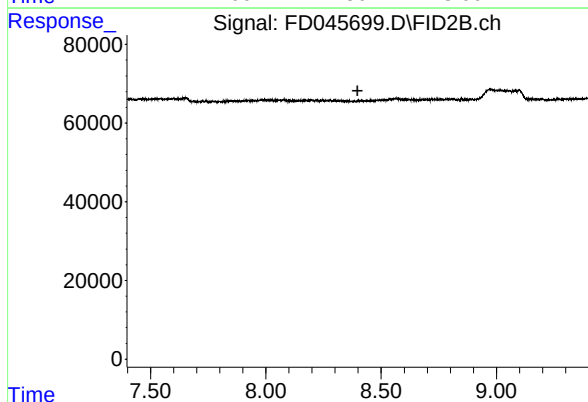


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.397 min
Response: 0
Conc: N.D.

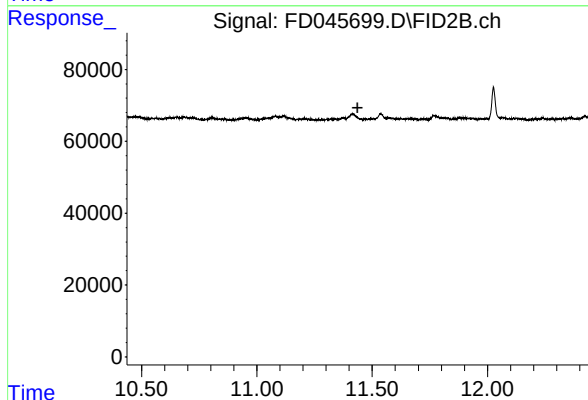


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.436 min
Response: 0
Conc: N.D.

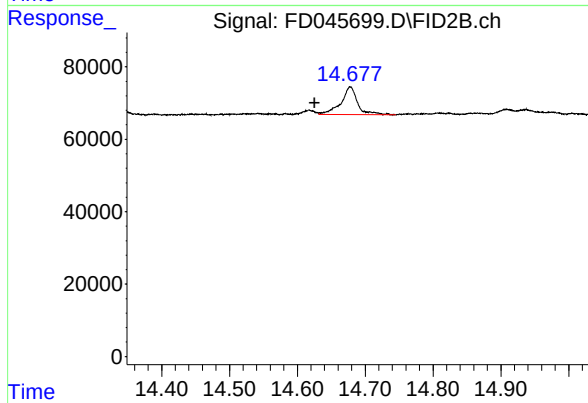

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.678 min
Delta R.T.: 0.053 min
Response: 130157
Conc: 0.82 ug/ml

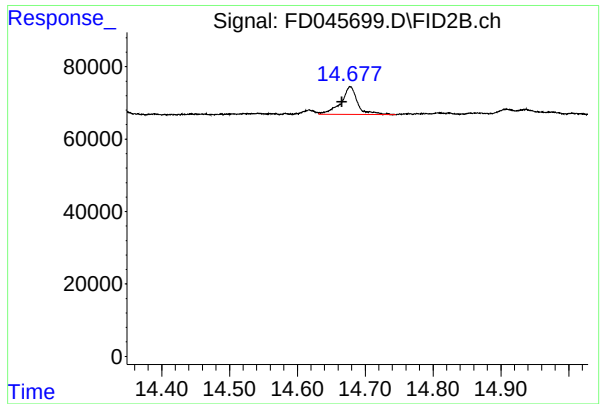

#15 Chrysene (C27.41)

R.T.: 14.678 min
Delta R.T.: 0.012 min
Response: 130157
Conc: 0.80 ug/ml

Instrument :
FID_D
ClientSampleId :
WASTE-1MS