

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD052025AR\
Data File : FD049362.D
Signal(s) : FID2B.ch
Acq On : 20 May 2025 23:51
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 21 03:17:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 050125.M
Quant Title : GC Extractables
QLast Update : Thu May 01 13:29:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	18.195	111112	1.012 ug/ml
20) T	Dibenz[a,h]anthracene...	18.195	111112	1.052 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD052025AR\
Data File : FD049362.D
Signal(s) : FID2B.ch
Acq On : 20 May 2025 23:51
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 21 03:17:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 050125.M
Quant Title : GC Extractables
QLast Update : Thu May 01 13:29:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

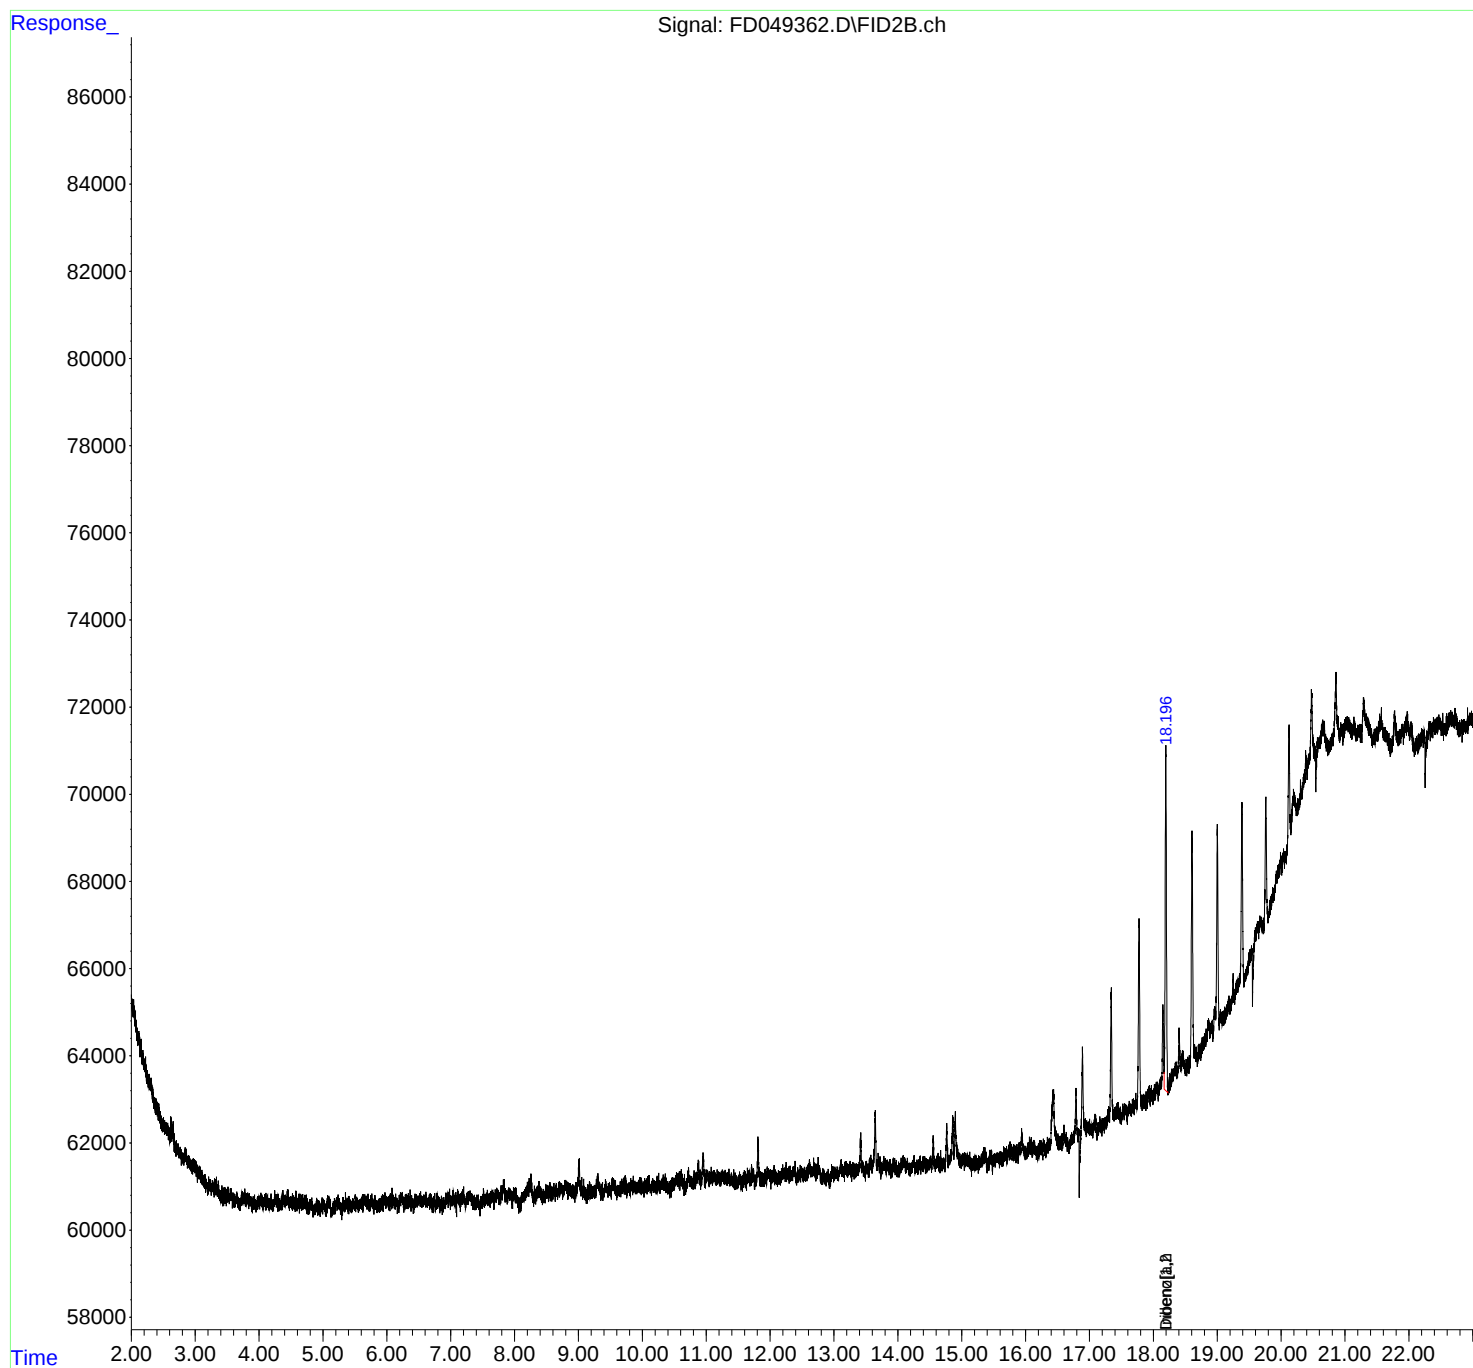


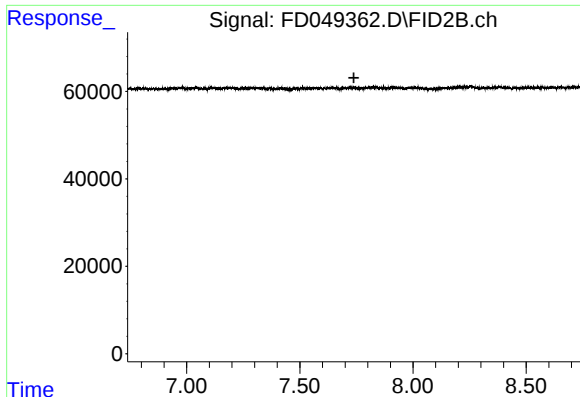

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.739 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
I.BLK

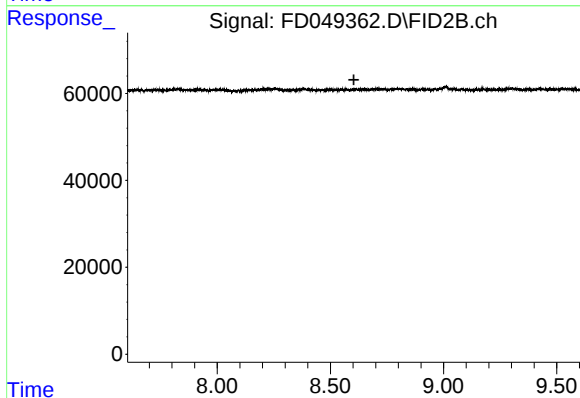


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.604 min
Response: 0
Conc: N.D.

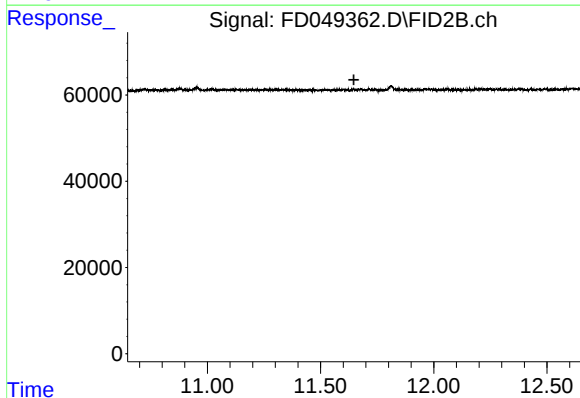


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.647 min
Response: 0
Conc: N.D.

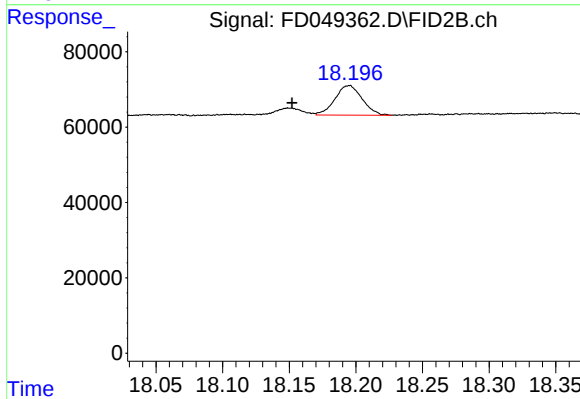

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.195 min
Delta R.T.: 0.043 min
Response: 111112
Conc: 1.01 ug/ml

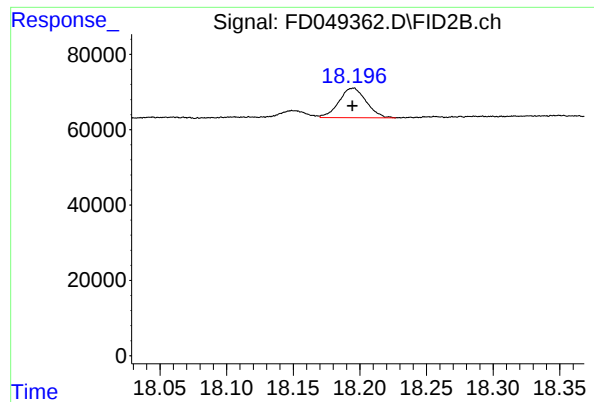

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.195 min
Delta R.T.: 0.000 min
Response: 111112
Conc: 1.05 ug/ml

Instrument :
FID_D
ClientSampleId :
I.BLK