

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD052222AL\
 Data File : FD042602.D
 Signal(s) : FID2B.CH
 Acq On : 21 May 2022 13:04
 Operator : UA/NP
 Sample : N2960-01DL 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 BIN-4-SP-1DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/23/2022
 Supervised By :Ankita Jodhani 05/23/2022

Integration File: autoint1.e
 Quant Time: May 23 01:27:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 051922.M
 Quant Title : GC Extractables
 QLast Update : Thu May 19 05:18:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.203	2720025	16.232 ug/ml
Spiked Amount	50.000	Recovery	= 32.46%
12) S 1-chlorooctadecane (S...	12.642	1992419	15.452 ug/mlm
Spiked Amount	50.000	Recovery	= 30.90%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD052222AL\
Data File : FD042602.D
Signal(s) : FID2B.CH
Acq On : 21 May 2022 13:04
Operator : UA/NP
Sample : N2960-01DL 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
BIN-4-SP-1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

Integration File: autoint1.e
Quant Time: May 23 01:27:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 051922.M
Quant Title : GC Extractables
QLast Update : Thu May 19 05:18:51 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

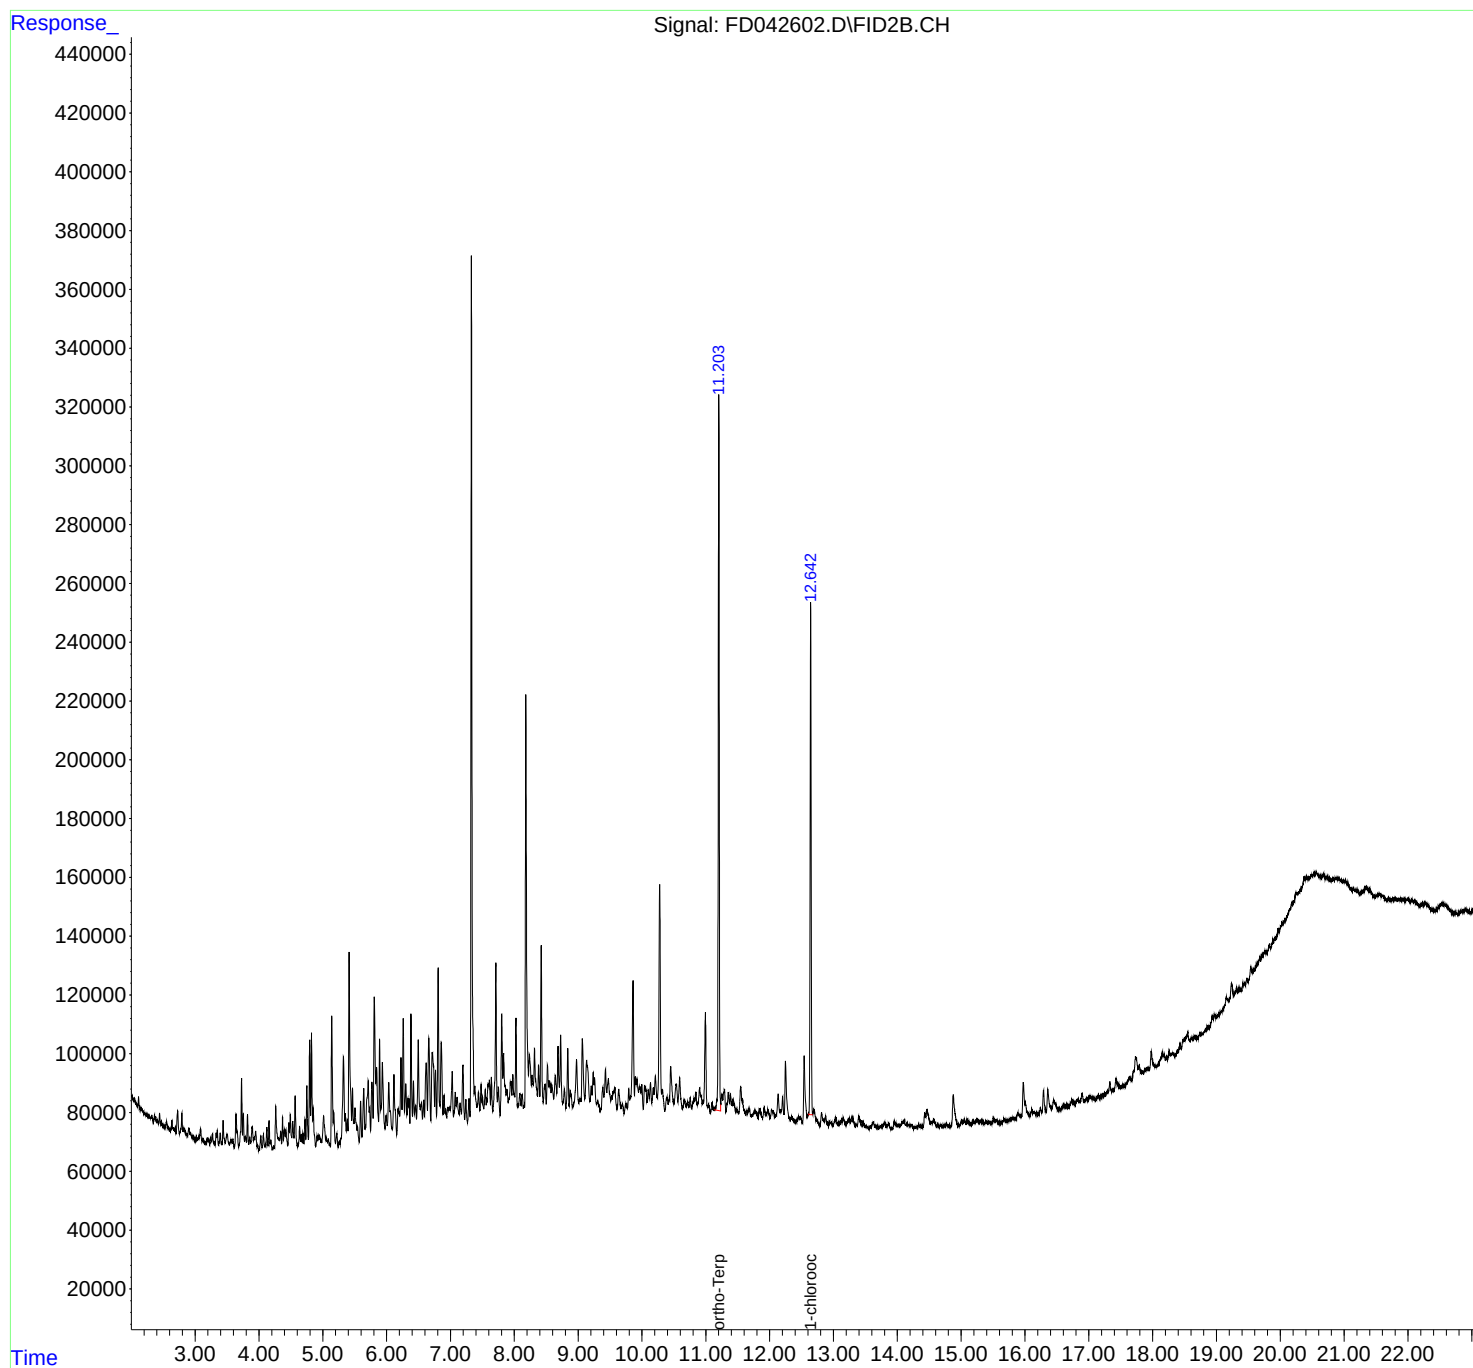

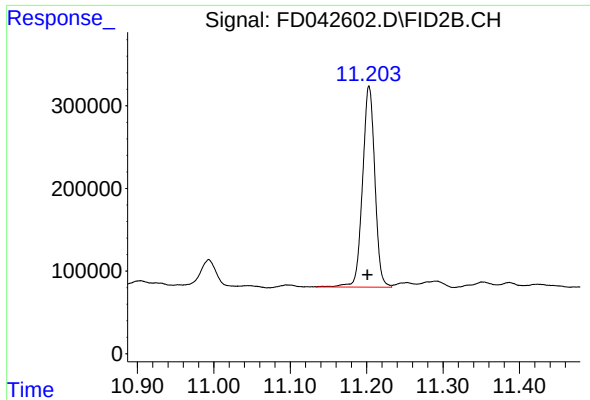


#9 ortho-Terphenyl (SURR)

R.T.: 11.203 min
Delta R.T.: 0.002 min
Response: 2720025
Conc: 16.23 ug/ml

Instrument :
FID_D
ClientSampleId :
BIN-4-SP-1DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

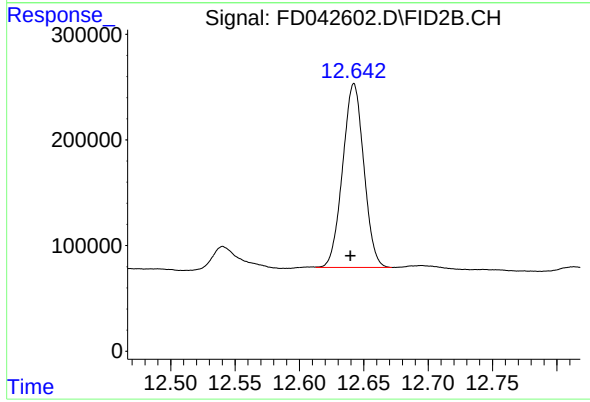

#12 1-chlorooctadecane (SURR)

R.T.: 12.642 min
Delta R.T.: 0.002 min
Response: 1992419
Conc: 15.45 ug/ml m