

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD052822AL\
Data File : FD042680.D
Signal(s) : FID2B.CH
Acq On : 28 May 2022 22:50
Operator : UA/NP
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 30 00:59:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 07:55:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.717	66896	0.512 ug/ml
18) T	n-Dotriacontane (C32)	18.547	83820	0.710 ug/ml
19) T	n-Tetratriacontane (C34)	19.332	75321	0.709 ug/ml
20) T	n-Hexatriacontane (C36)	20.072	199853	2.044 ug/ml
21) T	n-Octatriacontane (C38)	20.813	282336	3.095 ug/ml
22) T	n-Tetracontane (C40)	21.735	789853	9.747 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD052822AL\
Data File : FD042680.D
Signal(s) : FID2B.CH
Acq On : 28 May 2022 22:50
Operator : UA/NP
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 30 00:59:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 07:55:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

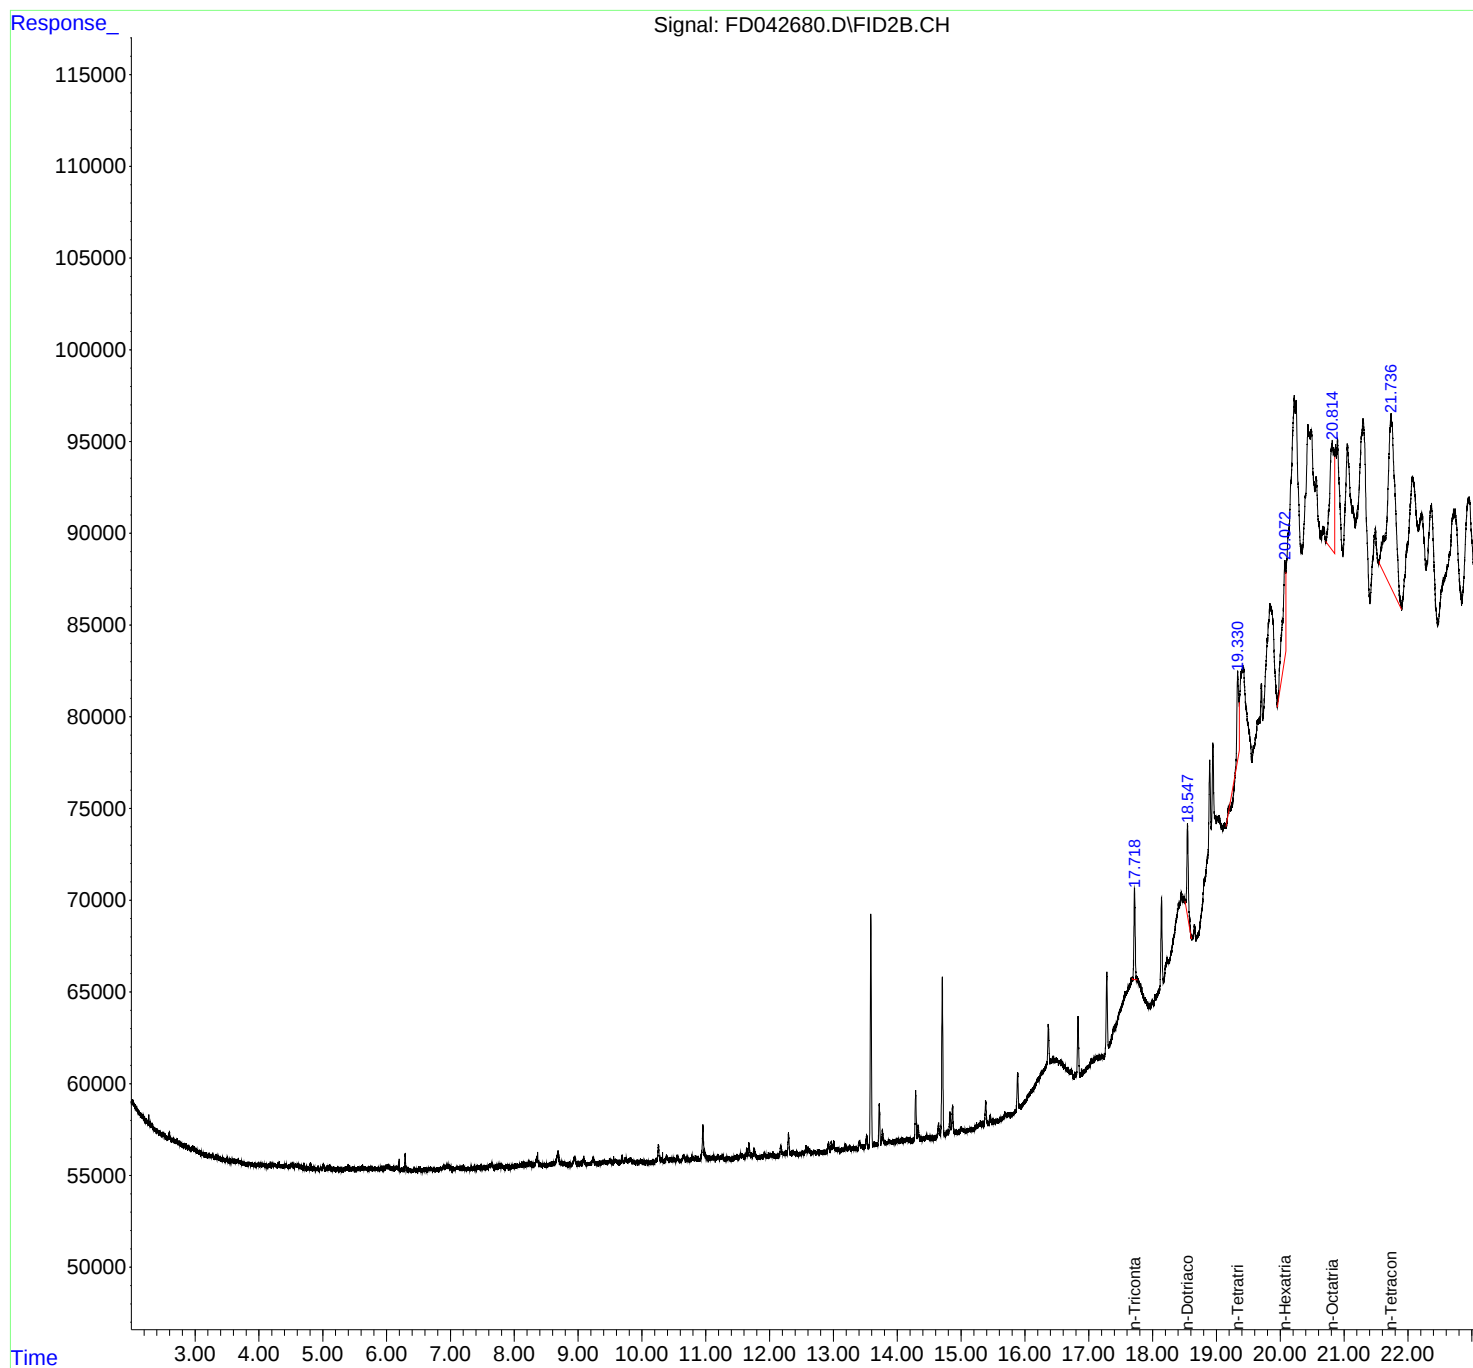


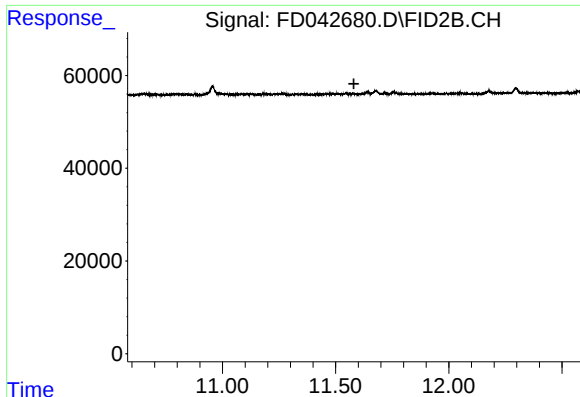

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.581 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

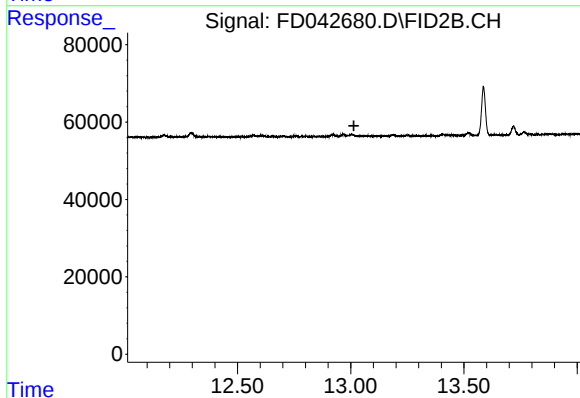


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.014 min
Response: 0
Conc: N.D.

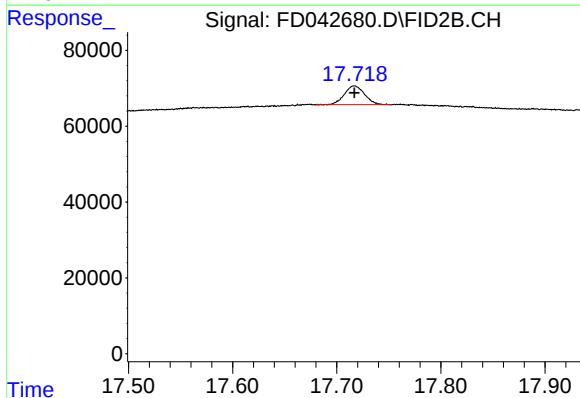


#17 n-Tricontane (C30)

R.T.: 17.717 min
Delta R.T.: 0.000 min
Response: 66896
Conc: 0.51 ug/ml

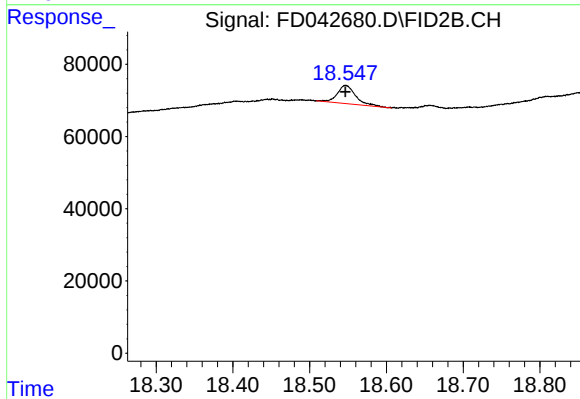

#18 n-Dotriacontane (C32)


R.T.: 18.547 min
Delta R.T.: 0.000 min
Response: 83820
Conc: 0.71 ug/ml

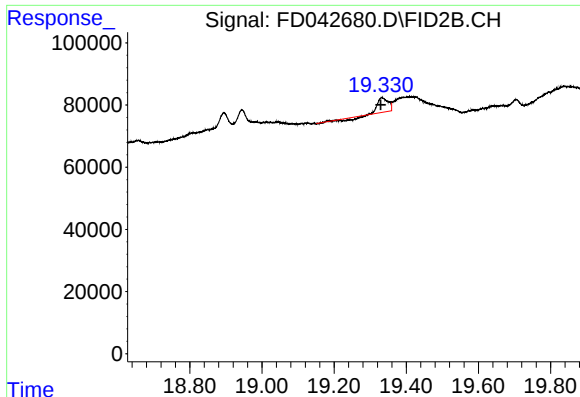

#19 n-Tetratriacontane (C34)


R.T.: 19.332 min
Delta R.T.: 0.003 min
Response: 75321
Conc: 0.71 ug/ml

Instrument :
FID_D
ClientSampleId :

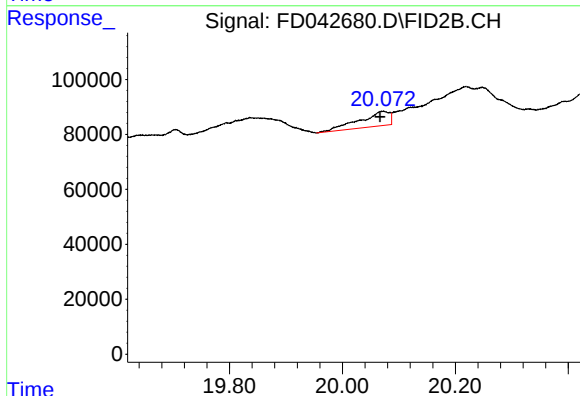


#20 n-Hexatriacontane (C36)

R.T.: 20.072 min
Delta R.T.: 0.006 min
Response: 199853
Conc: 2.04 ug/ml

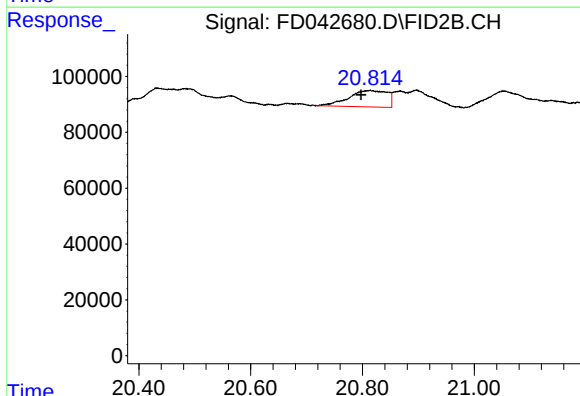

#21 n-Octatriacontane (C38)

R.T.: 20.813 min
Delta R.T.: 0.016 min
Response: 282336
Conc: 3.10 ug/ml

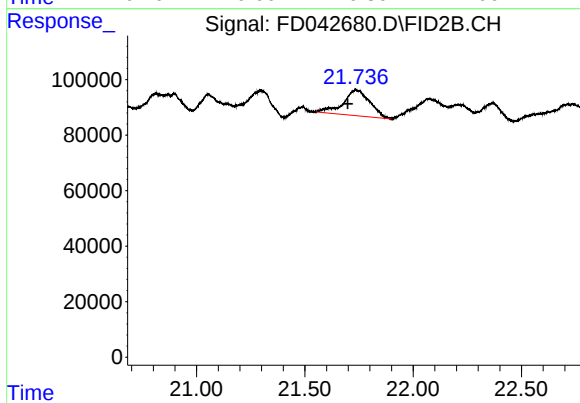

#22 n-Tetracontane (C40)

R.T.: 21.735 min
Delta R.T.: 0.037 min
Response: 789853
Conc: 9.75 ug/ml