

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060221AL\
 Data File : FD037653.D
 Signal(s) : FID2B.CH
 Acq On : 02 Jun 2021 18:37
 Operator : DD\AJ
 Sample : M2575-07
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 03 03:26:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 02:07:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.458	4022079	34.298 ug/ml
Spiked Amount 50.000		Recovery =	68.60%
12) S 1-chlorooctadecane (S...	12.893	3086450	33.967 ug/ml
Spiked Amount 50.000		Recovery =	67.93%
Target Compounds			
10) T n-Eicosane (C20)	12.501f	158303	1.453 ug/ml
14) T n-Tetracosane (C24)	14.708	88522	0.817 ug/ml
16) T n-Octacosane (C28)	16.746	422692	3.990 ug/ml
17) T n-Tricontane (C30)	17.595	153052	1.454 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060221AL\
Data File : FD037653.D
Signal(s) : FID2B.CH
Acq On : 02 Jun 2021 18:37
Operator : DD\AJ
Sample : M2575-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 03 03:26:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 02:07:09 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

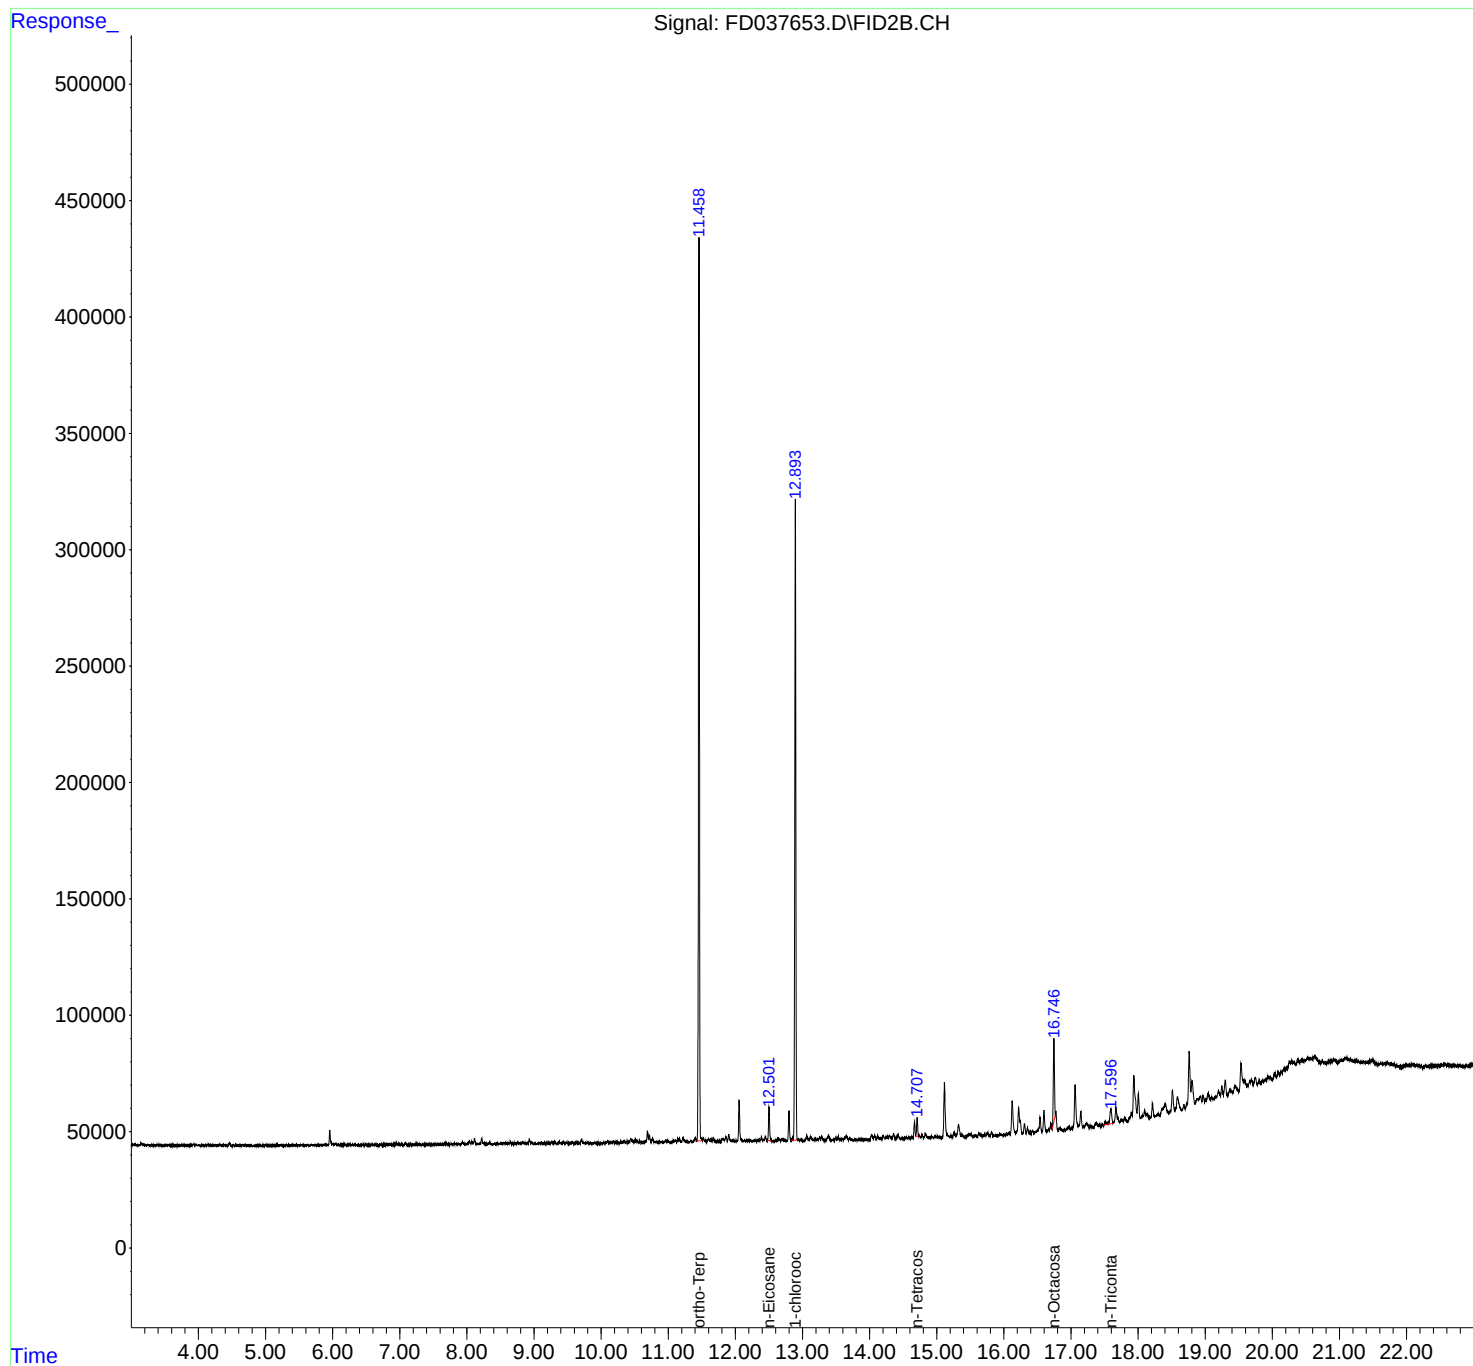


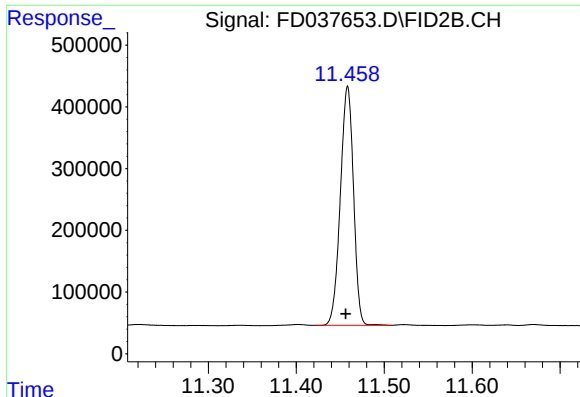

#9 ortho-Terphenyl (SURR)


R.T.: 11.458 min
Delta R.T.: 0.002 min
Response: 4022079
Conc: 34.30 ug/ml

Instrument :
FID_D
ClientSampleId :

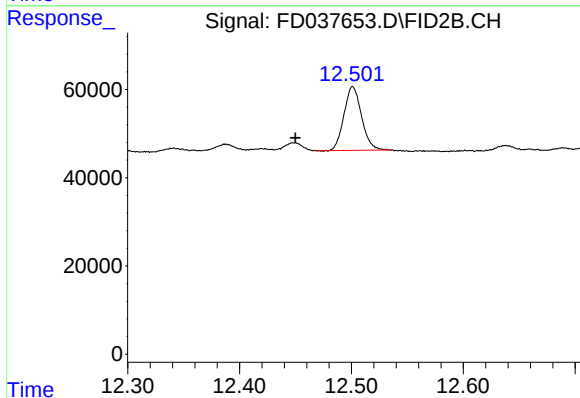


#10 n-Eicosane (C20)

R.T.: 12.501 min
Delta R.T.: 0.051 min
Response: 158303
Conc: 1.45 ug/ml

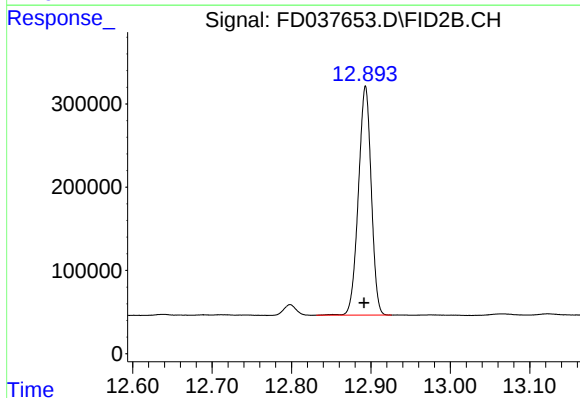


#12 1-chlorooctadecane (SURR)

R.T.: 12.893 min
Delta R.T.: 0.002 min
Response: 3086450
Conc: 33.97 ug/ml

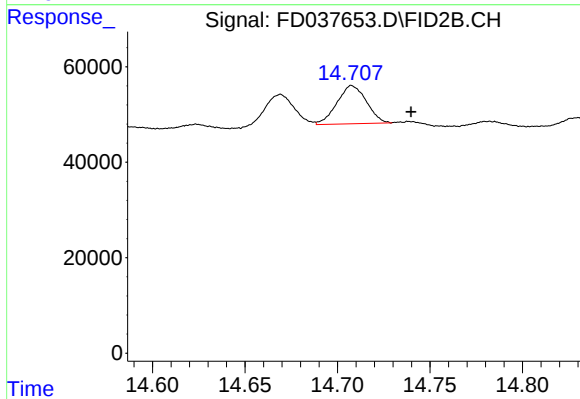

#14 n-Tetracosane (C24)


R.T.: 14.708 min
Delta R.T.: -0.032 min
Response: 88522
Conc: 0.82 ug/ml

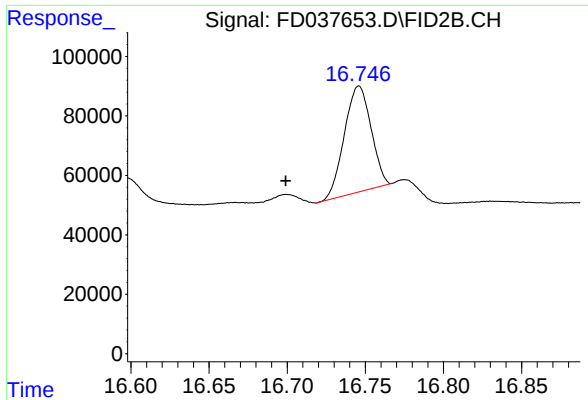

#16 n-Octacosane (C28)

R.T.: 16.746 min
Delta R.T.: 0.047 min
Response: 422692
Conc: 3.99 ug/ml

Instrument :
FID_D
ClientSampleId :

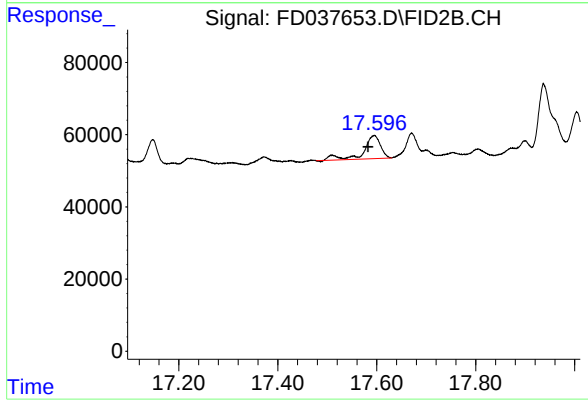

#17 n-Tricontane (C30)

R.T.: 17.595 min
Delta R.T.: 0.013 min
Response: 153052
Conc: 1.45 ug/ml