

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060222AL\
 Data File : FD042736.D
 Signal(s) : FID2B.CH
 Acq On : 02 Jun 2022 13:12
 Operator : UA/NP
 Sample : N3107-01DL 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 14:57:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 07:55:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.579	1083095	6.521 ug/ml
Spiked Amount 50.000		Recovery =	13.04%
12) S 1-chlorooctadecane (S...	13.014	822926	6.301 ug/ml
Spiked Amount 50.000		Recovery =	12.60%
Target Compounds			
10) T n-Eicosane (C20)	12.623f	85236	0.567 ug/ml
14) T n-Tetracosane (C24)	14.832	39947	0.266 ug/ml
17) T n-Tricontane (C30)	17.719	92780	0.710 ug/ml
18) T n-Dotriacontane (C32)	18.548	132450	1.122 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060222AL\
Data File : FD042736.D
Signal(s) : FID2B.CH
Acq On : 02 Jun 2022 13:12
Operator : UA/NP
Sample : N3107-01DL 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 14:57:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 07:55:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

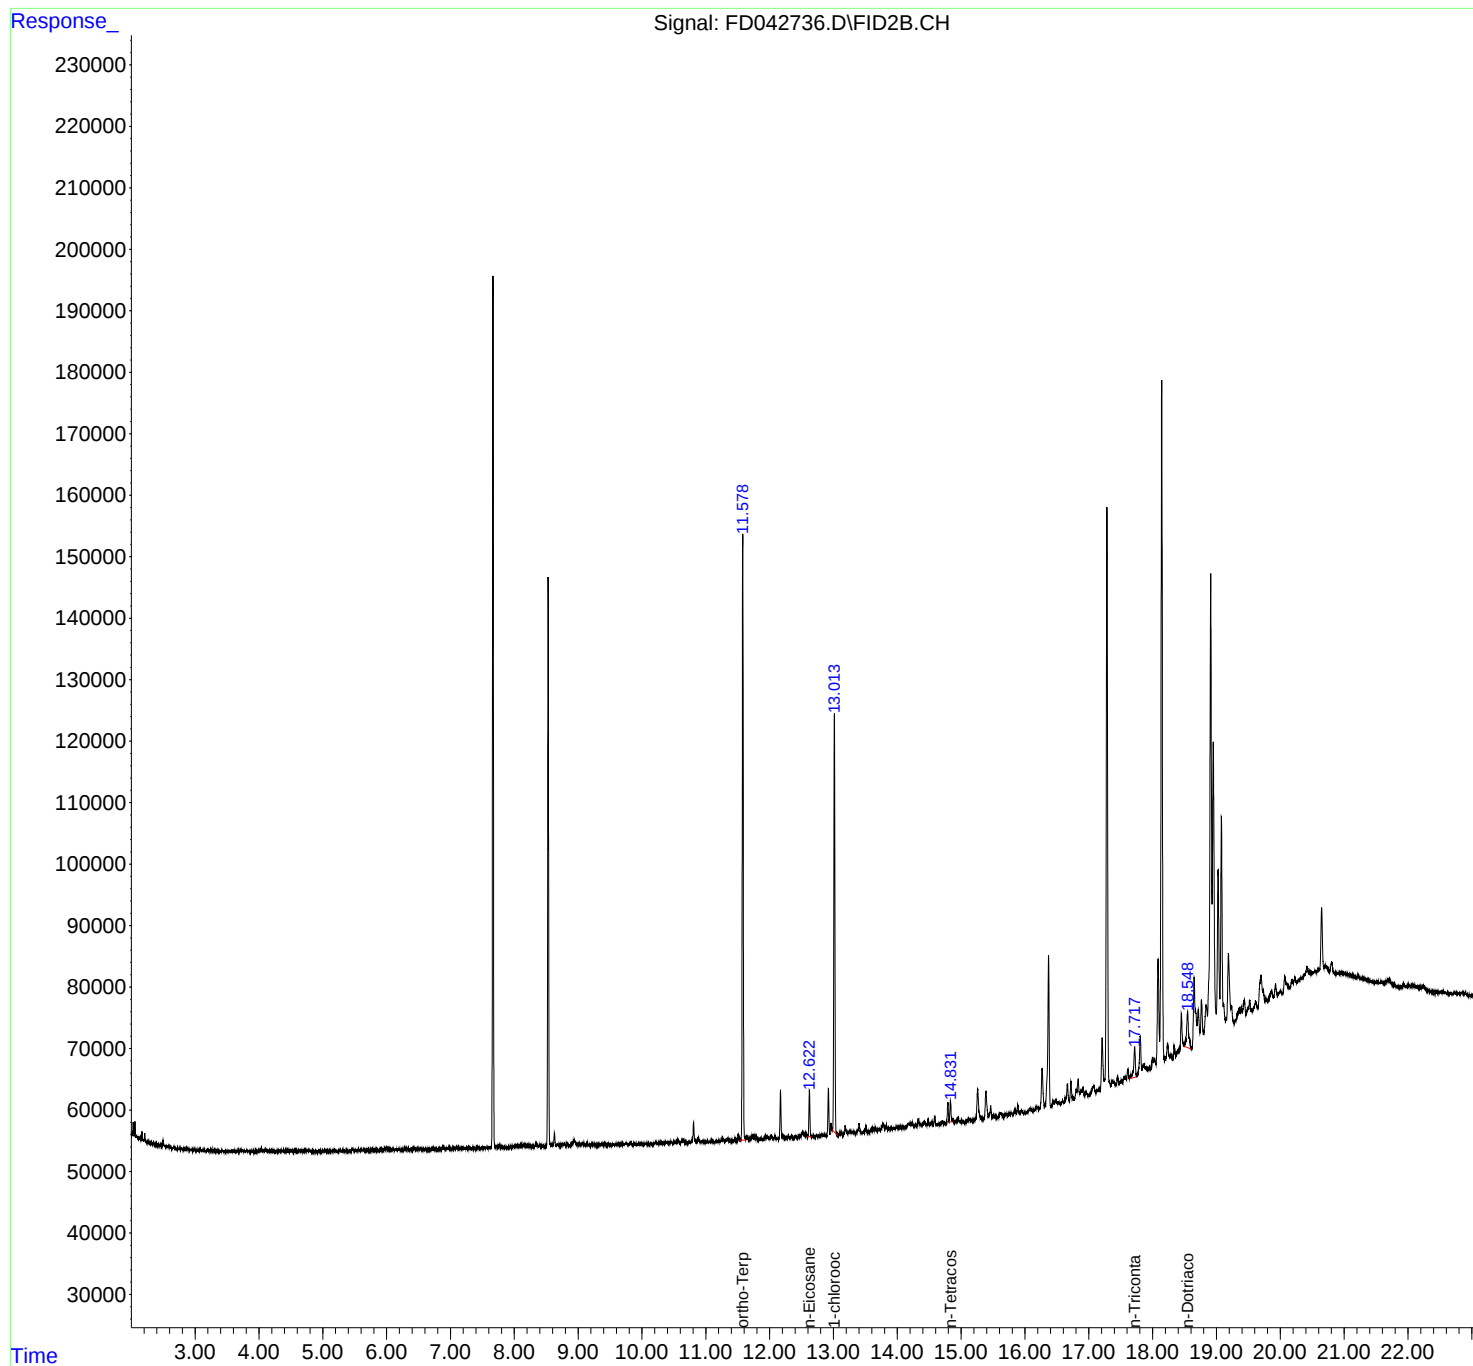


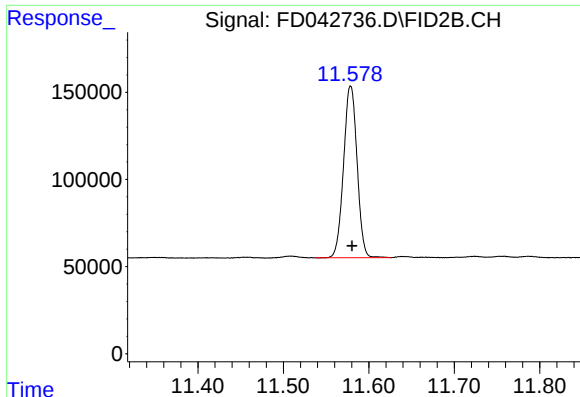

#9 ortho-Terphenyl (SURR)


R.T.: 11.579 min
Delta R.T.: -0.002 min
Response: 1083095
Conc: 6.52 ug/ml

Instrument :
FID_D
ClientSampleId :

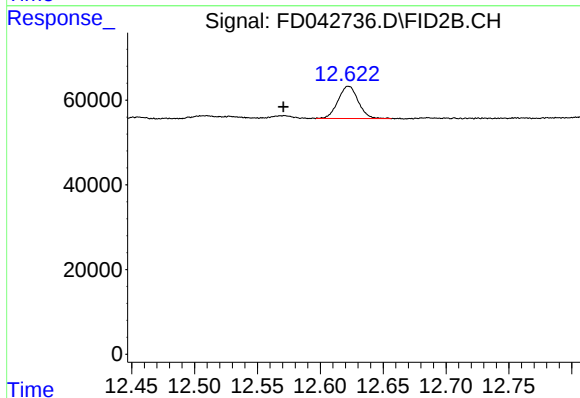


#10 n-Eicosane (C20)

R.T.: 12.623 min
Delta R.T.: 0.052 min
Response: 85236
Conc: 0.57 ug/ml

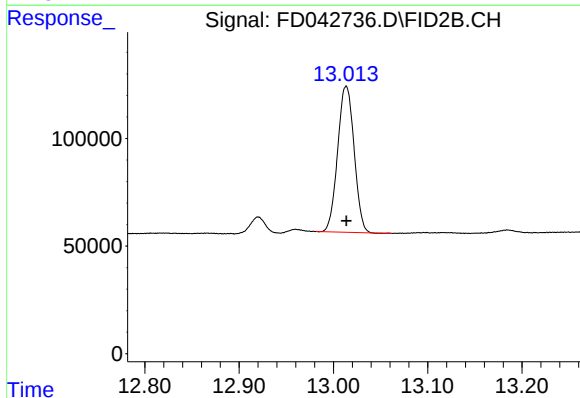


#12 1-chlorooctadecane (SURR)

R.T.: 13.014 min
Delta R.T.: 0.000 min
Response: 822926
Conc: 6.30 ug/ml

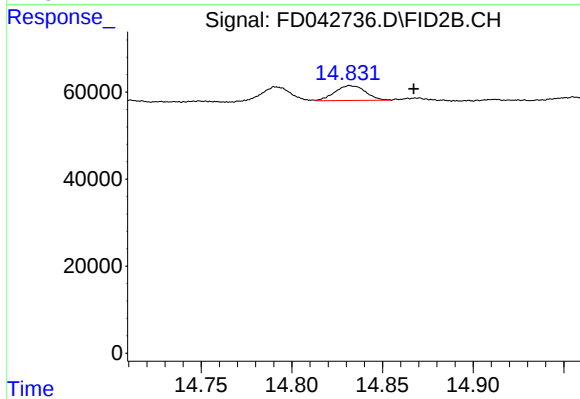

#14 n-Tetracosane (C24)


R.T.: 14.832 min
Delta R.T.: -0.035 min
Response: 39947
Conc: 0.27 ug/ml

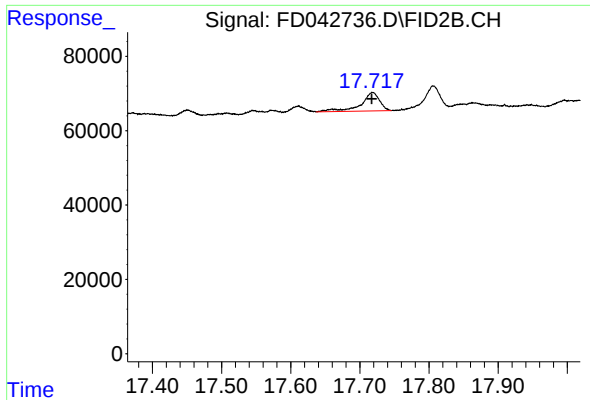

#17 n-Tricontane (C30)

R.T.: 17.719 min
Delta R.T.: 0.002 min
Response: 92780
Conc: 0.71 ug/ml

Instrument :
FID_D
ClientSampleId :

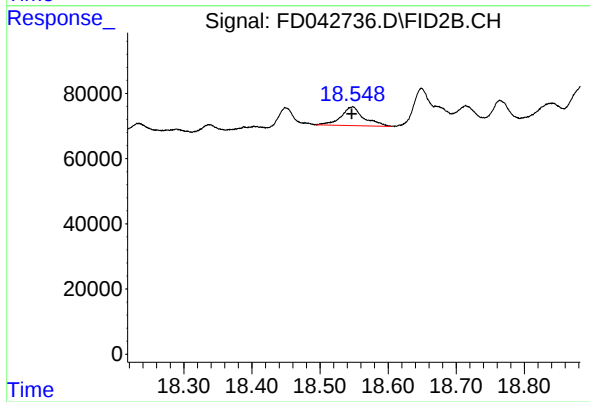

#18 n-Dotriacontane (C32)

R.T.: 18.548 min
Delta R.T.: 0.001 min
Response: 132450
Conc: 1.12 ug/ml