

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060222AL\
 Data File : FD042749.D
 Signal(s) : FID2B.CH
 Acq On : 02 Jun 2022 23:57
 Operator : UA/NP
 Sample : N3108-01D
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 03 01:42:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 07:55:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.589	9108725	54.844 ug/ml
Spiked Amount 50.000		Recovery =	109.69%
12) S 1-chlorooctadecane (S...	13.021	7270437	55.669 ug/ml
Spiked Amount 50.000		Recovery =	111.34%
Target Compounds			
10) T n-Eicosane (C20)	12.626f	62198	0.414 ug/ml
16) T n-Octacosane (C28)	16.834	44349	0.318 ug/ml
17) T n-Tricontane (C30)	17.721	72184	0.552 ug/ml
18) T n-Dotriacontane (C32)	18.550	207191	1.755 ug/ml
19) T n-Tetratriacontane (C34)	19.333	197510	1.858 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060222AL\
Data File : FD042749.D
Signal(s) : FID2B.CH
Acq On : 02 Jun 2022 23:57
Operator : UA/NP
Sample : N3108-01D
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 03 01:42:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 07:55:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

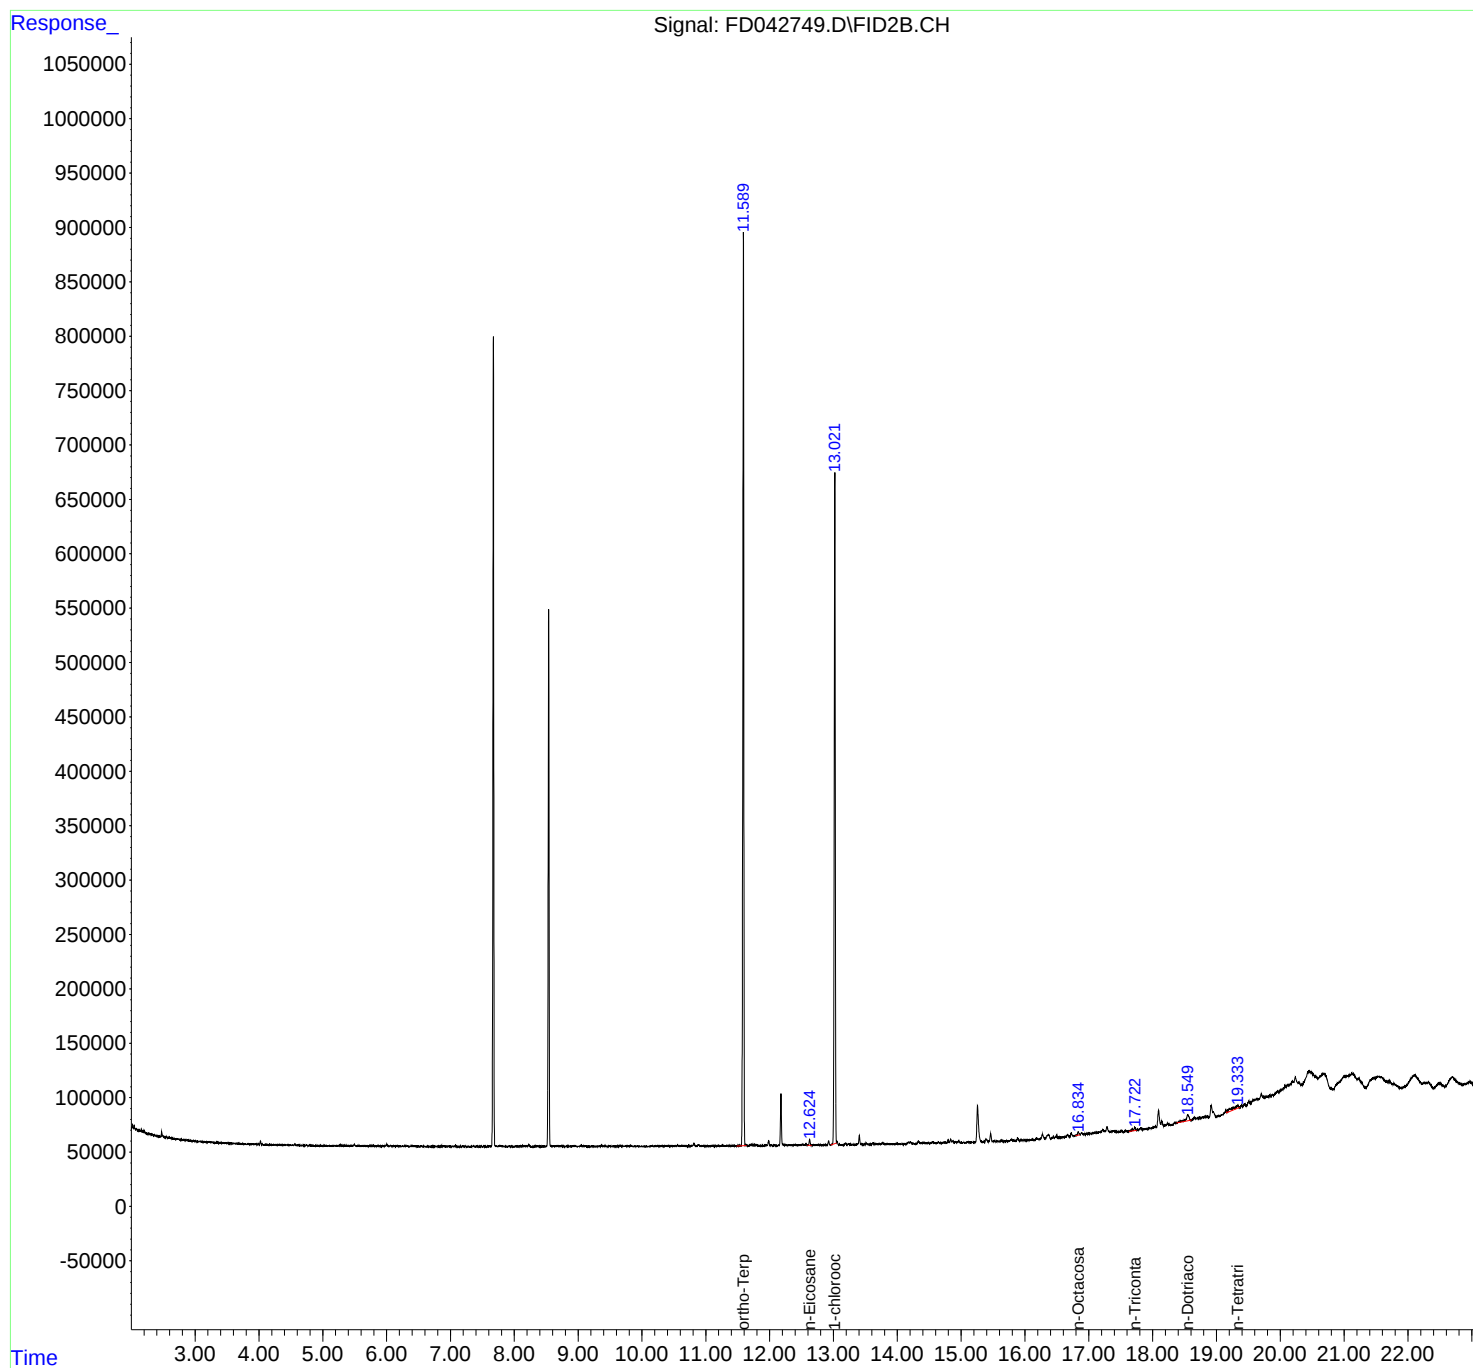


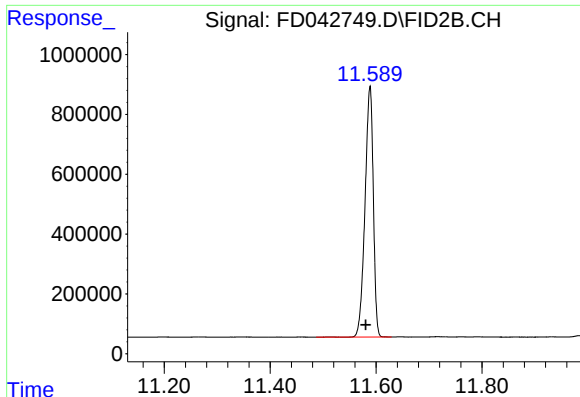

#9 ortho-Terphenyl (SURR)


R.T.: 11.589 min
Delta R.T.: 0.008 min
Response: 9108725
Conc: 54.84 ug/ml

Instrument :
FID_D
ClientSampleId :

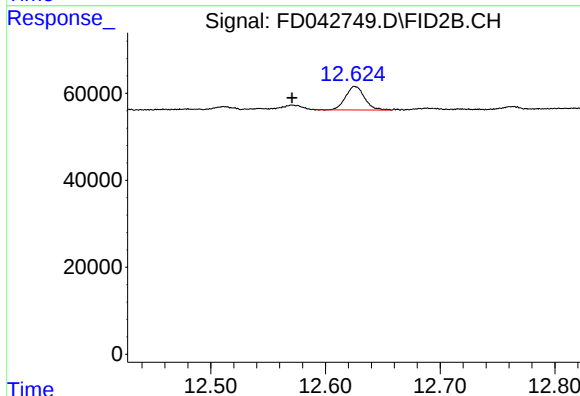


#10 n-Eicosane (C20)

R.T.: 12.626 min
Delta R.T.: 0.055 min
Response: 62198
Conc: 0.41 ug/ml

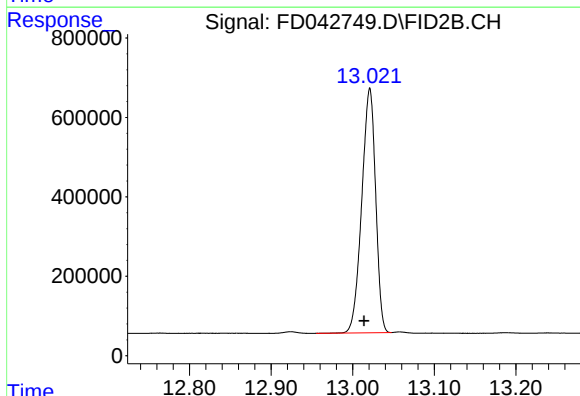


#12 1-chlorooctadecane (SURR)

R.T.: 13.021 min
Delta R.T.: 0.007 min
Response: 7270437
Conc: 55.67 ug/ml

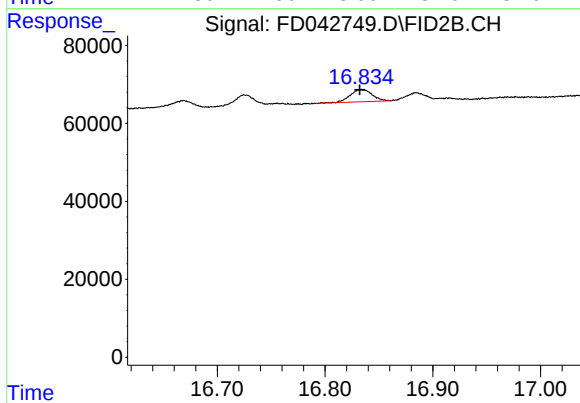

#16 n-Octacosane (C28)


R.T.: 16.834 min
Delta R.T.: 0.002 min
Response: 44349
Conc: 0.32 ug/ml

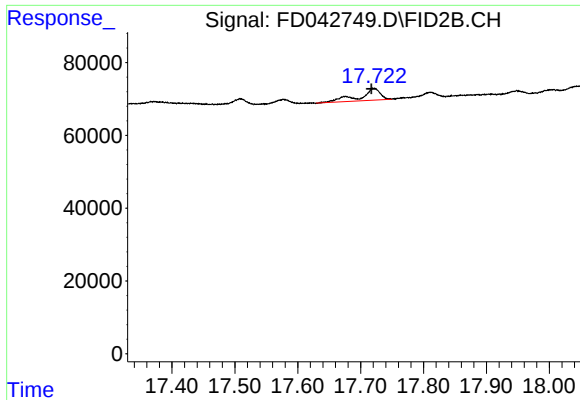

#17 n-Tricontane (C30)


R.T.: 17.721 min
Delta R.T.: 0.004 min
Response: 72184
Conc: 0.55 ug/ml

Instrument :
FID_D
ClientSampleId :

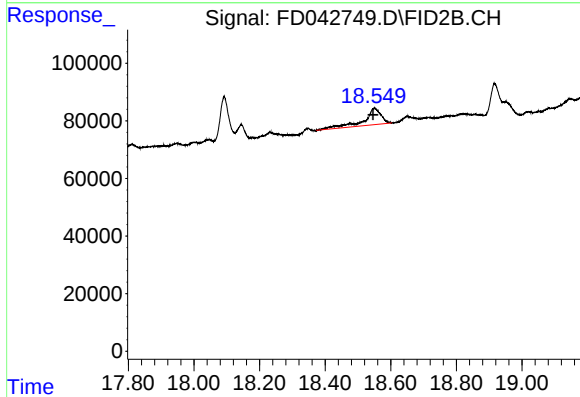

#18 n-Dotriacontane (C32)

R.T.: 18.550 min
Delta R.T.: 0.003 min
Response: 207191
Conc: 1.75 ug/ml

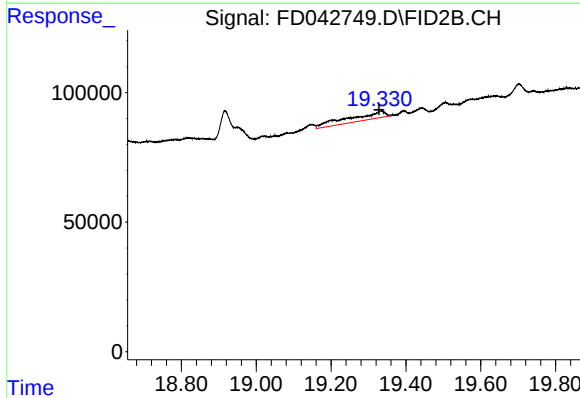

#19 n-Tetratriacontane (C34)

R.T.: 19.333 min
Delta R.T.: 0.004 min
Response: 197510
Conc: 1.86 ug/ml