

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060222AL\
 Data File : FD042735.D
 Signal(s) : FID2B.CH
 Acq On : 02 Jun 2022 12:30
 Operator : UA/NP
 Sample : N3083-23DL 100X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 D-17-5-B-SB-41(13.5-14)DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/03/2022
 Supervised By :Ankita Jodhani 06/03/2022

Integration File: sample.E
 Quant Time: Jun 02 13:11:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 07:55:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.579	108598	0.654 ug/mlm
Spiked Amount	50.000	Recovery	= 1.31%
12) S 1-chlorooctadecane (S...	13.015	81374	0.623 ug/ml
Spiked Amount	50.000	Recovery	= 1.25%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060222AL\
Data File : FD042735.D
Signal(s) : FID2B.CH
Acq On : 02 Jun 2022 12:30
Operator : UA/NP
Sample : N3083-23DL 100X
Misc :
ALS Vial : 56 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
D-17-5-B-SB-41(13.5-14)DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

Integration File: sample.E
Quant Time: Jun 02 13:11:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 07:55:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

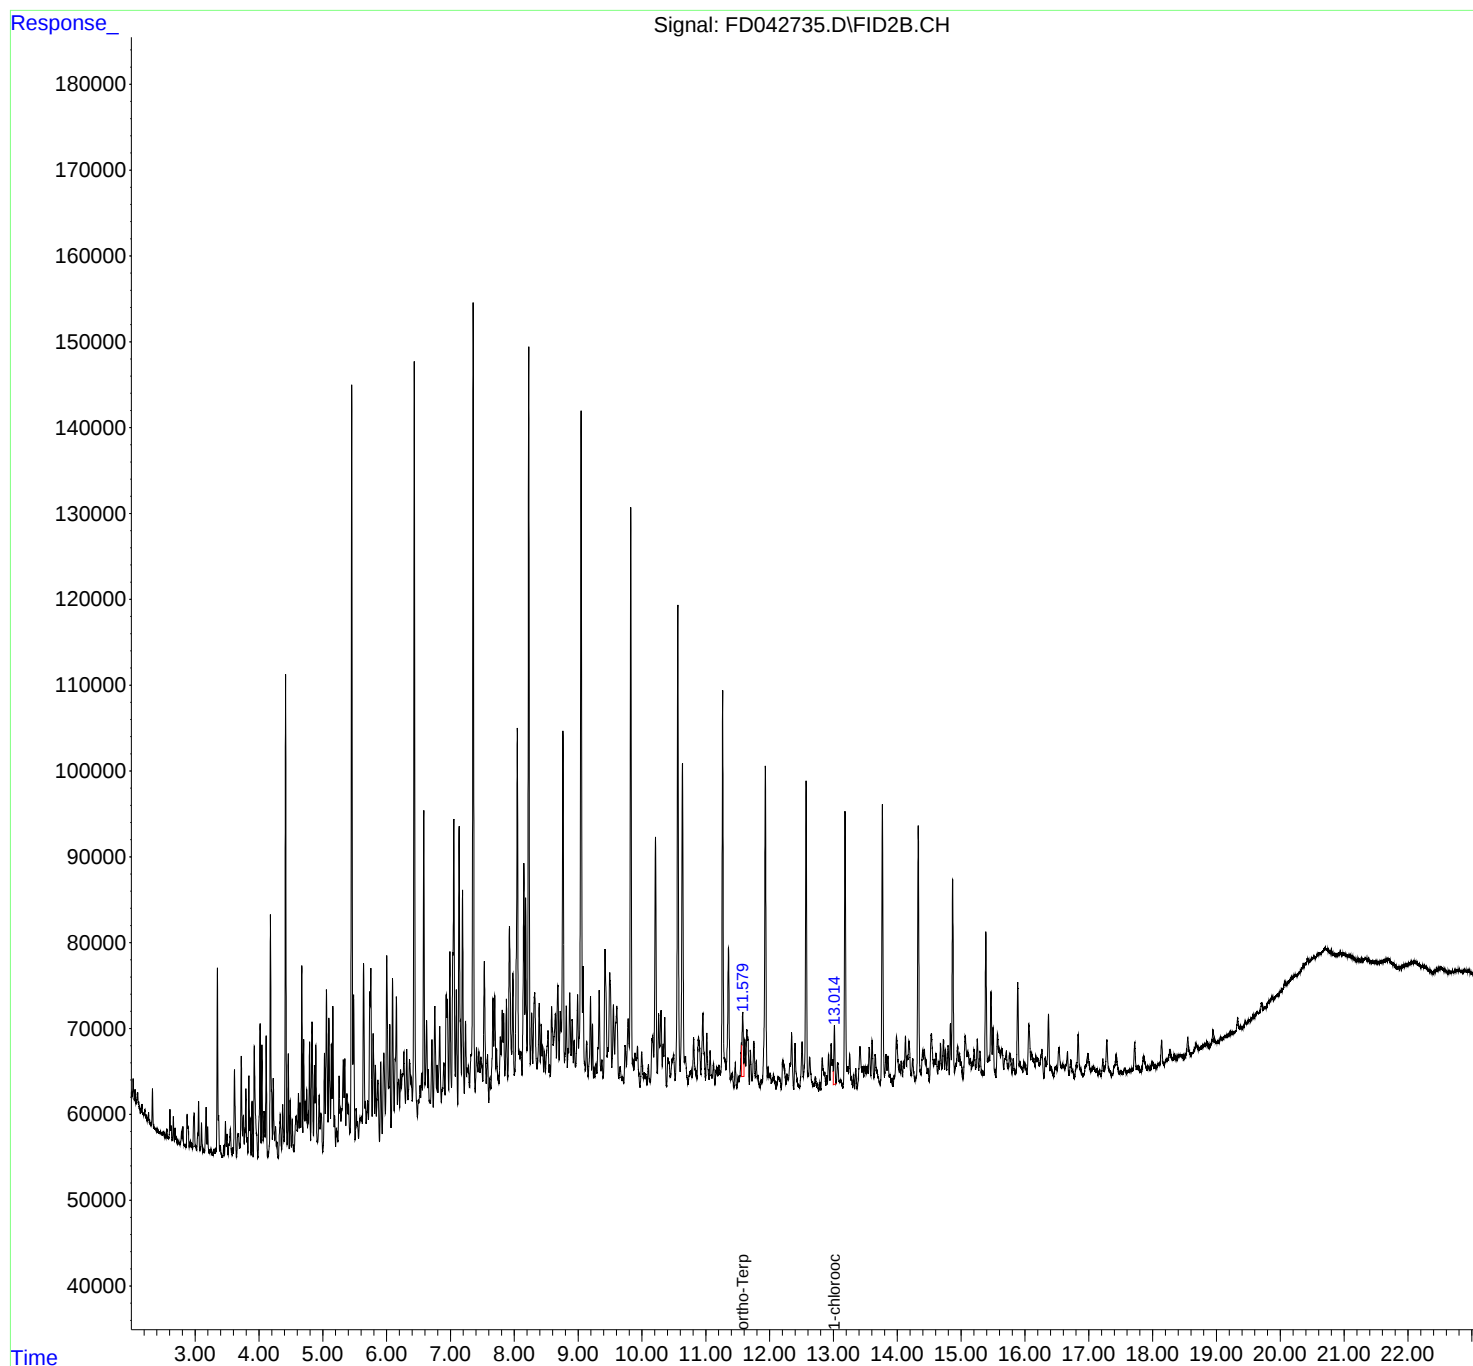

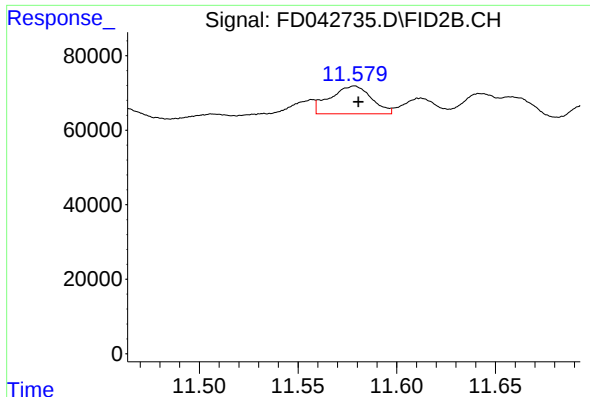


#9 ortho-Terphenyl (SURR)

R.T.: 11.579 min
Delta R.T.: -0.002 min
Response: 108598
Conc: 0.65 ug/ml

Instrument :
FID_D
ClientSampleId :
D-17-5-B-SB-41(13.5-14)DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

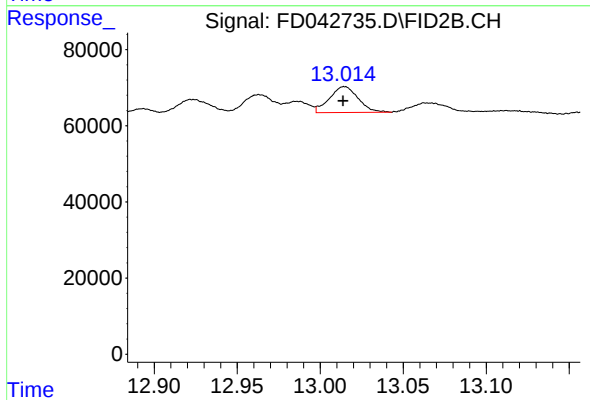

#12 1-chlorooctadecane (SURR)

R.T.: 13.015 min
Delta R.T.: 0.000 min
Response: 81374
Conc: 0.62 ug/ml