

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060823AR\
Data File : FD045826.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2023 10:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 12:19:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:44:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T Benzo[a]anthracene (C...	14.670	30407	0.194 ug/ml
15) T Chrysene (C27.41)	14.670	30407	0.184 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD060823AR\
Data File : FD045826.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2023 10:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 12:19:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:44:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

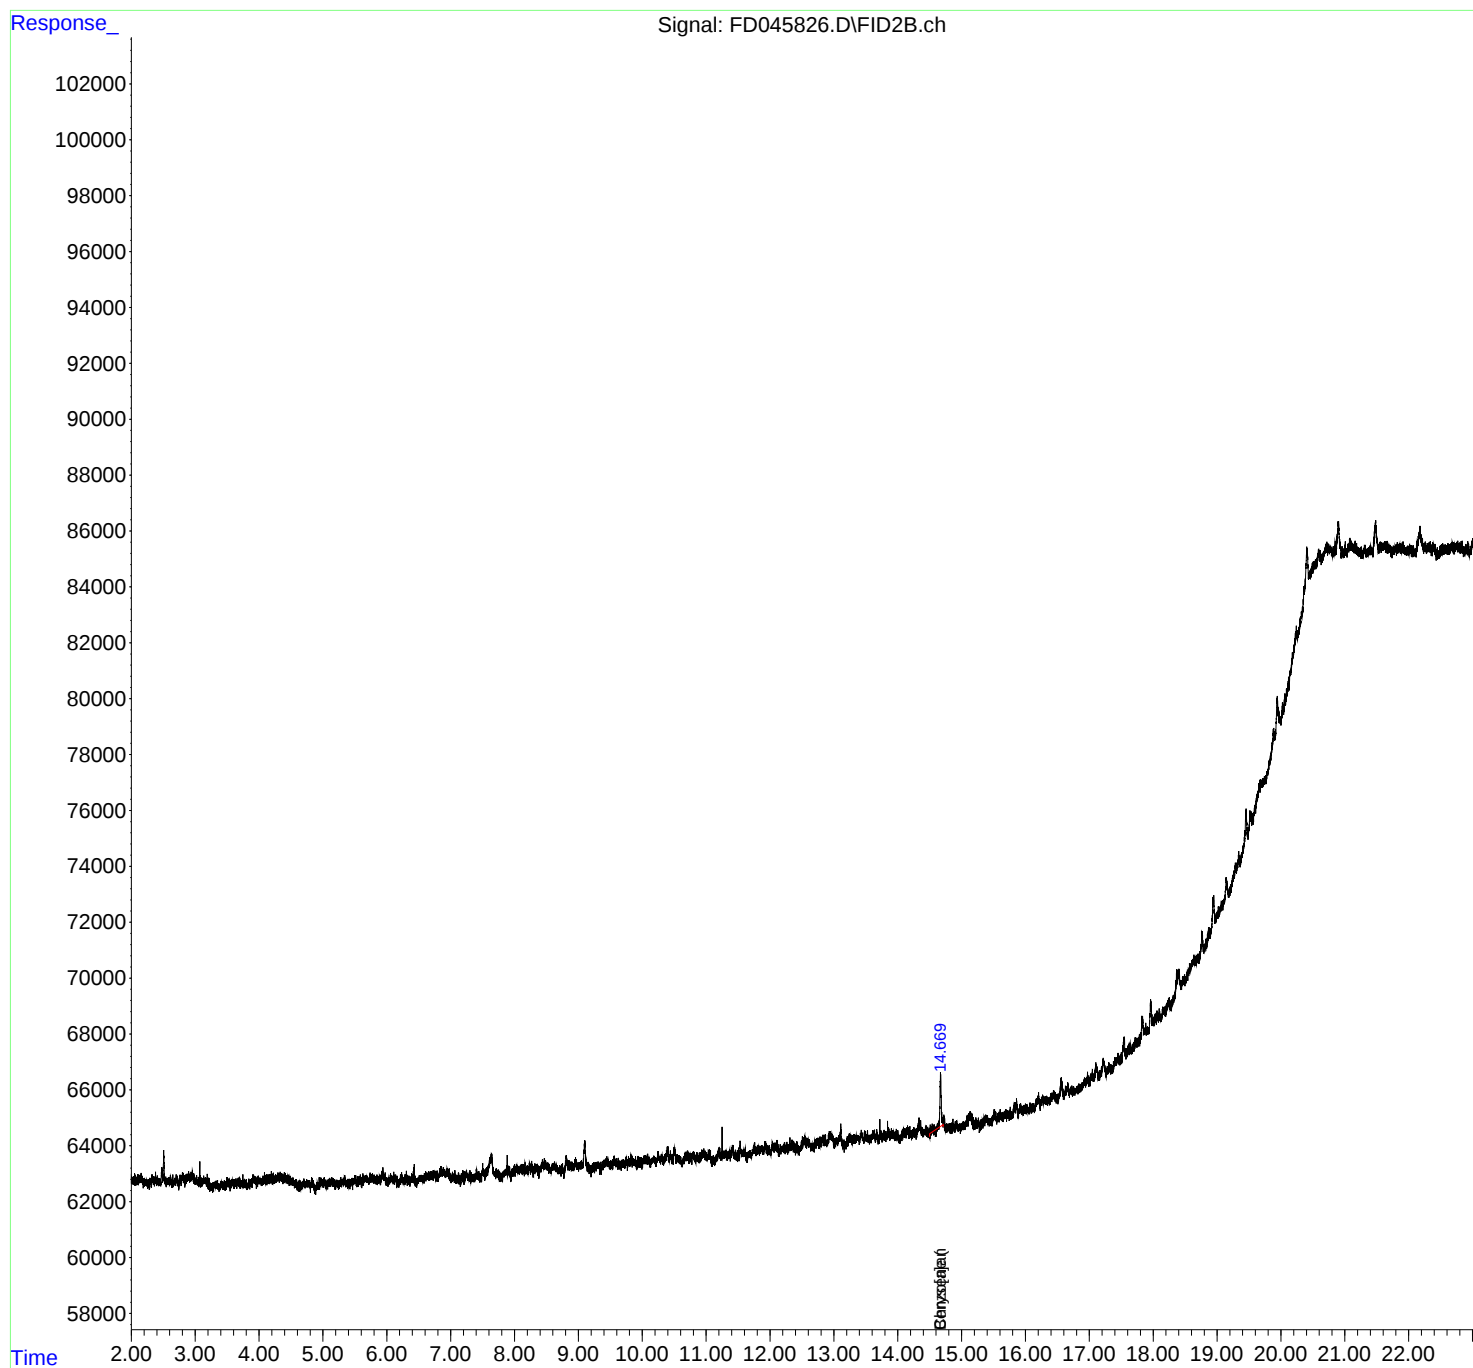


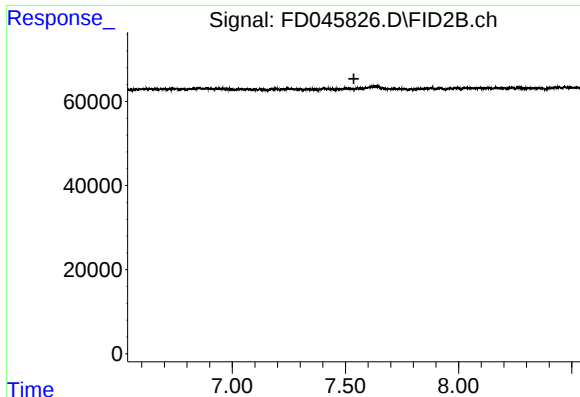

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.537 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

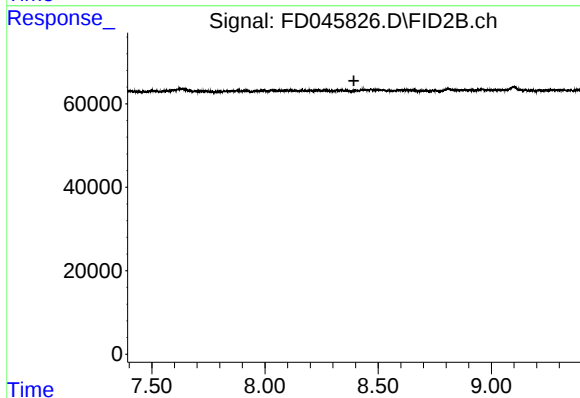


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.393 min
Response: 0
Conc: N.D.

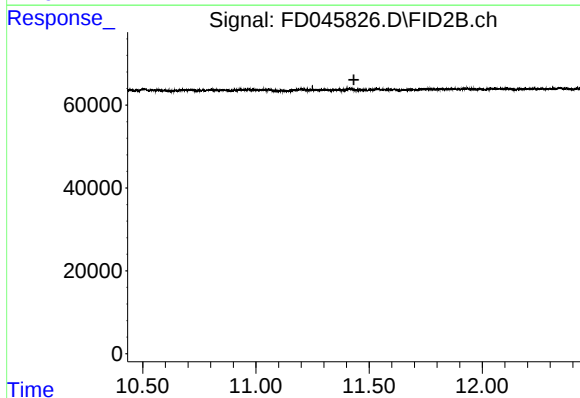


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.433 min
Response: 0
Conc: N.D.

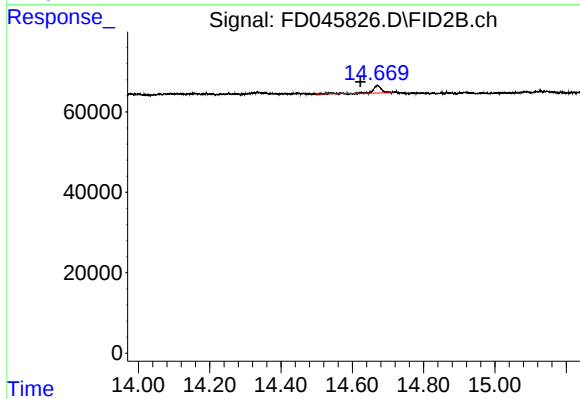

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.670 min
Delta R.T.: 0.047 min
Response: 30407
Conc: 0.19 ug/ml

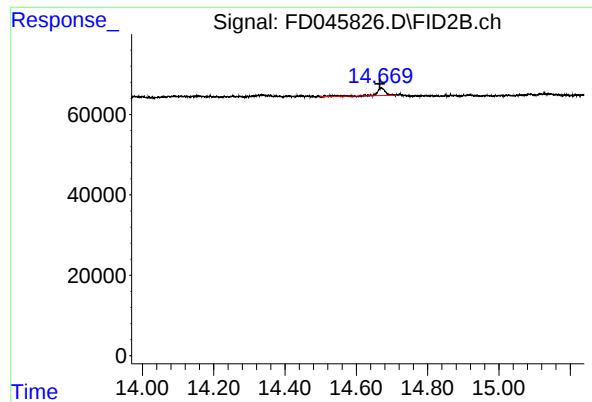

#15 Chrysene (C27.41)

R.T.: 14.670 min
Delta R.T.: 0.005 min
Response: 30407
Conc: 0.18 ug/ml

Instrument :

FID_D

ClientSampleId :