

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD061325AR\
Data File : FD049479.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2025 06:29
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 13 21:18:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 052425.M
Quant Title : GC Extractables
QLast Update : Tue May 27 03:11:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	18.187	132656	1.039 ug/ml
20) T	Dibenz[a,h]anthracene...	18.187	132656	0.985 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD061325AR\
Data File : FD049479.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2025 06:29
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 13 21:18:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 052425.M
Quant Title : GC Extractables
QLast Update : Tue May 27 03:11:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

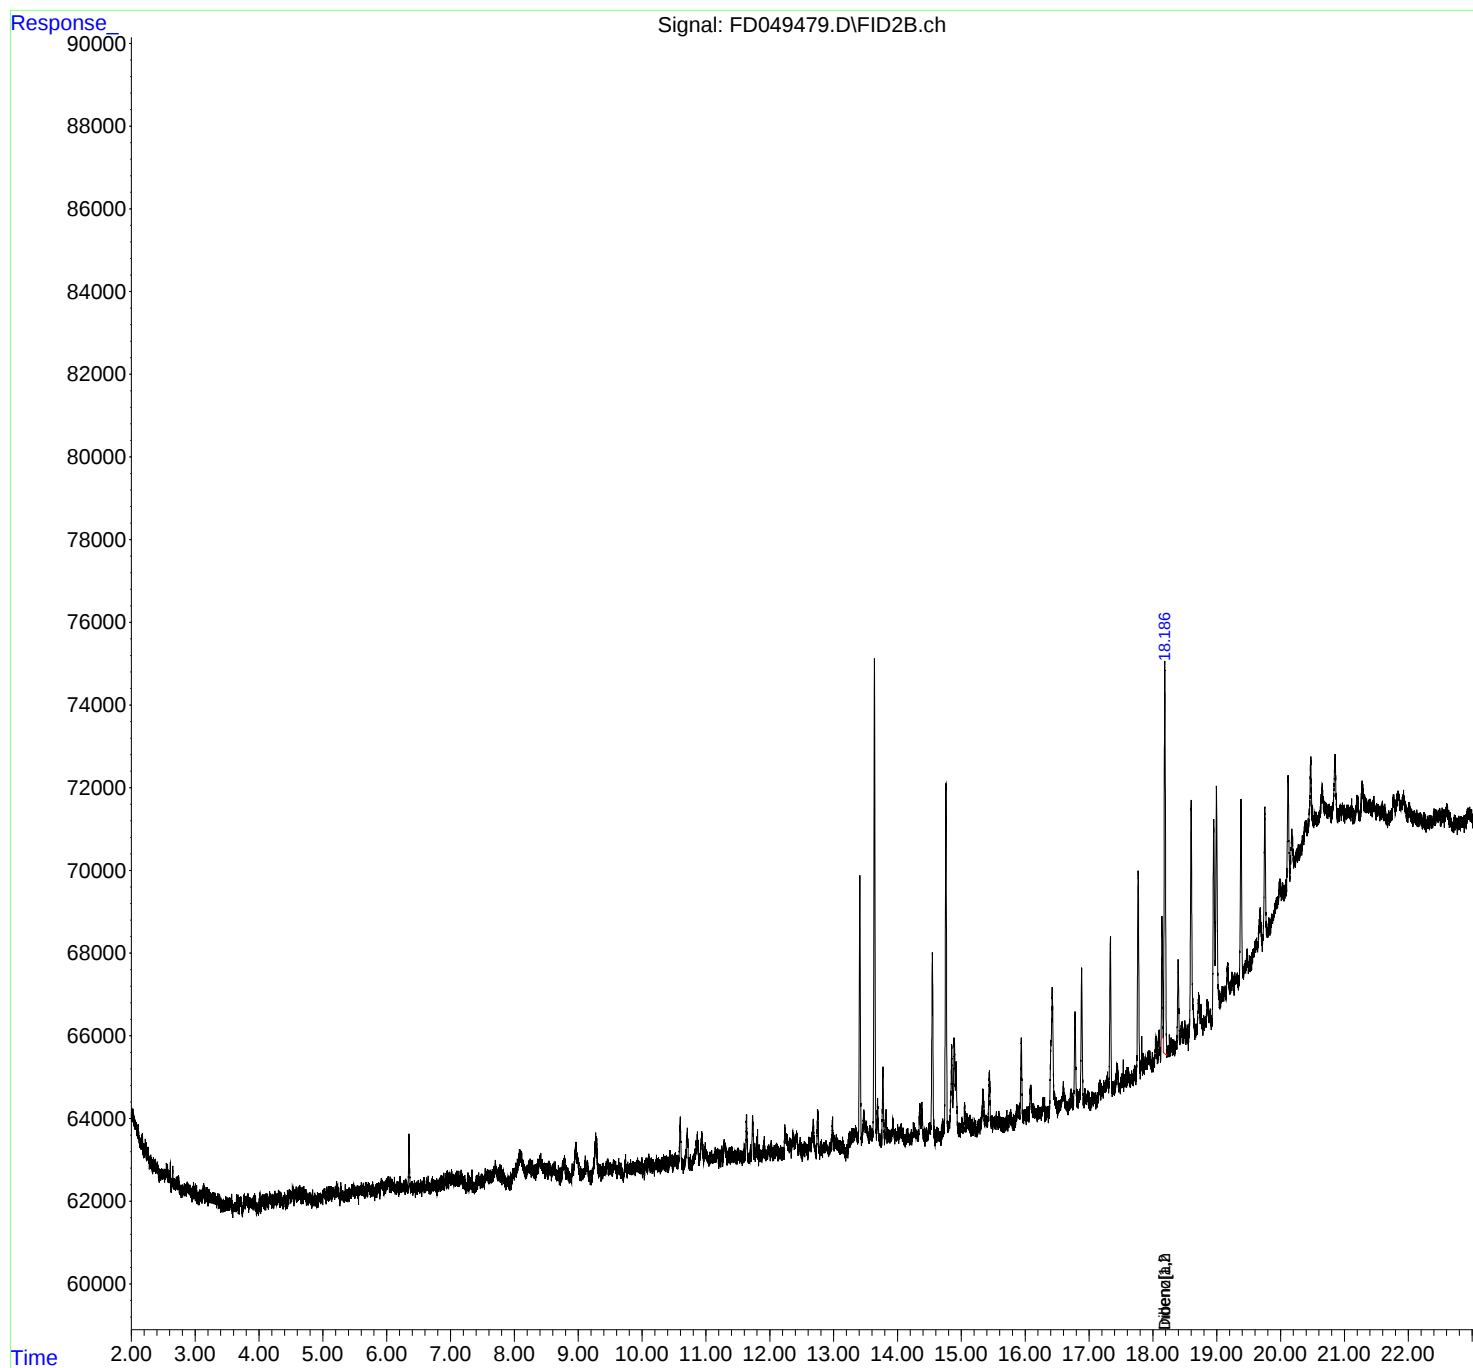


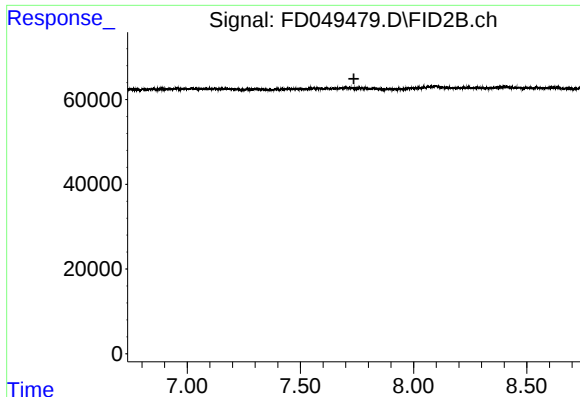

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T. : 7.736 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
MECL2

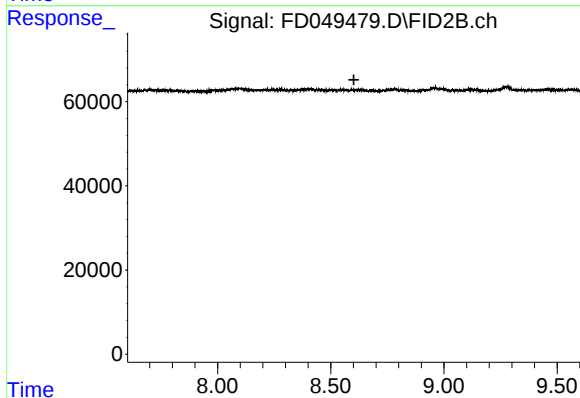


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 8.602 min
Response: 0
Conc: N.D.

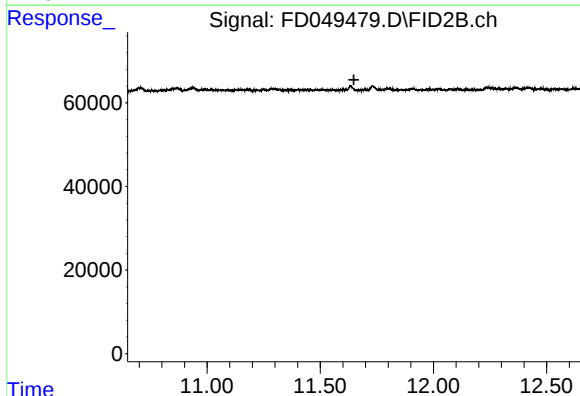


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.648 min
Response: 0
Conc: N.D.

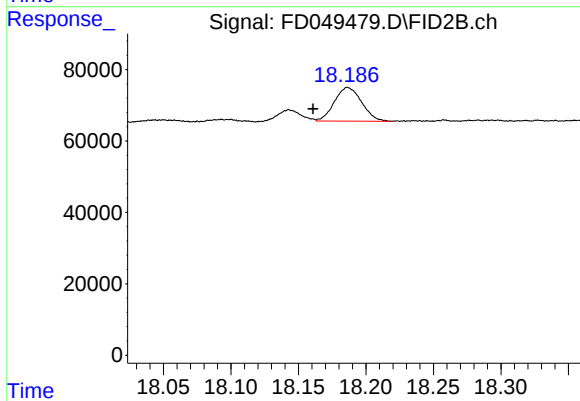

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.187 min
Delta R.T.: 0.026 min
Response: 132656
Conc: 1.04 ug/ml

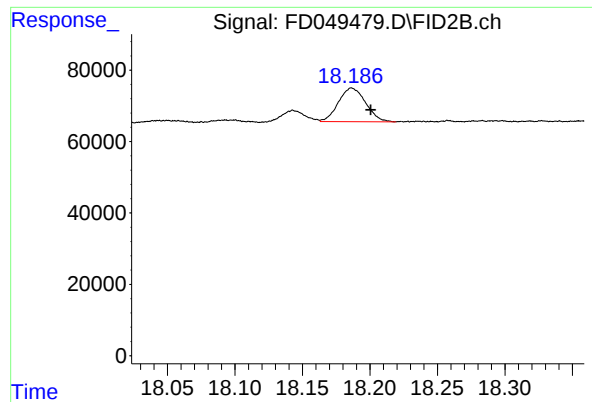

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.187 min
Delta R.T.: -0.014 min
Response: 132656
Conc: 0.99 ug/ml

Instrument :
FID_D
ClientSampleId :
MECL2