

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD062425AR\
 Data File : FD049502.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jun 2025 05:43
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Jun 24 23:51:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 15:23:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	Indeno[1,2,3-cd]pyren...	18.190	114029	0.931 ug/ml
20) T	Dibenz[a,h]anthracene...	18.190	114029	0.890 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD062425AR\
Data File : FD049502.D
Signal(s) : FID2B.ch
Acq On : 24 Jun 2025 05:43
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 24 23:51:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 15:23:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

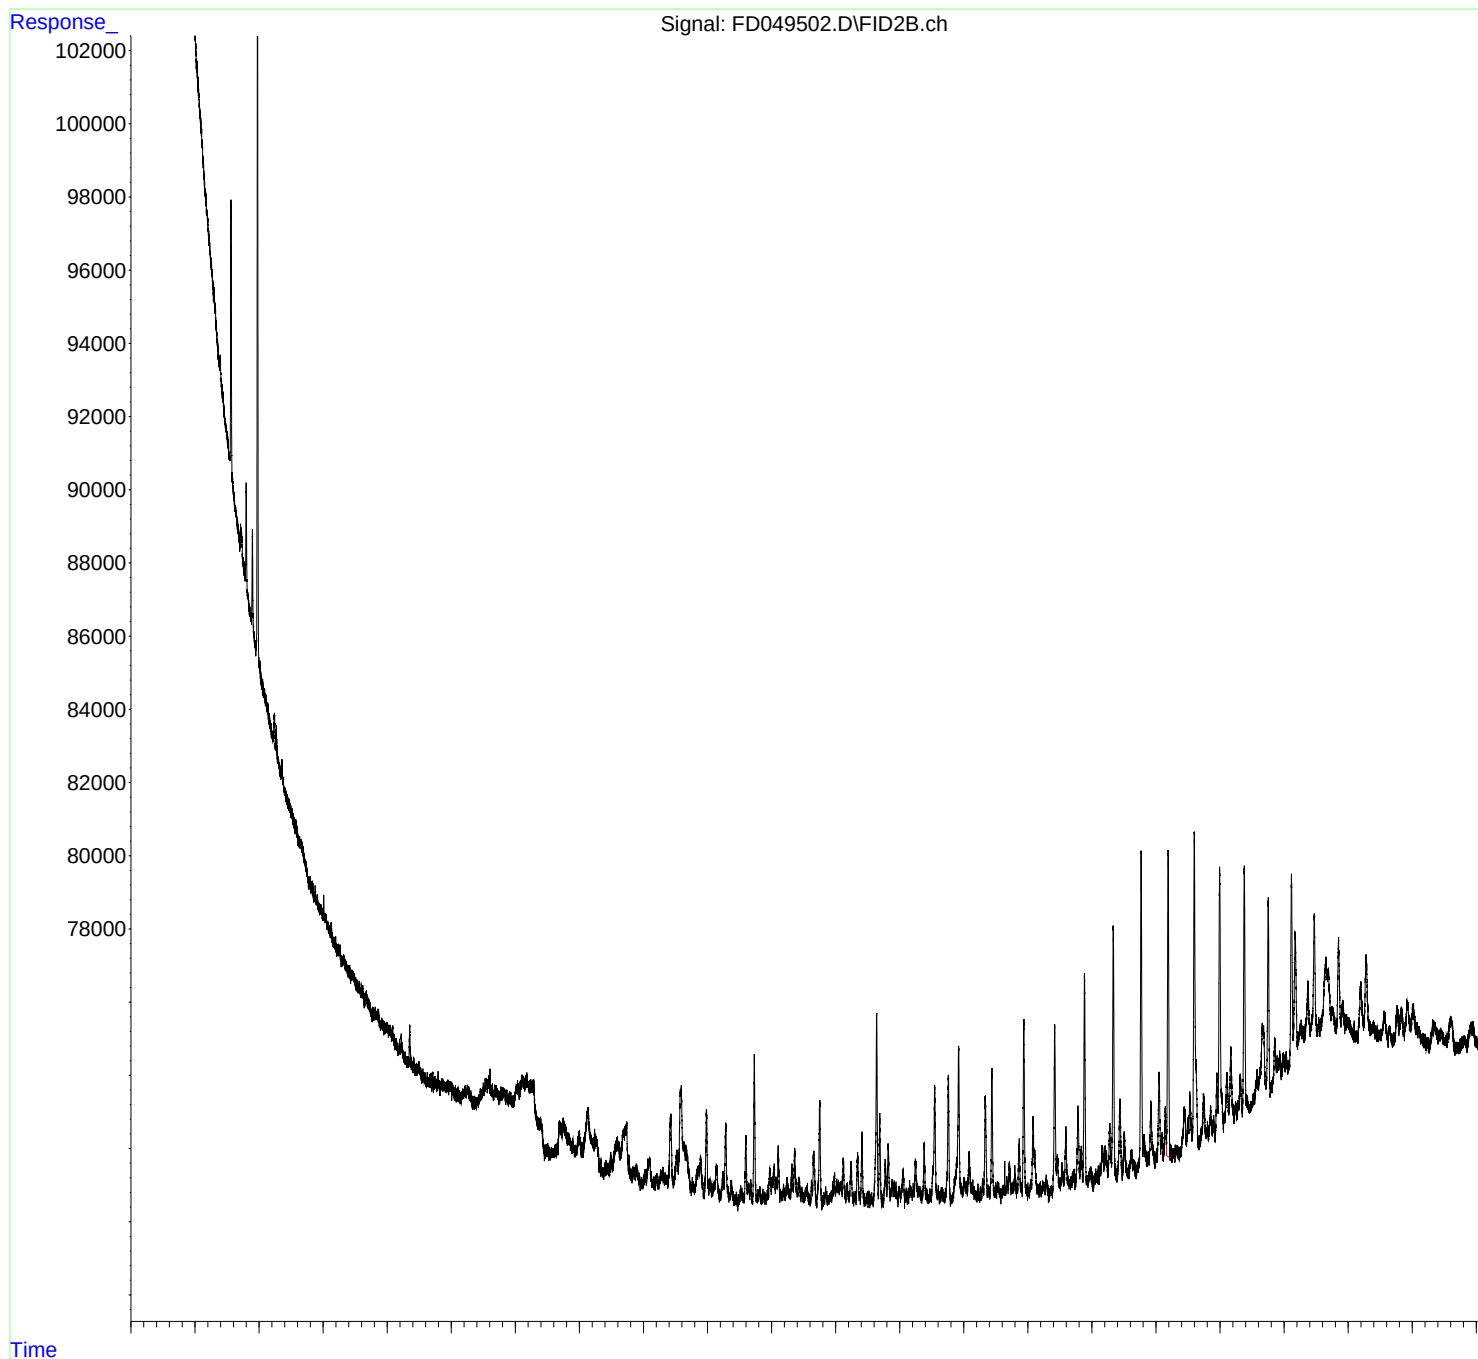


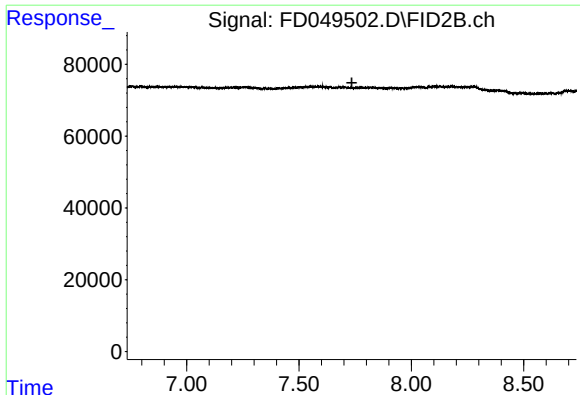

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T.: 7.735 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
MECL2

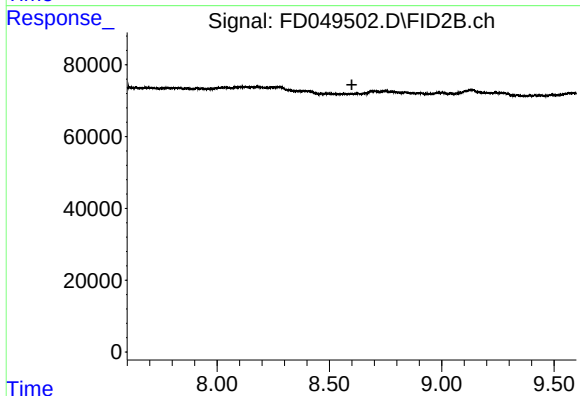


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 8.599 min
Response: 0
Conc: N.D.

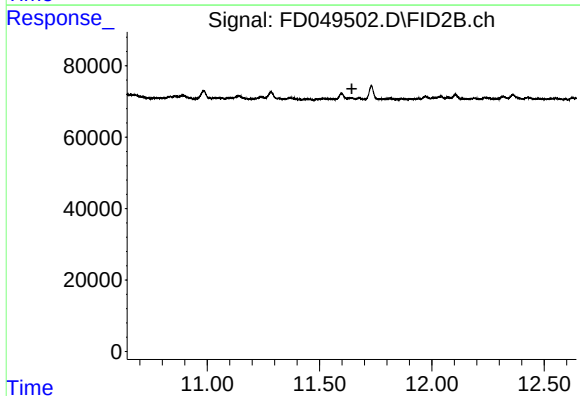


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.643 min
Response: 0
Conc: N.D.

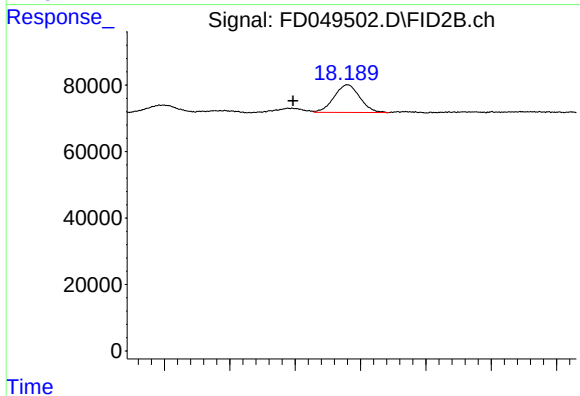

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.190 min
Delta R.T.: 0.042 min
Response: 114029
Conc: 0.93 ug/ml

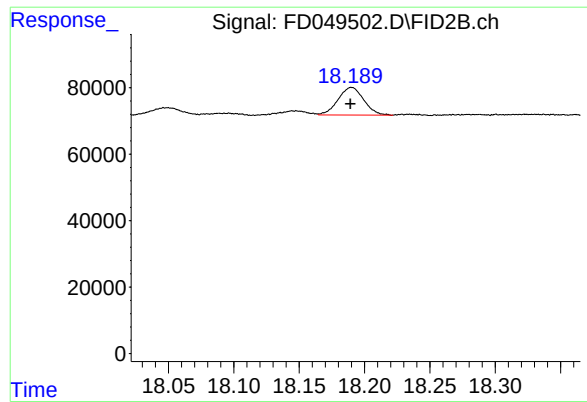

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.190 min
Delta R.T.: 0.000 min
Response: 114029
Conc: 0.89 ug/ml

Instrument :
FID_D
ClientSampleId :
MECL2