

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD062723AR\
 Data File : FD046038.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2023 20:10
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 02:16:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 062423.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 25 04:38:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
12) T	Fluoranthene (C21.85)	12.507f	99230	0.485 ug/ml
14) T	Benzo[a]anthracene (C...	14.646	117661	0.654 ug/ml
15) T	Chrysene (C27.41)	14.646	117661	0.599 ug/ml
16) T	benzo[b]fluoranthene ...	16.162	152235	0.812 ug/ml
17) T	Bnezo[k]fluoranthene ...	16.162	152235	0.770 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD062723AR\
Data File : FD046038.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2023 20:10
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 02:16:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 062423.M
Quant Title : GC Extractables
QLast Update : Sun Jun 25 04:38:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

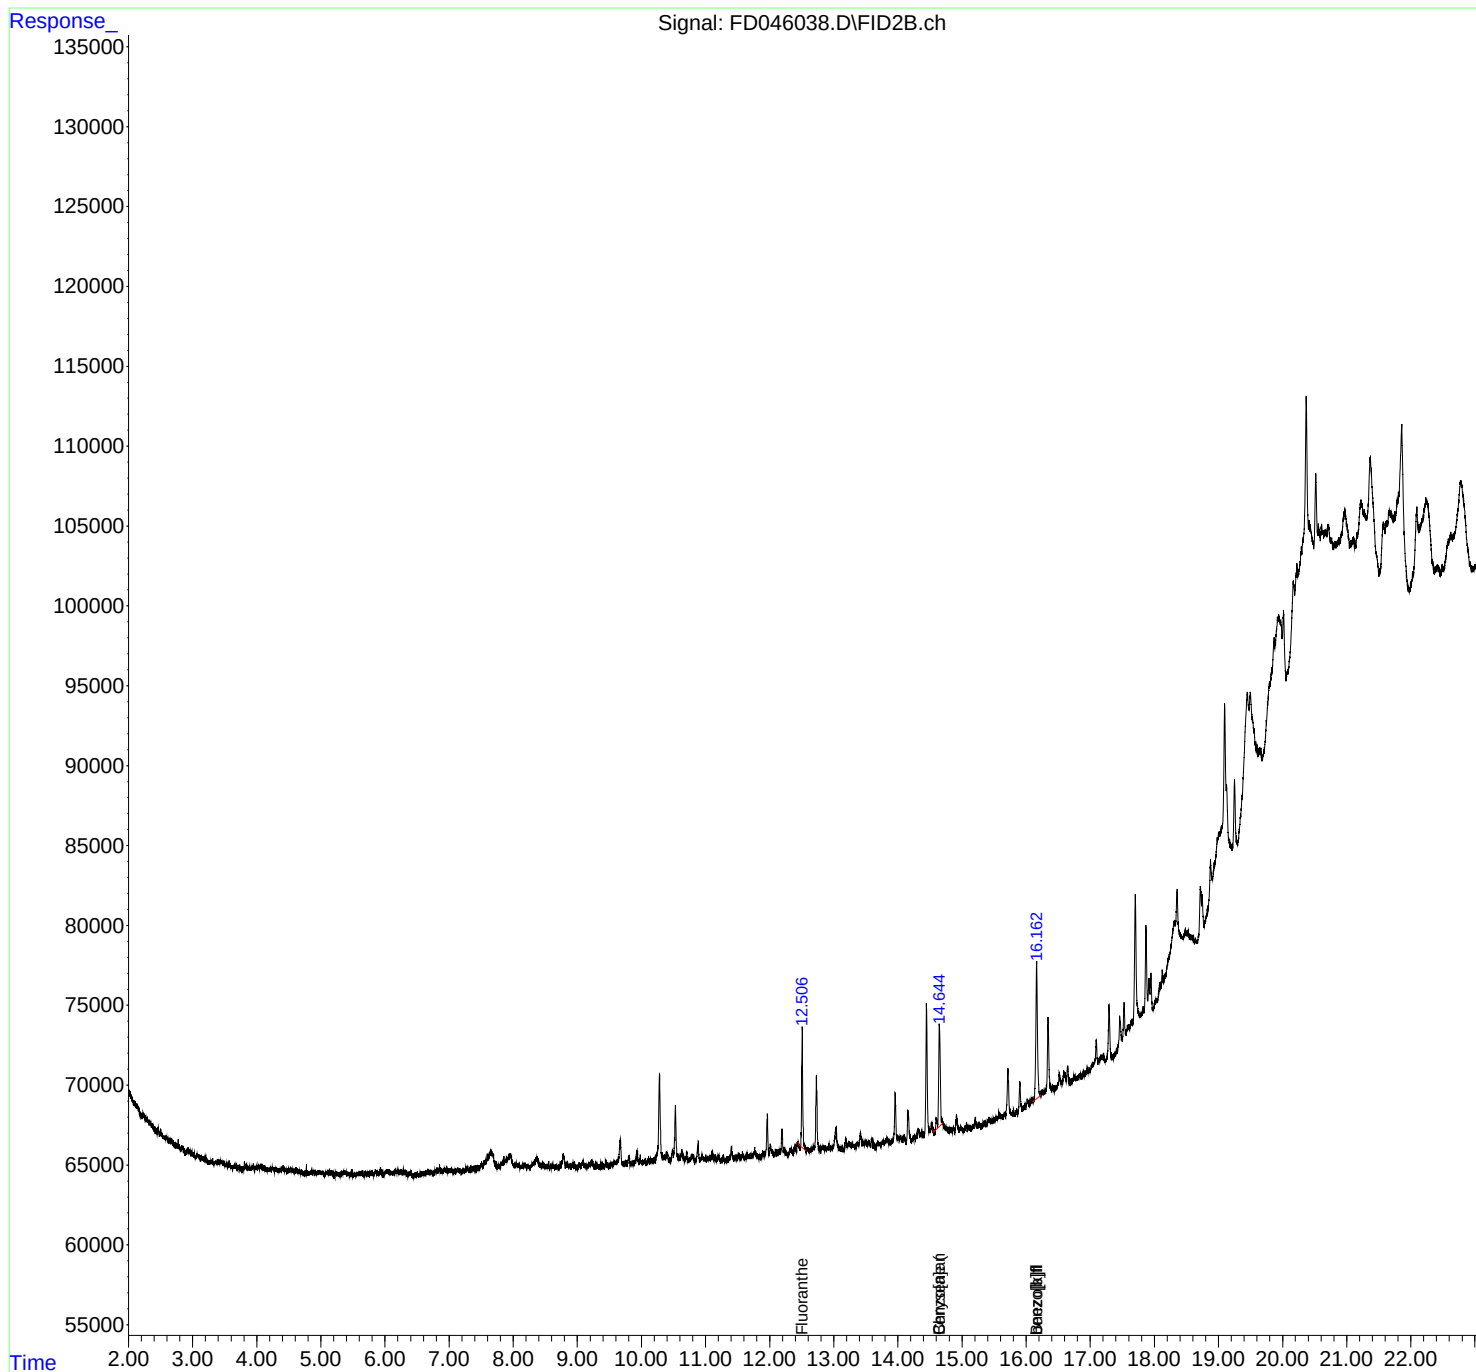


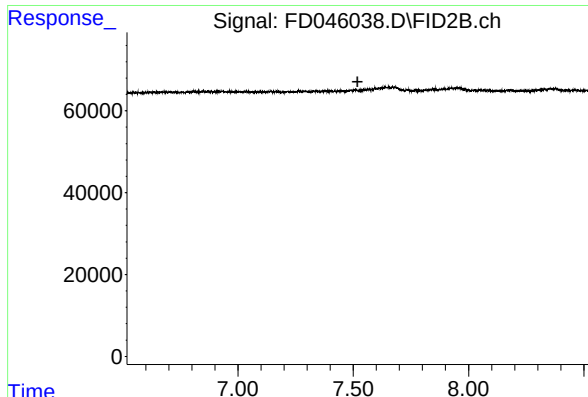

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.518 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

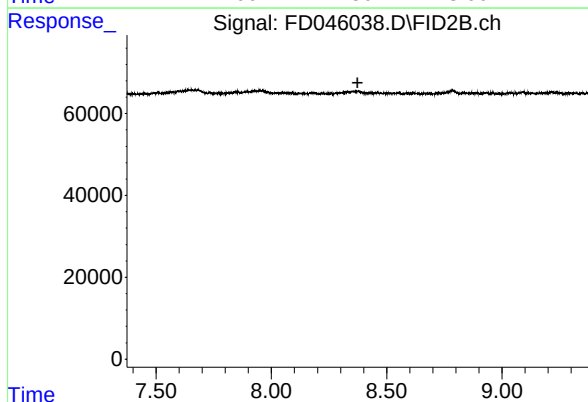


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.374 min
Response: 0
Conc: N.D.

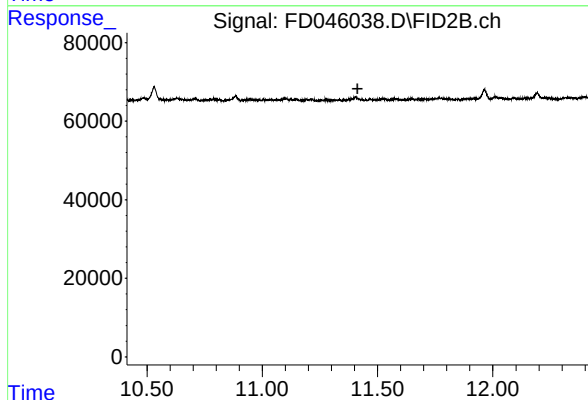


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.413 min
Response: 0
Conc: N.D.

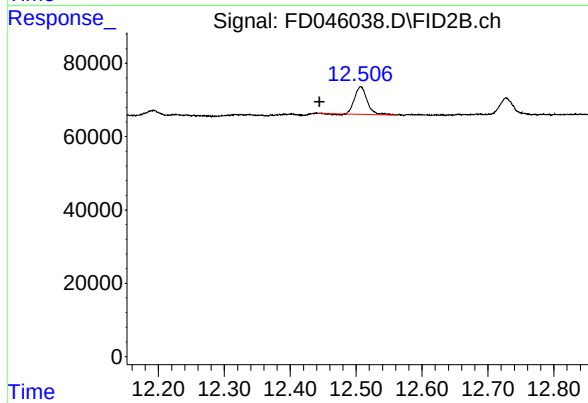

#12 Fluoranthene (C21.85)


R.T.: 12.507 min
Delta R.T.: 0.062 min
Response: 99230
Conc: 0.48 ug/ml

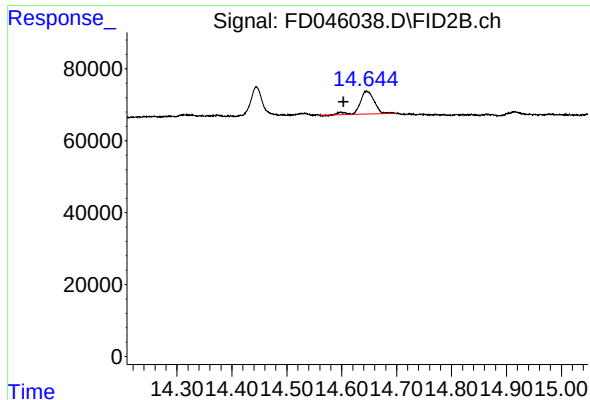

#14 Benzo[a]anthracene (C26.37)


R.T.: 14.646 min
Delta R.T.: 0.042 min
Response: 117661
Conc: 0.65 ug/ml

Instrument :
FID_D
ClientSampleId :

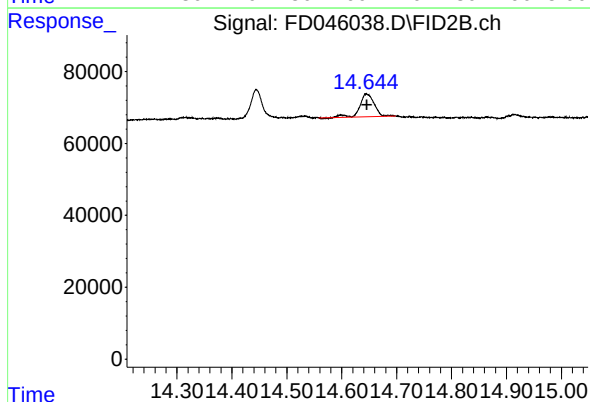


#15 Chrysene (C27.41)

R.T.: 14.646 min
Delta R.T.: 0.000 min
Response: 117661
Conc: 0.60 ug/ml

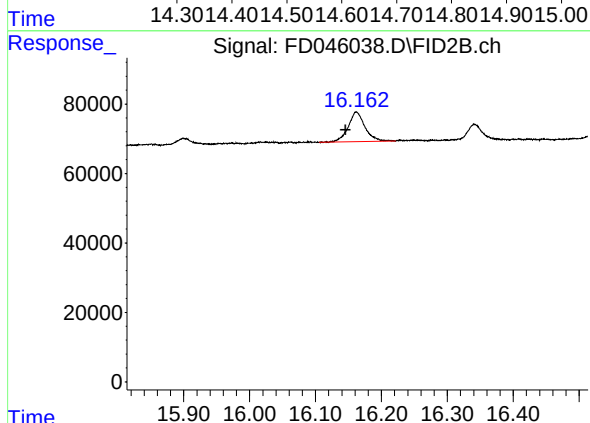

#16 benzo[b]fluoranthene (C30.41)

R.T.: 16.162 min
Delta R.T.: 0.016 min
Response: 152235
Conc: 0.81 ug/ml

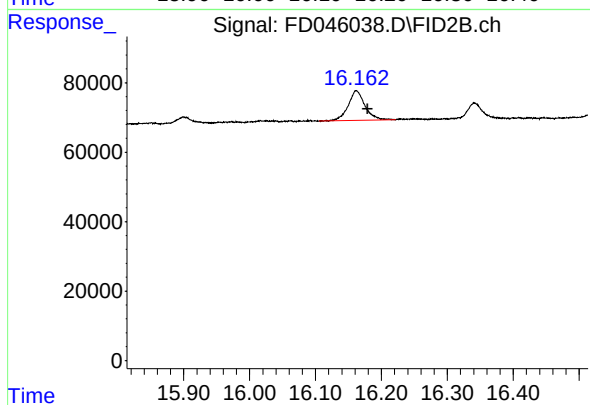

#17 Bnezo[k]fluoranthene (C30.14)

R.T.: 16.162 min
Delta R.T.: -0.017 min
Response: 152235
Conc: 0.77 ug/ml