

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD070120AL\
 Data File : FD033860.D
 Signal(s) : FID2B.CH
 Acq On : 02 Jul 2020 00:43
 Operator : DD\AJ
 Sample : L2814-18DL 10X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 PL-02-063020-3DL

Integration File: autoint1.e
 Quant Time: Jul 02 02:46:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 061820.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 19 09:06:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.453	406338	2.843 ug/ml
Spiked Amount 50.000		Recovery =	5.69%
12) S 1-chlorooctadecane (S...	12.872	3290320	27.984 ug/ml
Spiked Amount 50.000		Recovery =	55.97%
Target Compounds			
10) T n-Eicosane (C20)	12.508f	598834	4.399 ug/ml
11) T n-Heneicosane (C21)	13.105	573078	4.198 ug/ml
14) T n-Tetracosane (C24)	14.723	276771	2.025 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD070120AL\
Data File : FD033860.D
Signal(s) : FID2B.CH
Acq On : 02 Jul 2020 00:43
Operator : DD\AJ
Sample : L2814-18DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
PL-02-063020-3DL

Integration File: autoint1.e
Quant Time: Jul 02 02:46:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 061820.M
Quant Title : GC Extractables
QLast Update : Fri Jun 19 09:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

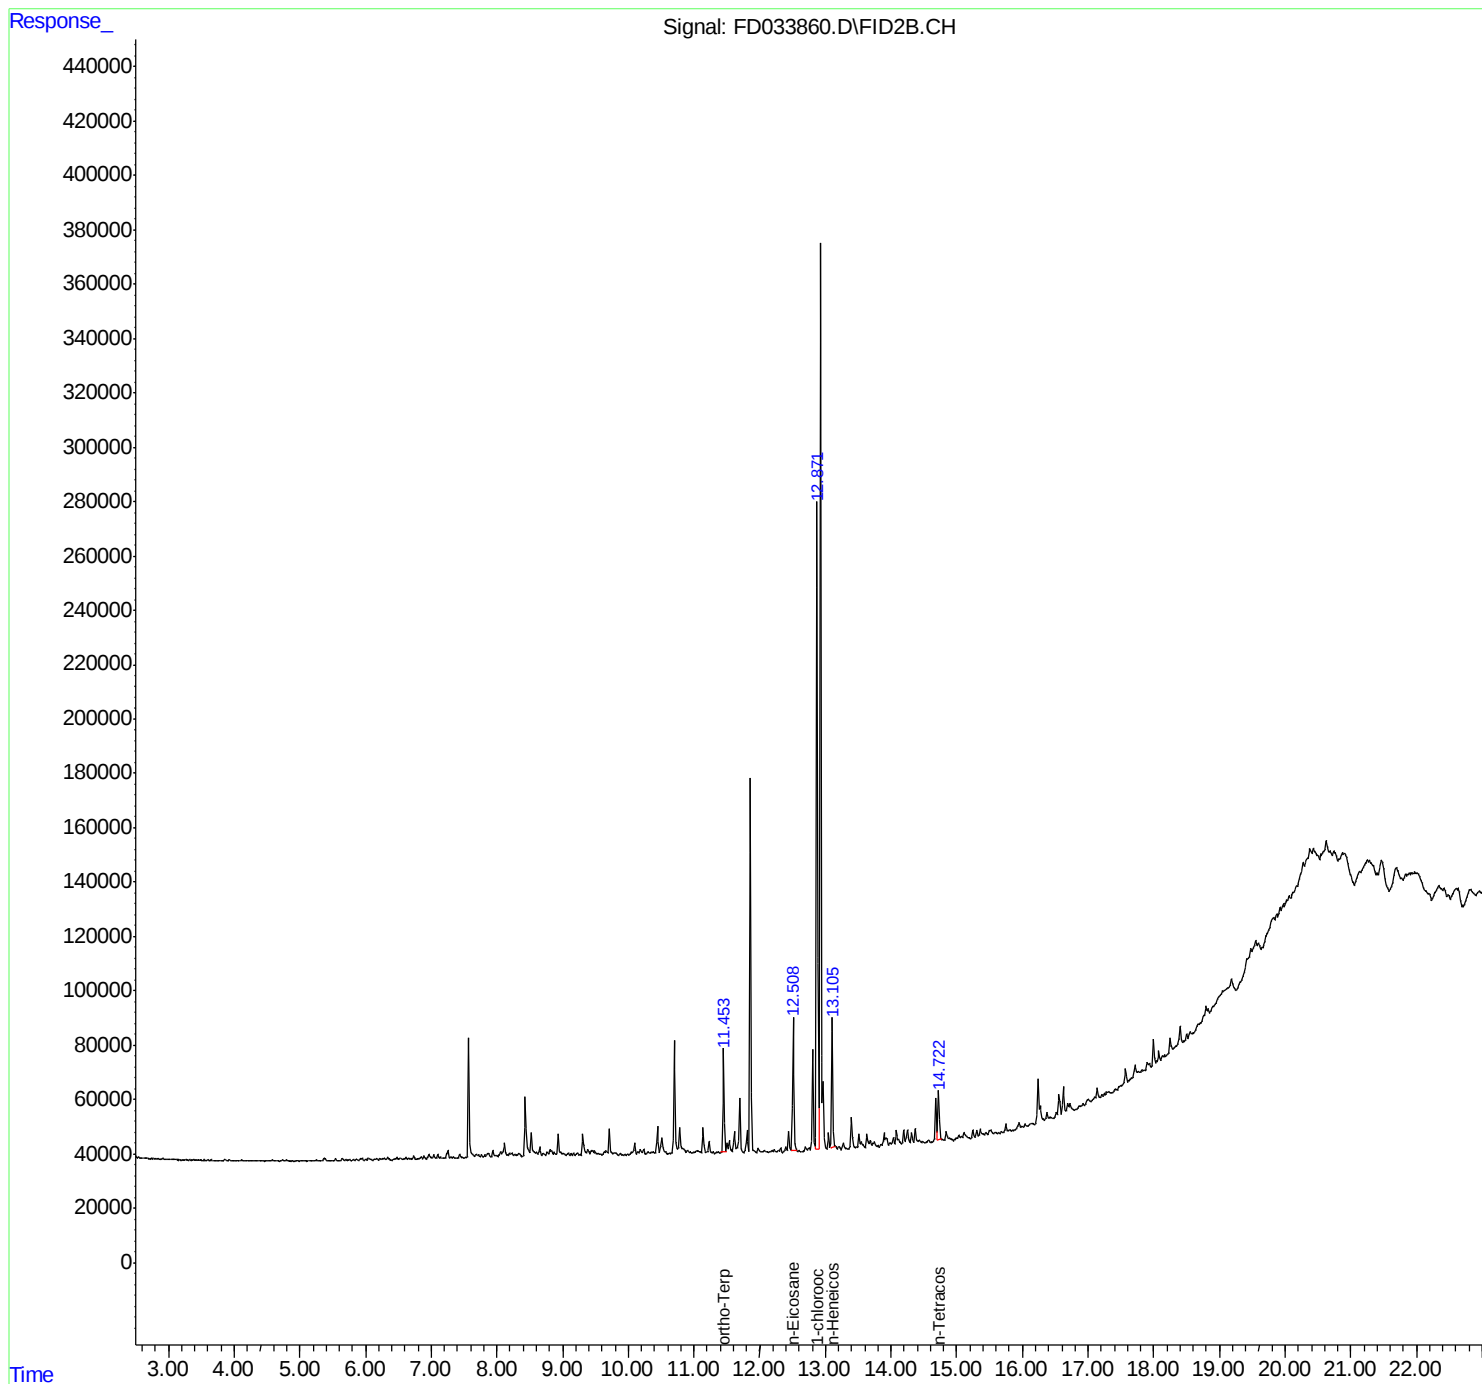


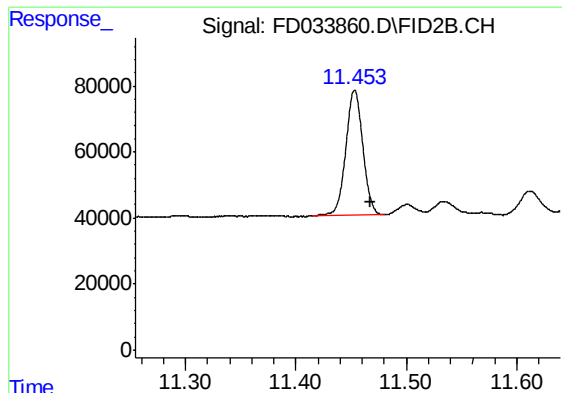

#9 ortho-Terphenyl (SURR)


R.T.: 11.453 min
Delta R.T.: -0.014 min
Response: 406338
Conc: 2.84 ug/ml

Instrument :
FID_D
ClientSampleId :
PL-02-063020-3DL

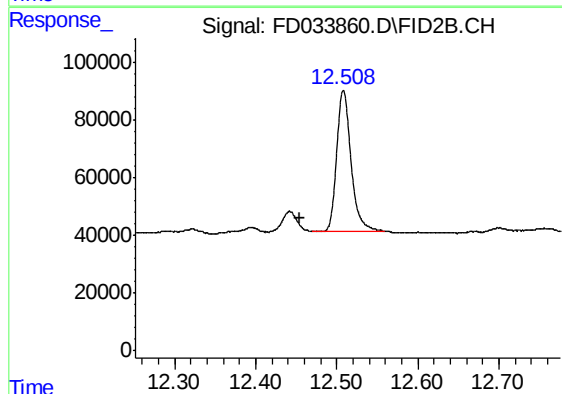


#10 n-Eicosane (C20)

R.T.: 12.508 min
Delta R.T.: 0.054 min
Response: 598834
Conc: 4.40 ug/ml

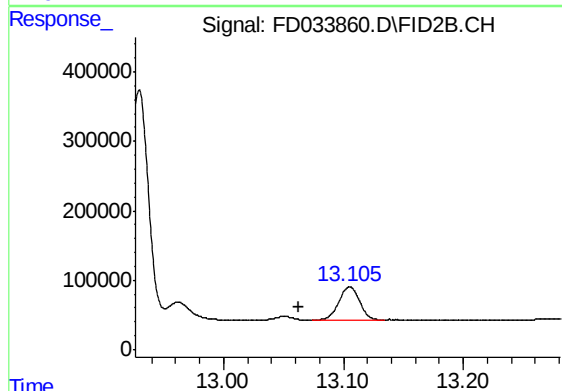


#11 n-Heneicosane (C21)

R.T.: 13.105 min
Delta R.T.: 0.043 min
Response: 573078
Conc: 4.20 ug/ml

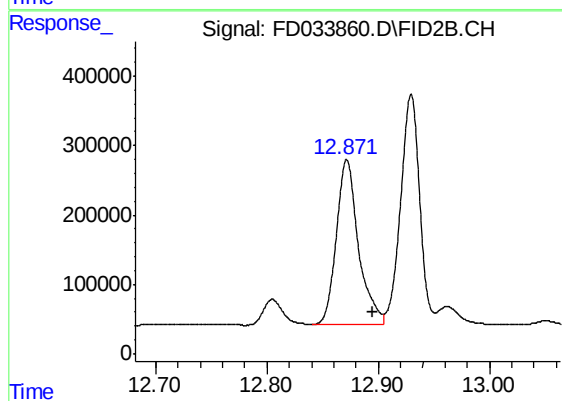

#12 1-chlorooctadecane (SURR)

R.T.: 12.872 min
Delta R.T.: -0.023 min
Response: 3290320
Conc: 27.98 ug/ml

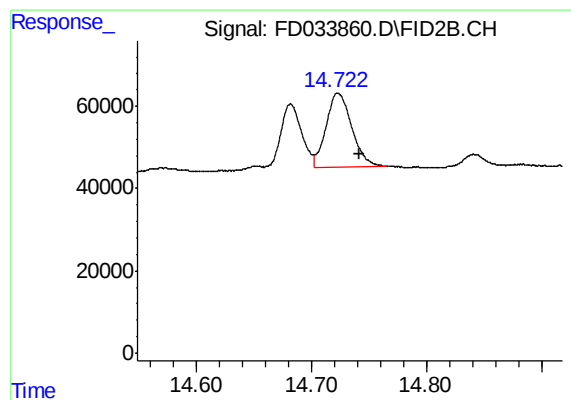

#14 n-Tetracosane (C24)

R.T.: 14.723 min
Delta R.T.: -0.019 min
Response: 276771
Conc: 2.02 ug/ml

Instrument :
FID_D
ClientSampleId :
PL-02-063020-3DL