

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD072123AL\
Data File : FD046180.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2023 22:29
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 23:28:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072023.M
Quant Title : GC Extractables
QLast Update : Thu Jul 20 14:31:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.347	317136	2.597 ug/ml
19) T	n-Tetratriacontane (C34)	19.123	204968	1.602 ug/ml
20) T	n-Hexatriacontane (C36)	19.865	1598521	13.958 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD072123AL\
Data File : FD046180.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2023 22:29
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 23:28:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072023.M
Quant Title : GC Extractables
QLast Update : Thu Jul 20 14:31:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

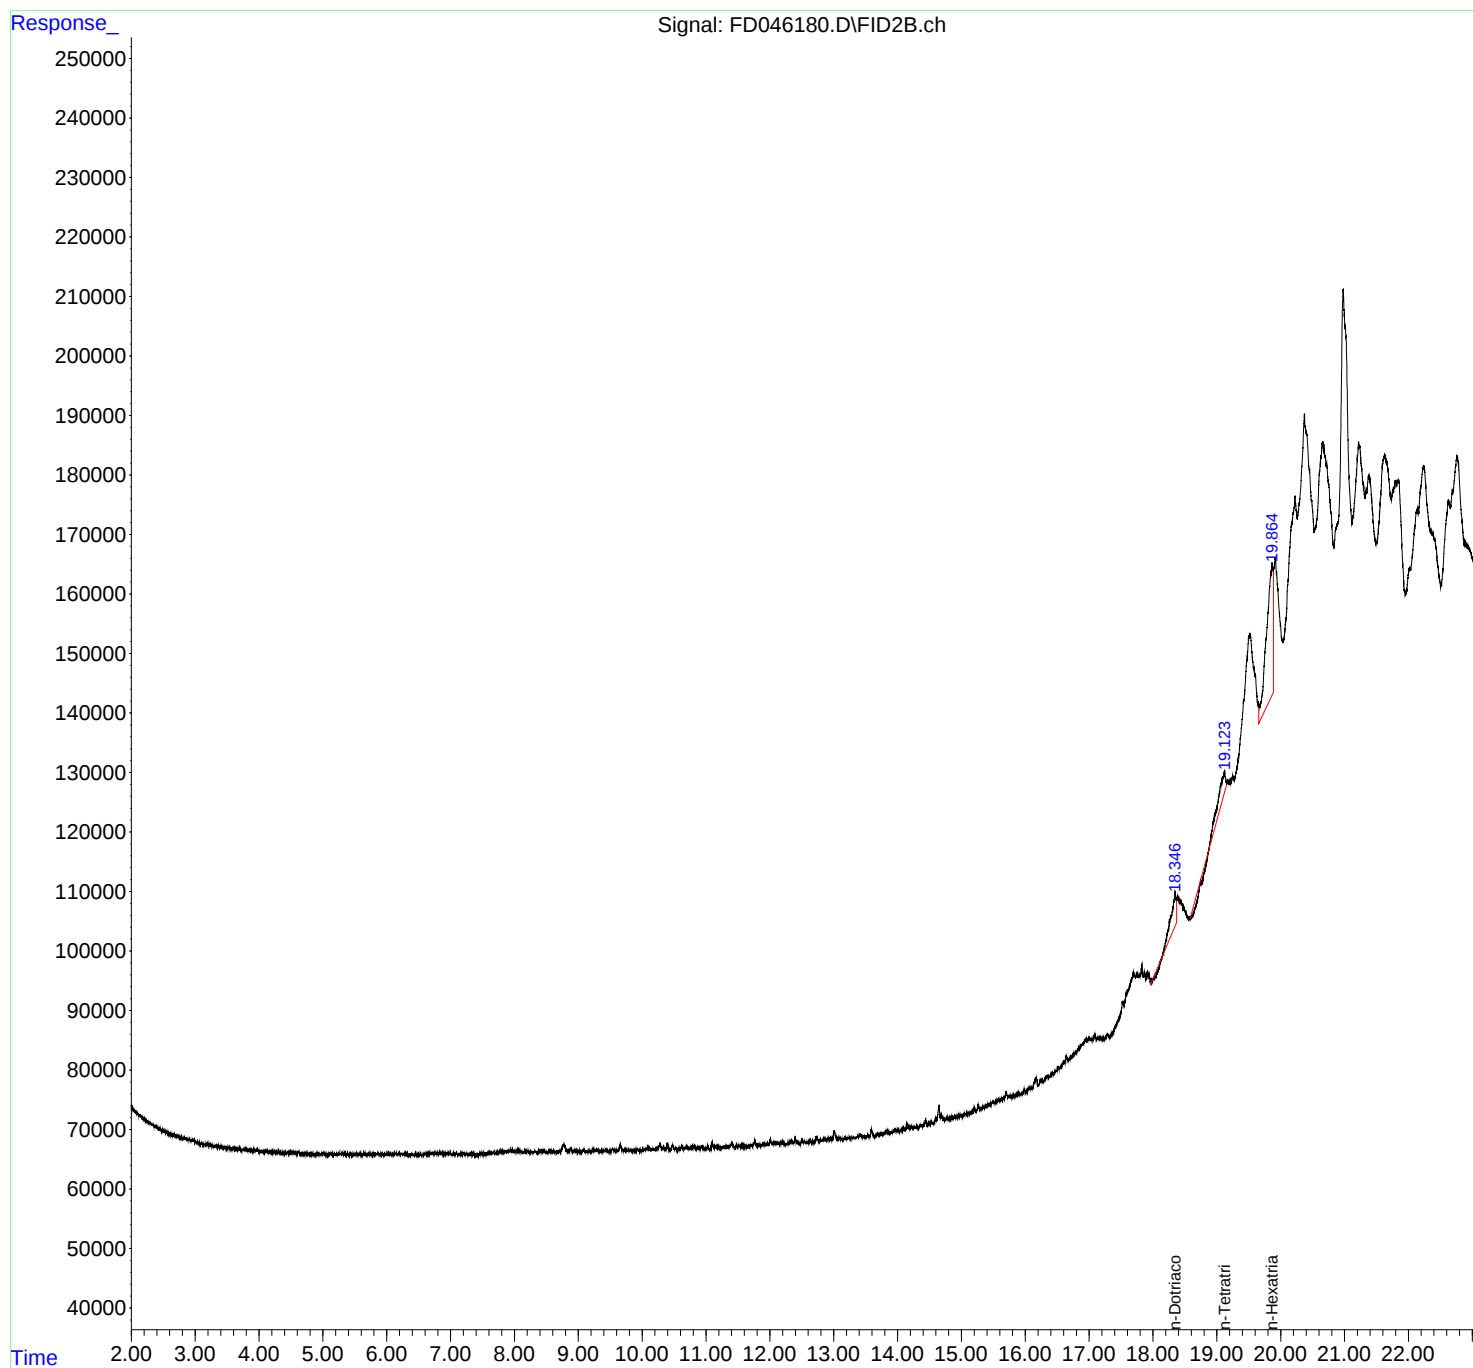


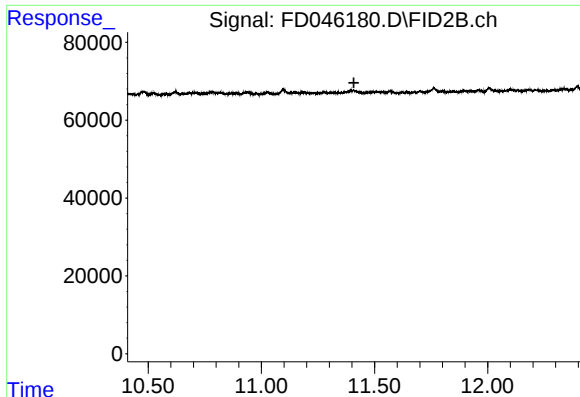

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.409 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

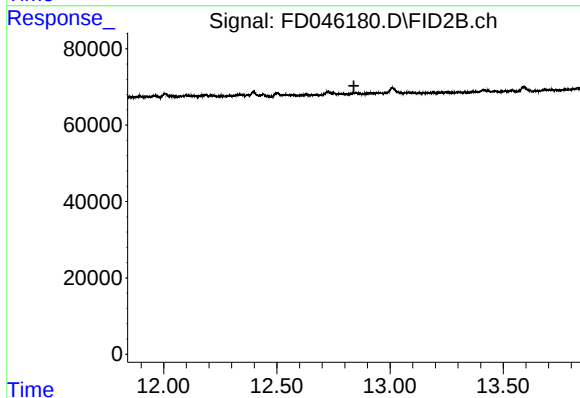


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.840 min
Response: 0
Conc: N.D.

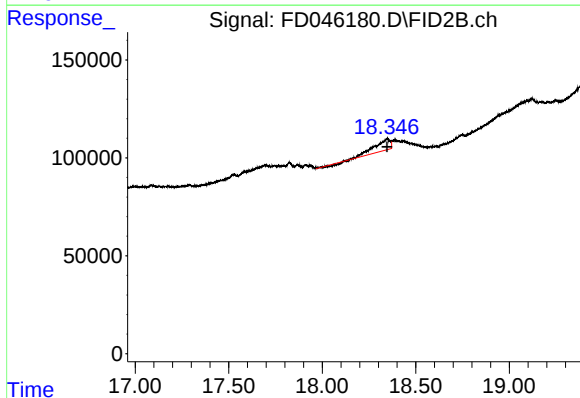


#18 n-Dotriacontane (C32)

R.T.: 18.347 min
Delta R.T.: 0.000 min
Response: 317136
Conc: 2.60 ug/ml

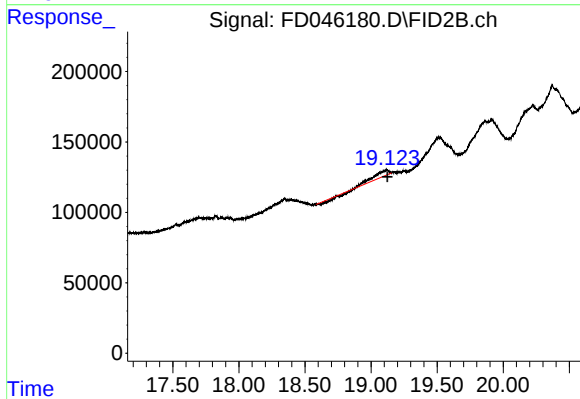

#19 n-Tetratriacontane (C34)

R.T.: 19.123 min
Delta R.T.: 0.000 min
Response: 204968
Conc: 1.60 ug/ml

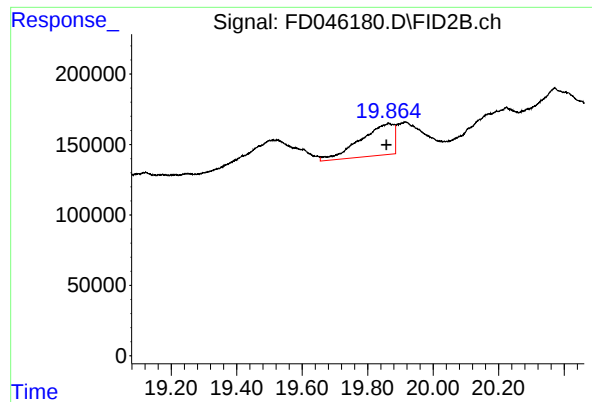

#20 n-Hexatriacontane (C36)

R.T.: 19.865 min
Delta R.T.: 0.007 min
Response: 1598521
Conc: 13.96 ug/ml

Instrument :
FID_D
ClientSampleId :