

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD072922AL\
Data File : FD043431.D
Signal(s) : FID2B.ch
Acq On : 30 Jul 2022 05:19
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 30 05:49:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:37:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.495	73116	0.529 ug/ml
20) T	n-Hexatriacontane (C36)	19.952f	130006	1.054 ug/ml
22) T	n-Tetracontane (C40)	21.629	941611	8.328 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD072922AL\
Data File : FD043431.D
Signal(s) : FID2B.ch
Acq On : 30 Jul 2022 05:19
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 30 05:49:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:37:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

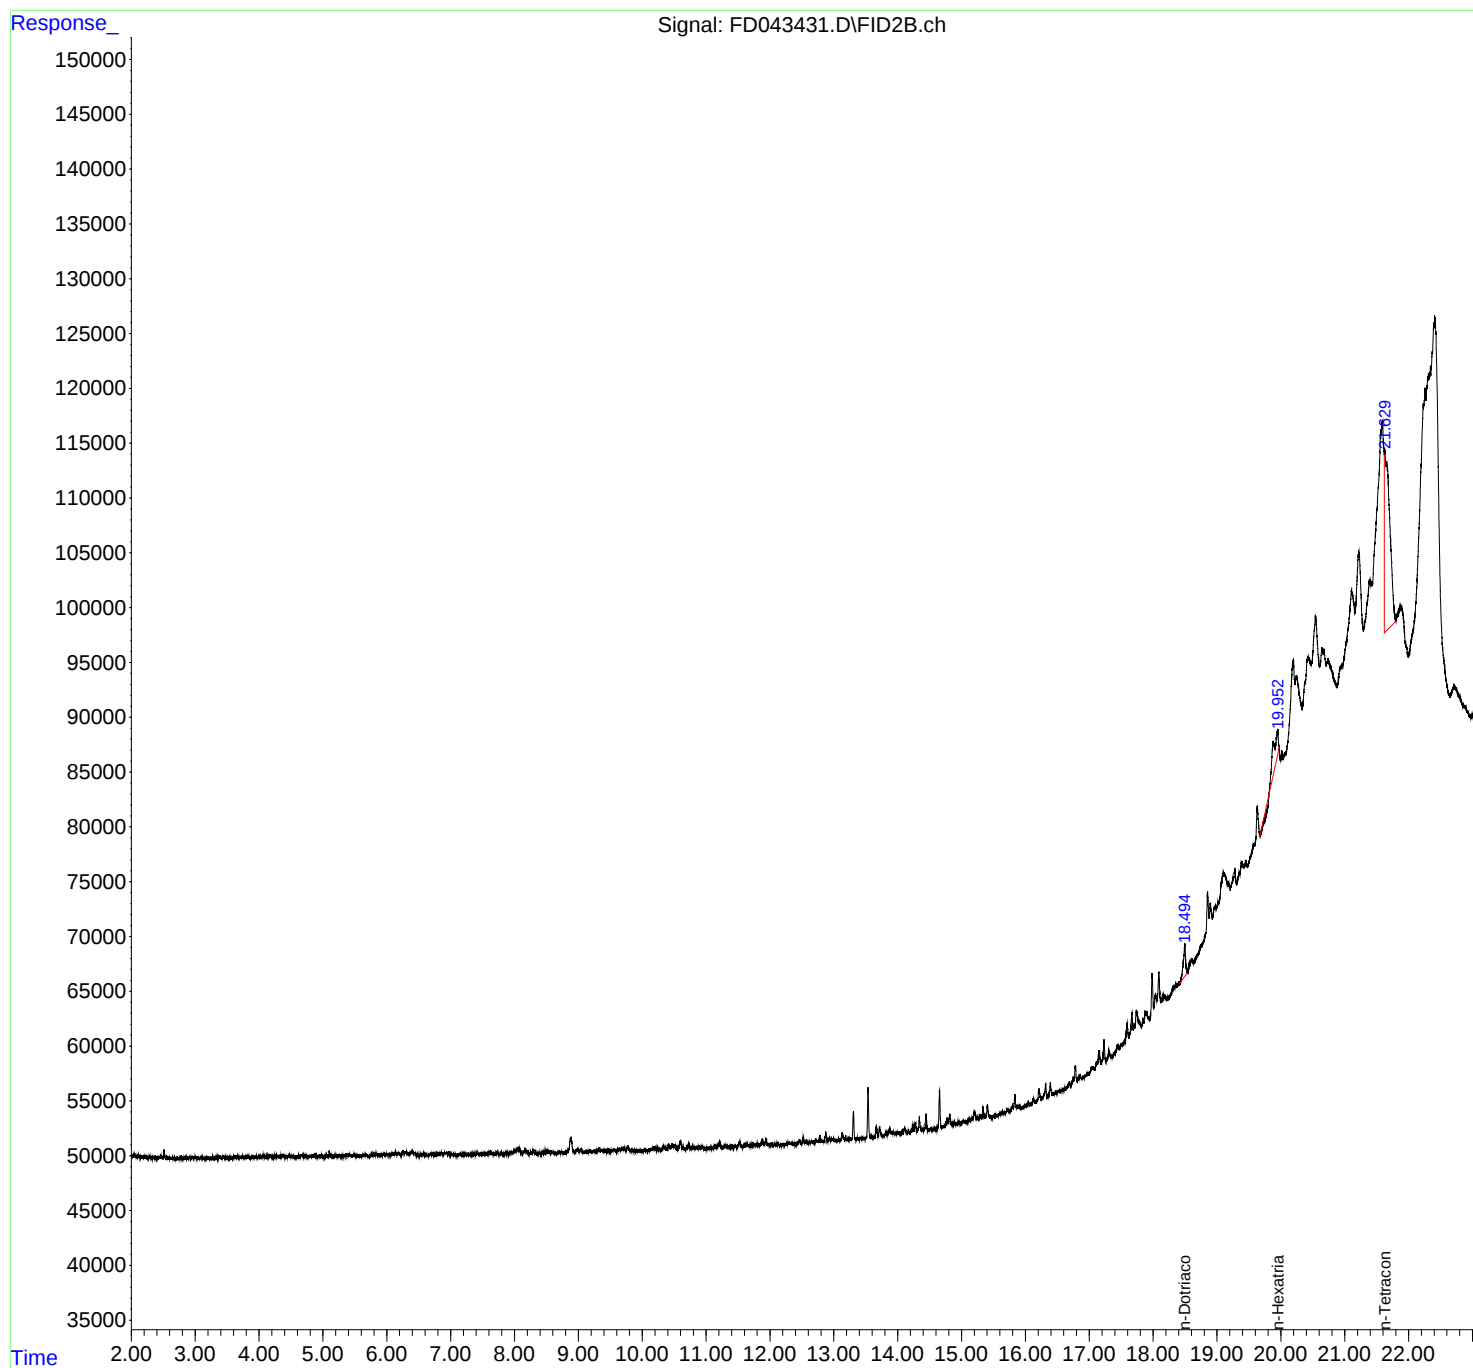


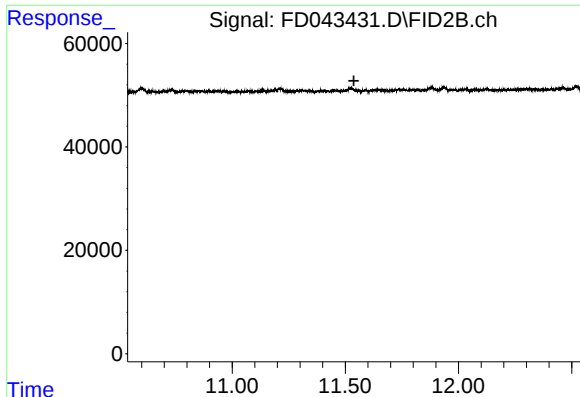

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.538 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

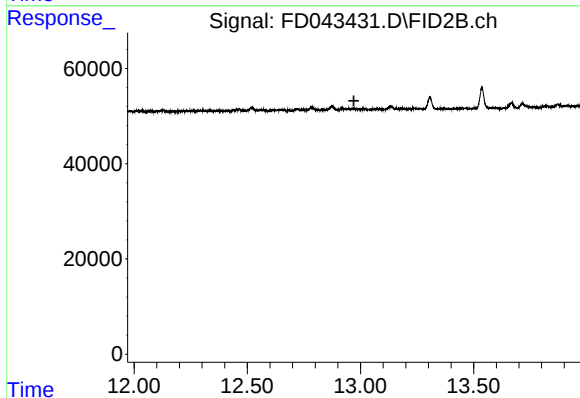


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.971 min
Response: 0
Conc: N.D.

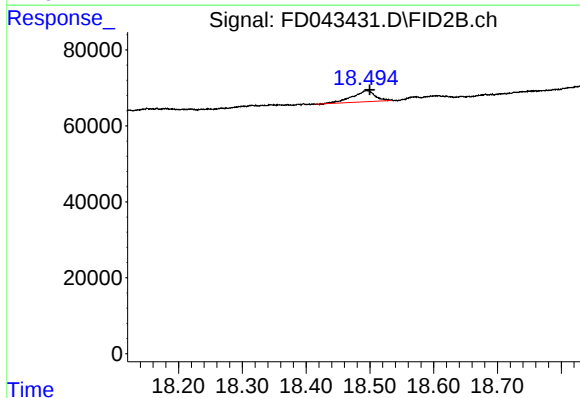


#18 n-Dotriacontane (C32)

R.T.: 18.495 min
Delta R.T.: -0.005 min
Response: 73116
Conc: 0.53 ug/ml

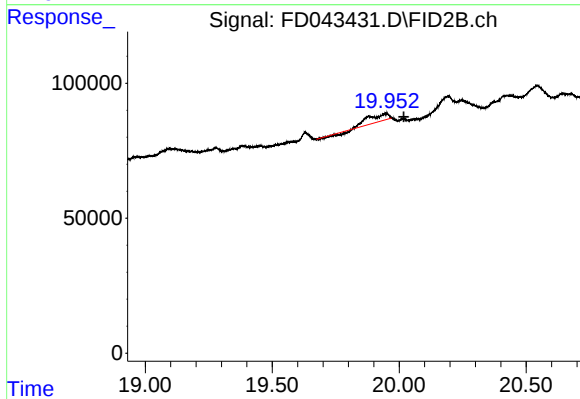

#20 n-Hexatriacontane (C36)

R.T.: 19.952 min
Delta R.T.: -0.066 min
Response: 130006
Conc: 1.05 ug/ml

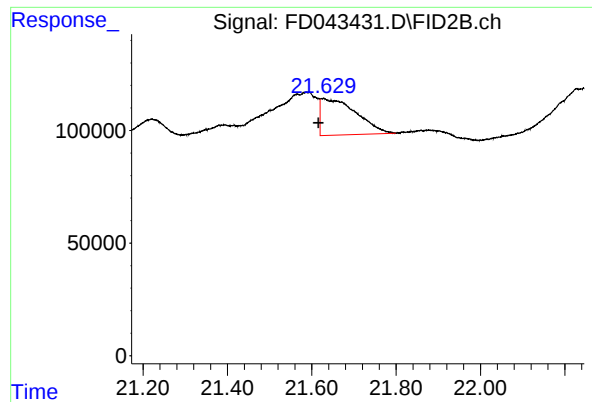

#22 n-Tetracontane (C40)

R.T.: 21.629 min
Delta R.T.: 0.012 min
Response: 941611
Conc: 8.33 ug/ml

Instrument :
FID_D
ClientSampleId :