

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD080122AL\
 Data File : FD043458.D
 Signal(s) : FID2B.ch
 Acq On : 02 Aug 2022 05:12
 Operator : YP/AJ
 Sample : N3970-04
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 07:11:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:37:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.530	3879664	24.509 ug/ml
Spiked Amount 50.000		Recovery =	49.02%
12) S 1-chlorooctadecane (S...	12.967	3072569	25.070 ug/ml
Spiked Amount 50.000		Recovery =	50.14%
Target Compounds			
10) T n-Eicosane (C20)	12.574	90193	0.623 ug/ml
14) T n-Tetracosane (C24)	14.785	34277	0.237 ug/ml
16) T n-Octacosane (C28)	16.782	46073	0.326 ug/ml
17) T n-Tricontane (C30)	17.666	61171	0.433 ug/ml
18) T n-Dotriacontane (C32)	18.496	62586	0.453 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD080122AL\
Data File : FD043458.D
Signal(s) : FID2B.ch
Acq On : 02 Aug 2022 05:12
Operator : YP/AJ
Sample : N3970-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 07:11:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:37:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

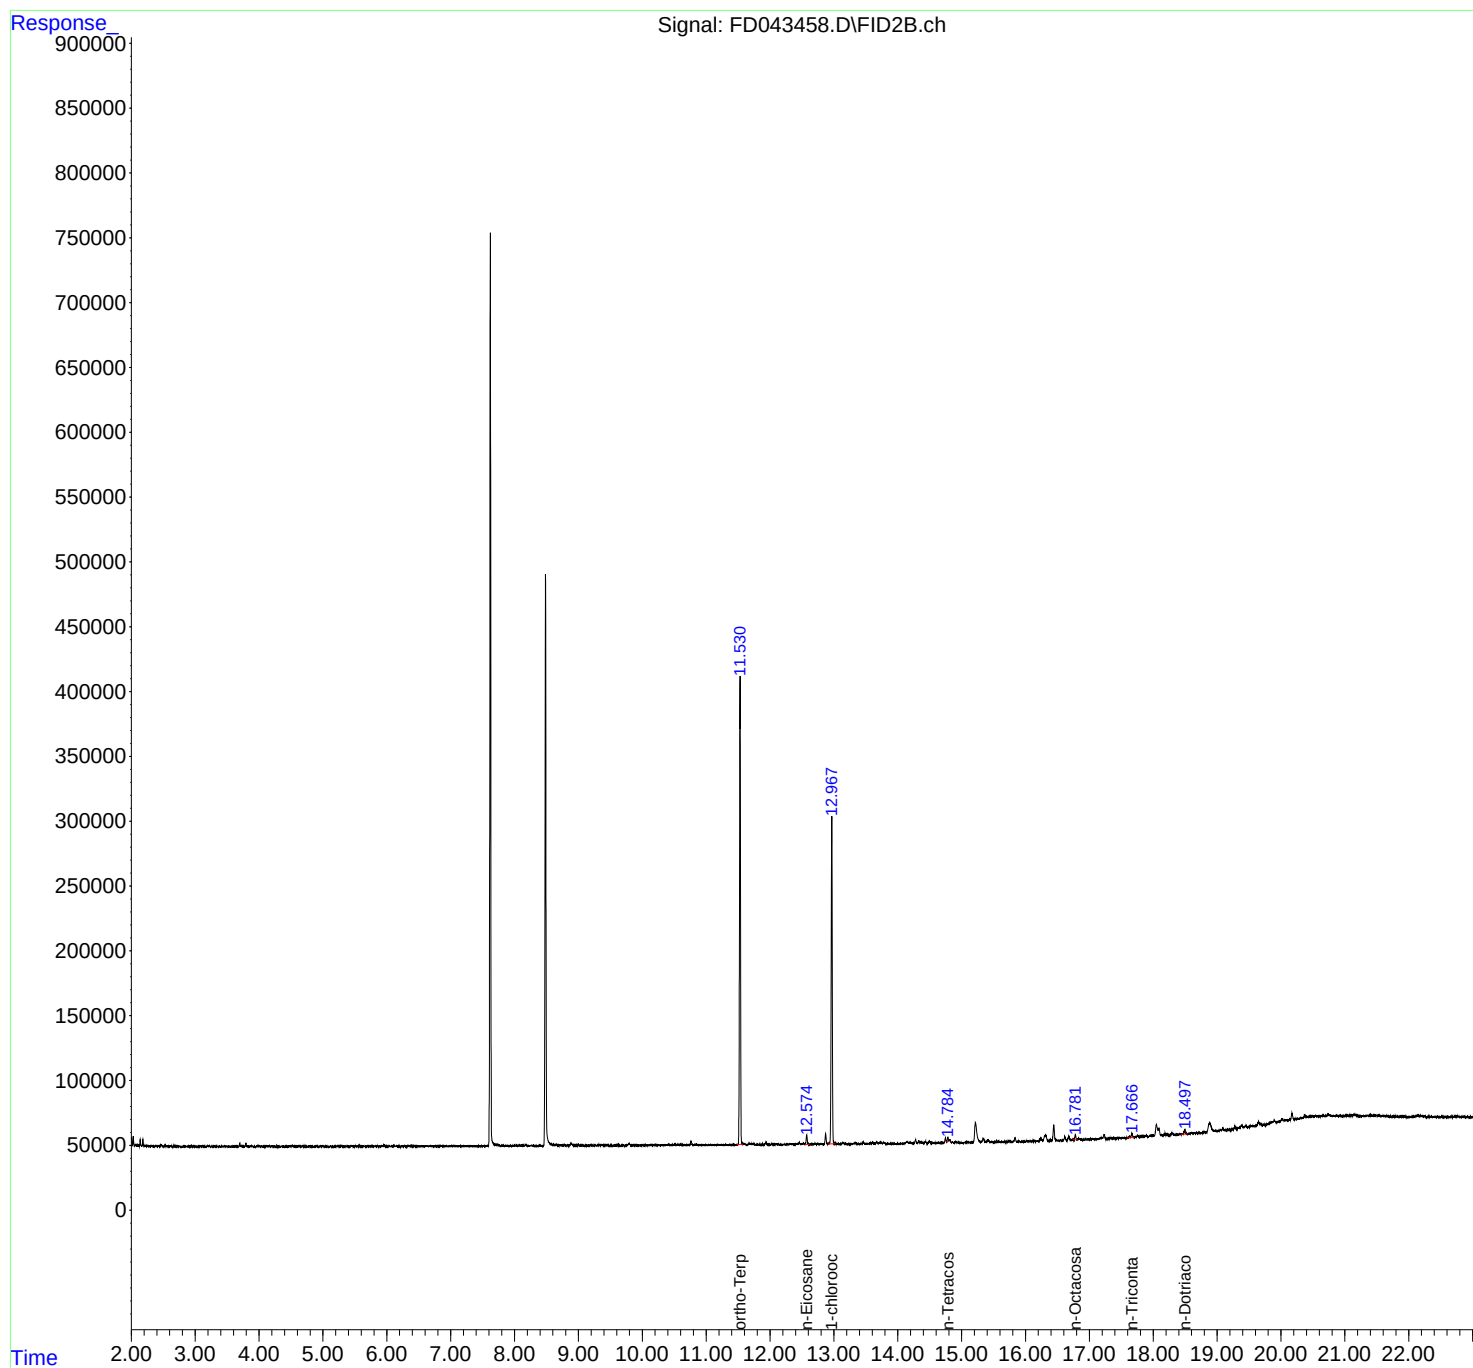


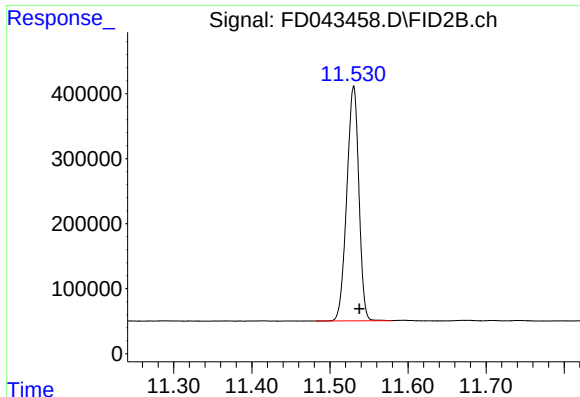

#9 ortho-Terphenyl (SURR)


R.T.: 11.530 min
Delta R.T.: -0.007 min
Response: 3879664
Conc: 24.51 ug/ml

Instrument :
FID_D
ClientSampleId :

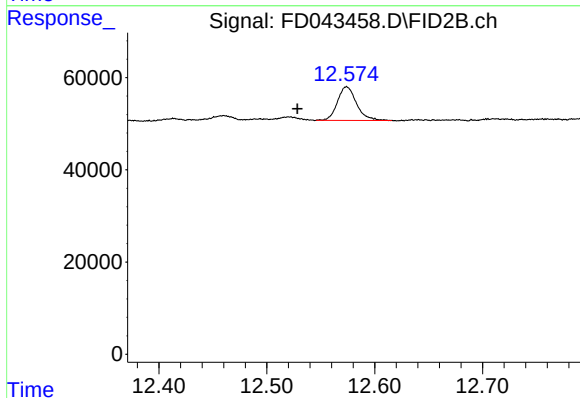


#10 n-Eicosane (C20)

R.T.: 12.574 min
Delta R.T.: 0.046 min
Response: 90193
Conc: 0.62 ug/ml

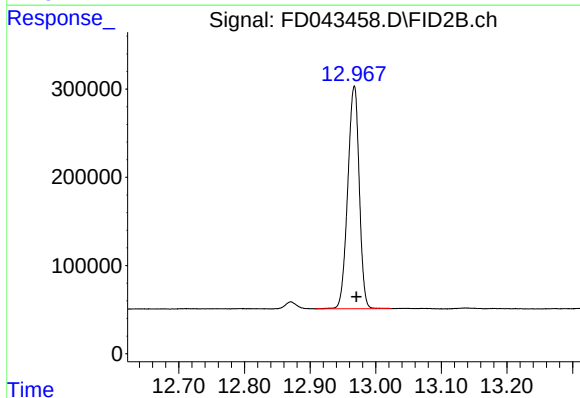


#12 1-chlorooctadecane (SURR)

R.T.: 12.967 min
Delta R.T.: -0.003 min
Response: 3072569
Conc: 25.07 ug/ml

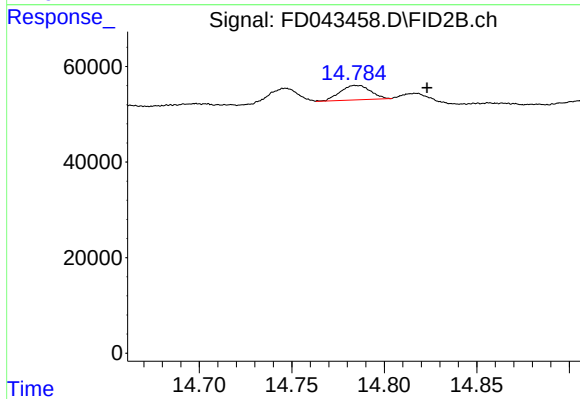

#14 n-Tetracosane (C24)


R.T.: 14.785 min
Delta R.T.: -0.038 min
Response: 34277
Conc: 0.24 ug/ml

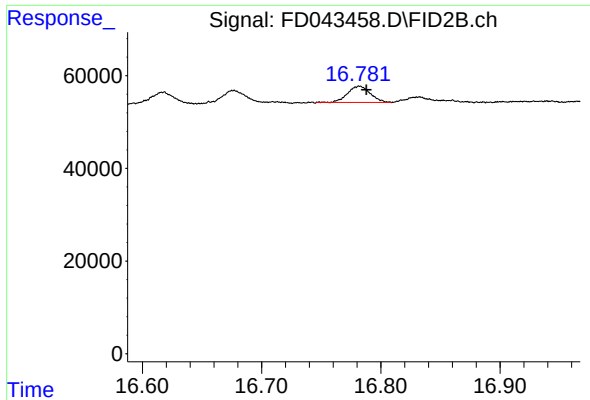

#16 n-Octacosane (C28)


R.T.: 16.782 min
Delta R.T.: -0.006 min
Response: 46073
Conc: 0.33 ug/ml

Instrument :
FID_D
ClientSampleId :

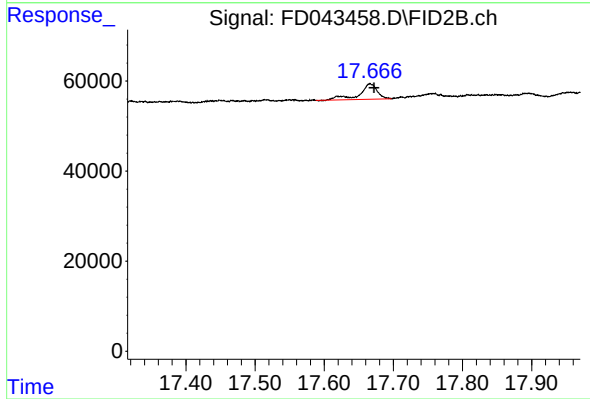

#17 n-Tricontane (C30)

R.T.: 17.666 min
Delta R.T.: -0.006 min
Response: 61171
Conc: 0.43 ug/ml

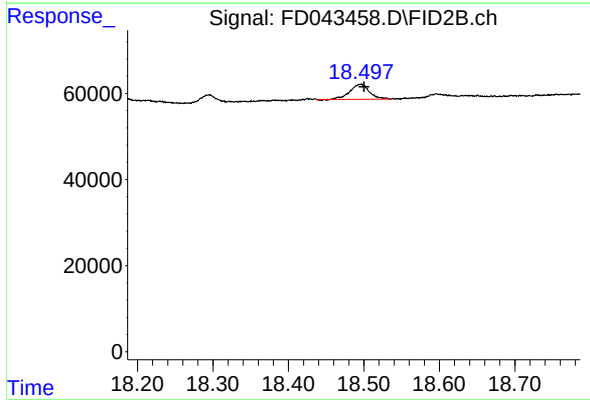

#18 n-Dotriacontane (C32)

R.T.: 18.496 min
Delta R.T.: -0.004 min
Response: 62586
Conc: 0.45 ug/ml