

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD080923AL\
 Data File : FD046311.D
 Signal(s) : FID2B.ch
 Acq On : 09 Aug 2023 12:13
 Operator : YP/AJ
 Sample : PB154615BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 09 23:59:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072023.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 20 14:31:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.830	6482415	53.874 ug/ml
Spiked Amount 50.000		Recovery =	107.75%
Target Compounds			
14) T n-Tetracosane (C24)	14.671	82363	0.598 ug/ml
15) T n-Hexacosane (C26)	15.684	130166	1.018 ug/ml
16) T n-Octacosane (C28)	16.626	187414	1.539 ug/ml
17) T n-Tricontane (C30)	17.506	250469	2.024 ug/ml
18) T n-Dotriacontane (C32)	18.332	268563	2.199 ug/ml
19) T n-Tetratriacontane (C34)	19.110	213869	1.672 ug/ml
20) T n-Hexatriacontane (C36)	19.842	88356	0.772 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD080923AL\
Data File : FD046311.D
Signal(s) : FID2B.ch
Acq On : 09 Aug 2023 12:13
Operator : YP/AJ
Sample : PB154615BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 09 23:59:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072023.M
Quant Title : GC Extractables
QLast Update : Thu Jul 20 14:31:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

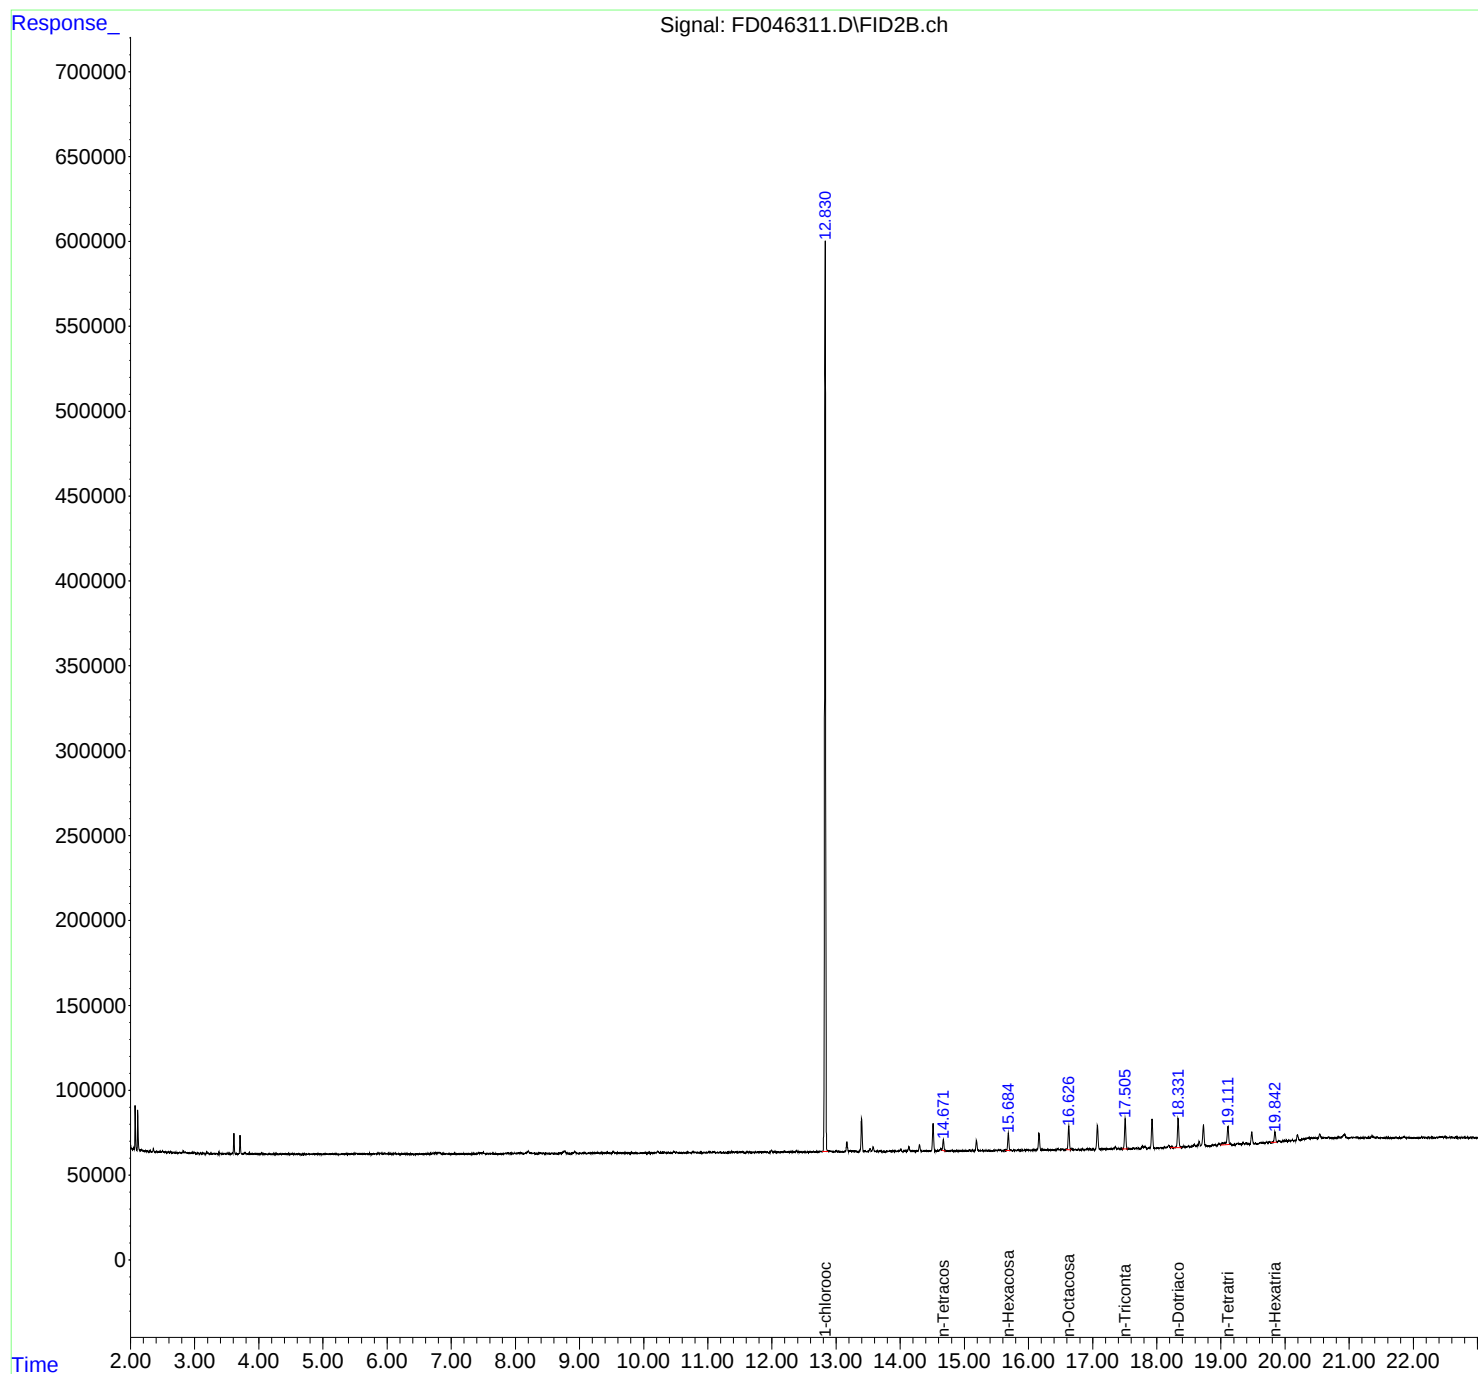


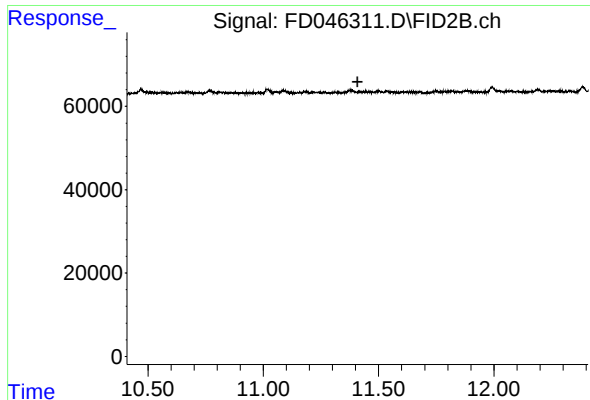

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.409 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

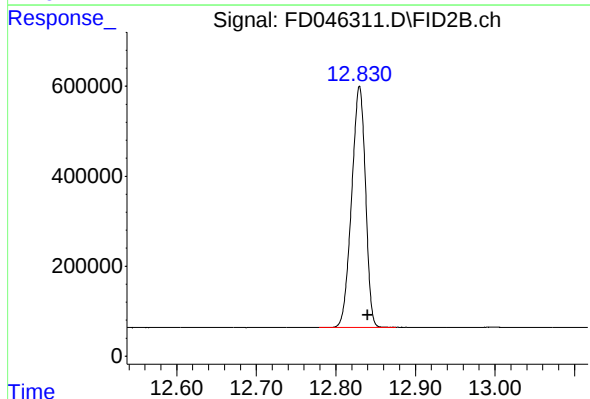


#12 1-chlorooctadecane (SURR)

R.T.: 12.830 min
Delta R.T.: -0.010 min
Response: 6482415
Conc: 53.87 ug/ml

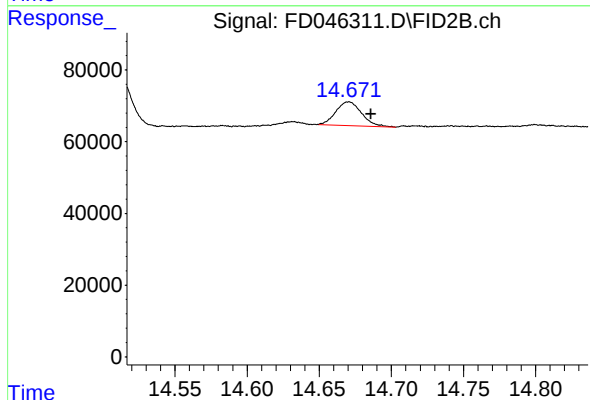


#14 n-Tetracosane (C24)

R.T.: 14.671 min
Delta R.T.: -0.015 min
Response: 82363
Conc: 0.60 ug/ml

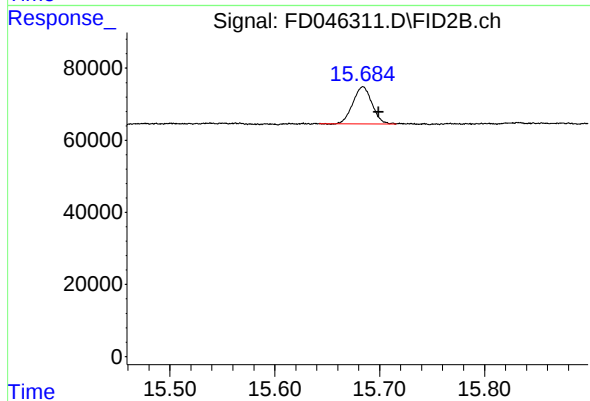

#15 n-Hexacosane (C26)


R.T.: 15.684 min
Delta R.T.: -0.015 min
Response: 130166
Conc: 1.02 ug/ml

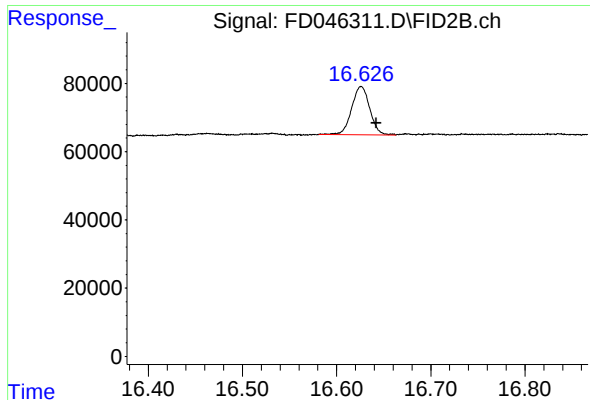

#16 n-Octacosane (C28)


R.T.: 16.626 min
Delta R.T.: -0.016 min
Response: 187414
Conc: 1.54 ug/ml

Instrument :
FID_D
ClientSampleId :

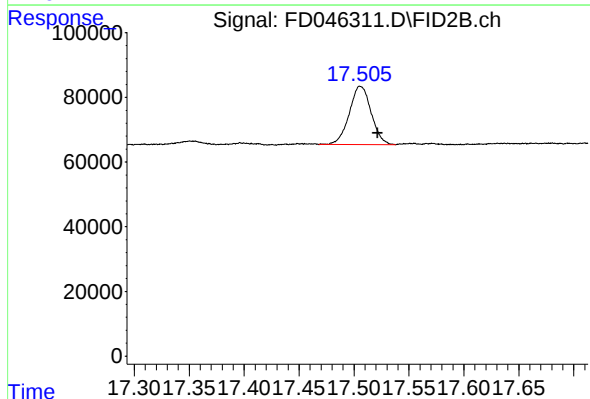


#17 n-Tricontane (C30)

R.T.: 17.506 min
Delta R.T.: -0.016 min
Response: 250469
Conc: 2.02 ug/ml

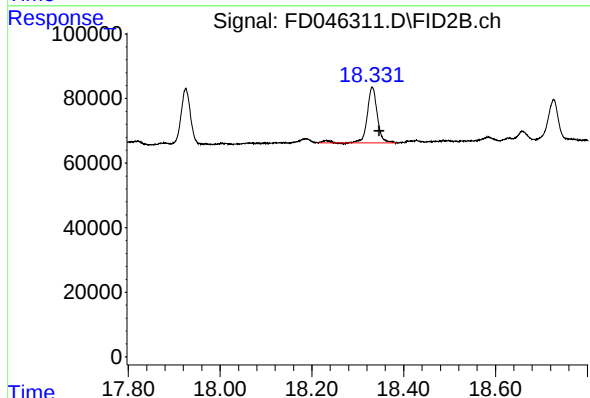


#18 n-Dotriacontane (C32)

R.T.: 18.332 min
Delta R.T.: -0.015 min
Response: 268563
Conc: 2.20 ug/ml

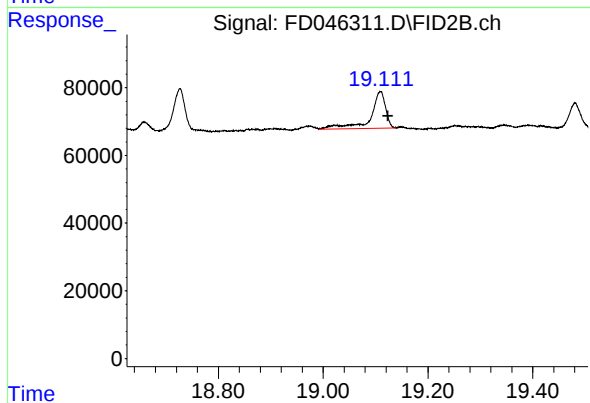

#19 n-Tetratriacontane (C34)

R.T.: 19.110 min
Delta R.T.: -0.014 min
Response: 213869
Conc: 1.67 ug/ml

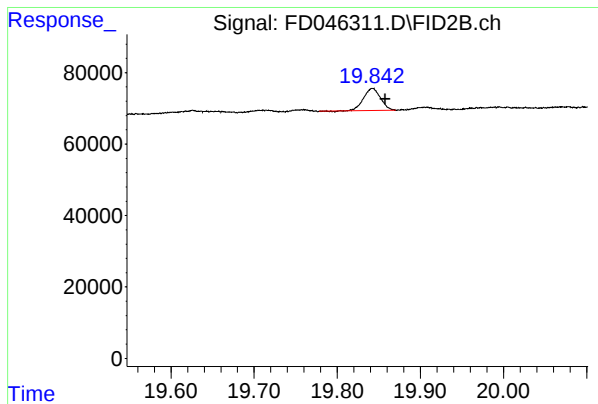

#20 n-Hexatriacontane (C36)

R.T.: 19.842 min
Delta R.T.: -0.015 min
Response: 88356
Conc: 0.77 ug/ml

Instrument :

FID_D

ClientSampleId :