

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD081621AL\
 Data File : FD038563.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2021 13:44
 Operator : AJ\MA
 Sample : M3404-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 TP1-1-6FT

Integration File: autoint1.e
 Quant Time: Aug 17 03:49:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 080321.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 04 03:20:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.368	6903749	50.576 ug/ml
Spiked Amount 50.000		Recovery =	101.15%
12) S 1-chlorooctadecane (S...	12.804	5485571	51.012 ug/ml
Spiked Amount 50.000		Recovery =	102.02%
Target Compounds			
3) T A~Naphthalene (C11.7)	5.877f	207025	1.586 ug/ml
6) T n-Tetradecane (C14)	7.999	121241	0.998 ug/ml
10) T n-Eicosane (C20)	12.408	721136	5.721 ug/ml
14) T n-Tetracosane (C24)	14.618	366556	2.850 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD081621AL\
Data File : FD038563.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2021 13:44
Operator : AJ\MA
Sample : M3404-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
TP1-1-6FT

Integration File: autoint1.e
Quant Time: Aug 17 03:49:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 080321.M
Quant Title : GC Extractables
QLast Update : Wed Aug 04 03:20:37 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

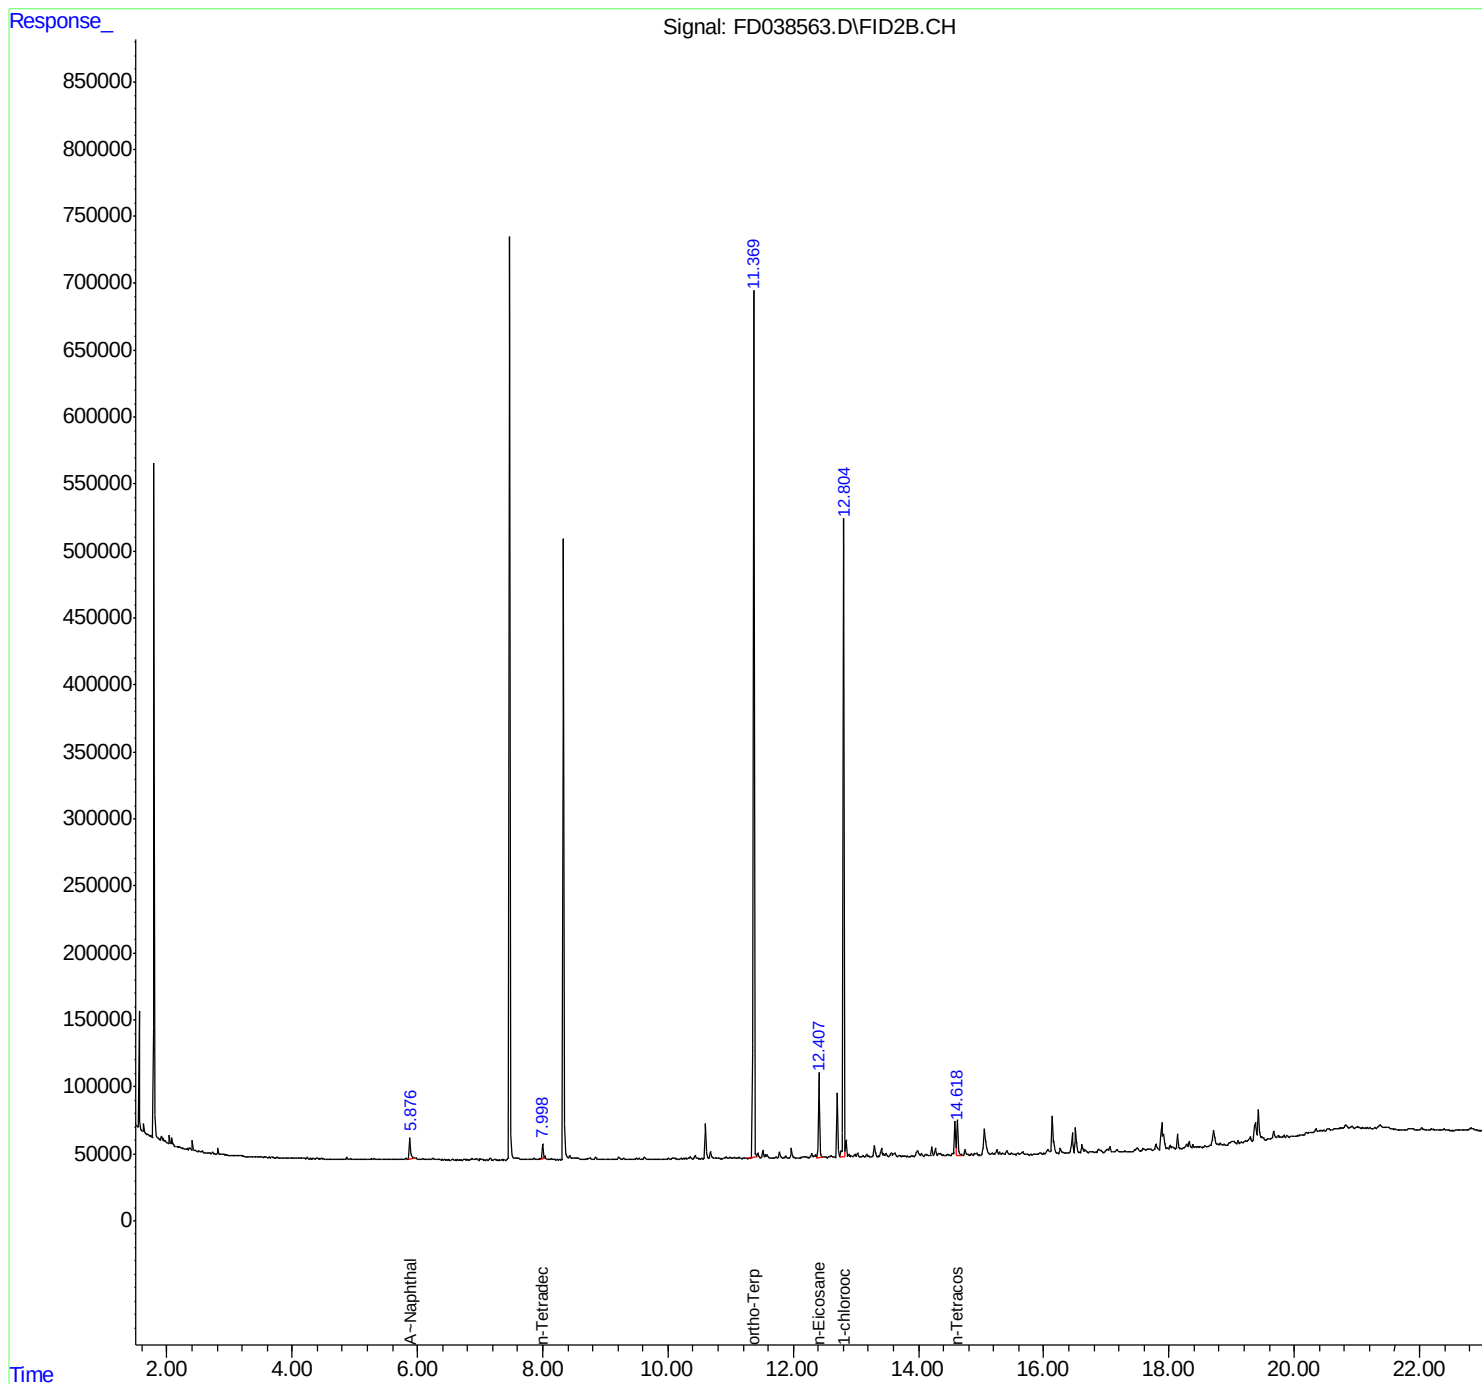


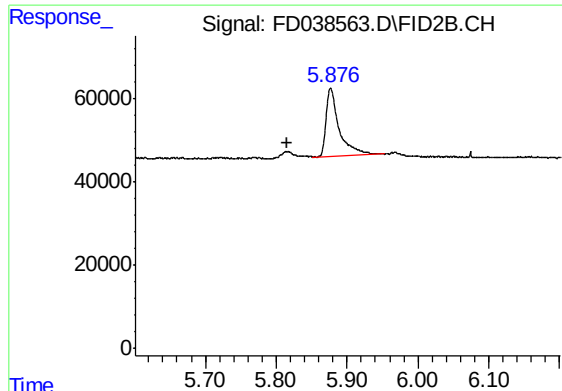

#3 A~Naphthalene (C11.7)


R.T.: 5.877 min
Delta R.T.: 0.062 min
Response: 207025
Conc: 1.59 ug/ml

Instrument :
FID_D
ClientSampleId :
TP1-1-6FT

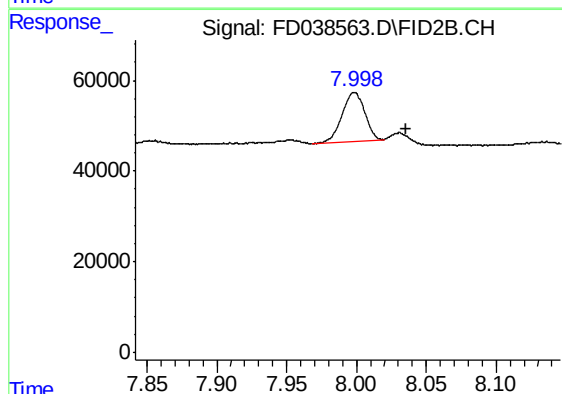


#6 n-Tetradecane (C14)

R.T.: 7.999 min
Delta R.T.: -0.037 min
Response: 121241
Conc: 1.00 ug/ml

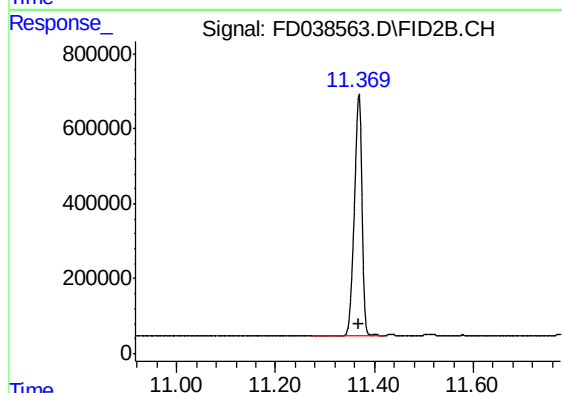


#9 ortho-Terphenyl (SURR)

R.T.: 11.368 min
Delta R.T.: 0.000 min
Response: 6903749
Conc: 50.58 ug/ml

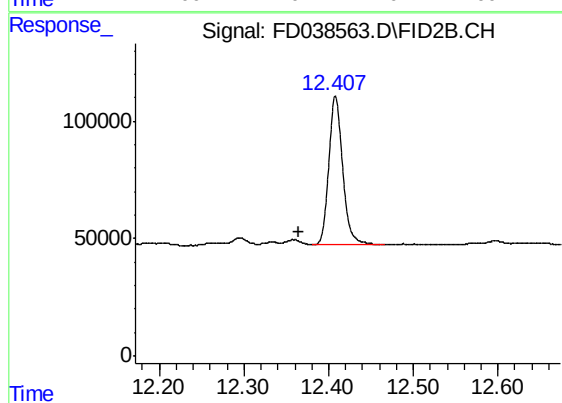

#10 n-Eicosane (C20)


R.T.: 12.408 min
Delta R.T.: 0.044 min
Response: 721136
Conc: 5.72 ug/ml

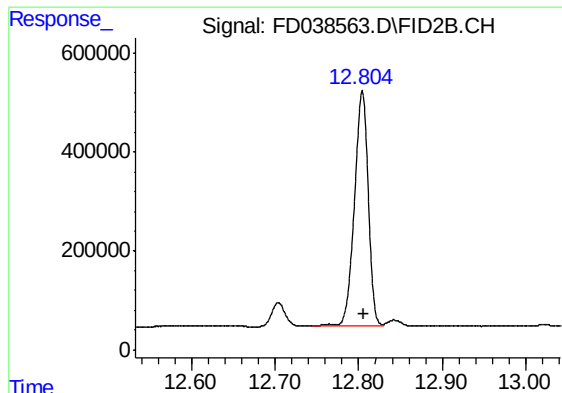

#12 1-chlorooctadecane (SURR)

R.T.: 12.804 min
Delta R.T.: -0.002 min
Response: 5485571
Conc: 51.01 ug/ml

Instrument :
FID_D
ClientSampleId :
TP1-1-6FT

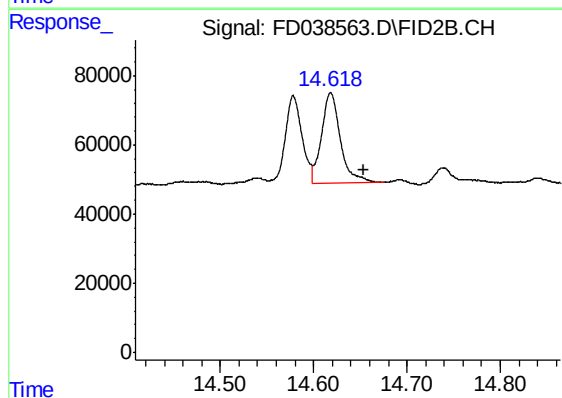

#14 n-Tetracosane (C24)

R.T.: 14.618 min
Delta R.T.: -0.036 min
Response: 366556
Conc: 2.85 ug/ml