

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD081822AL\
Data File : FD043659.D
Signal(s) : FID2B.ch
Acq On : 18 Aug 2022 17:19
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 18:47:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:37:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.270	21362	0.166 ug/ml
21) T	n-Octatriacontane (C38)	20.721	556046	4.702 ug/ml
22) T	n-Tetracontane (C40)	21.649	142103	1.257 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD081822AL\
Data File : FD043659.D
Signal(s) : FID2B.ch
Acq On : 18 Aug 2022 17:19
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 18:47:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:37:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

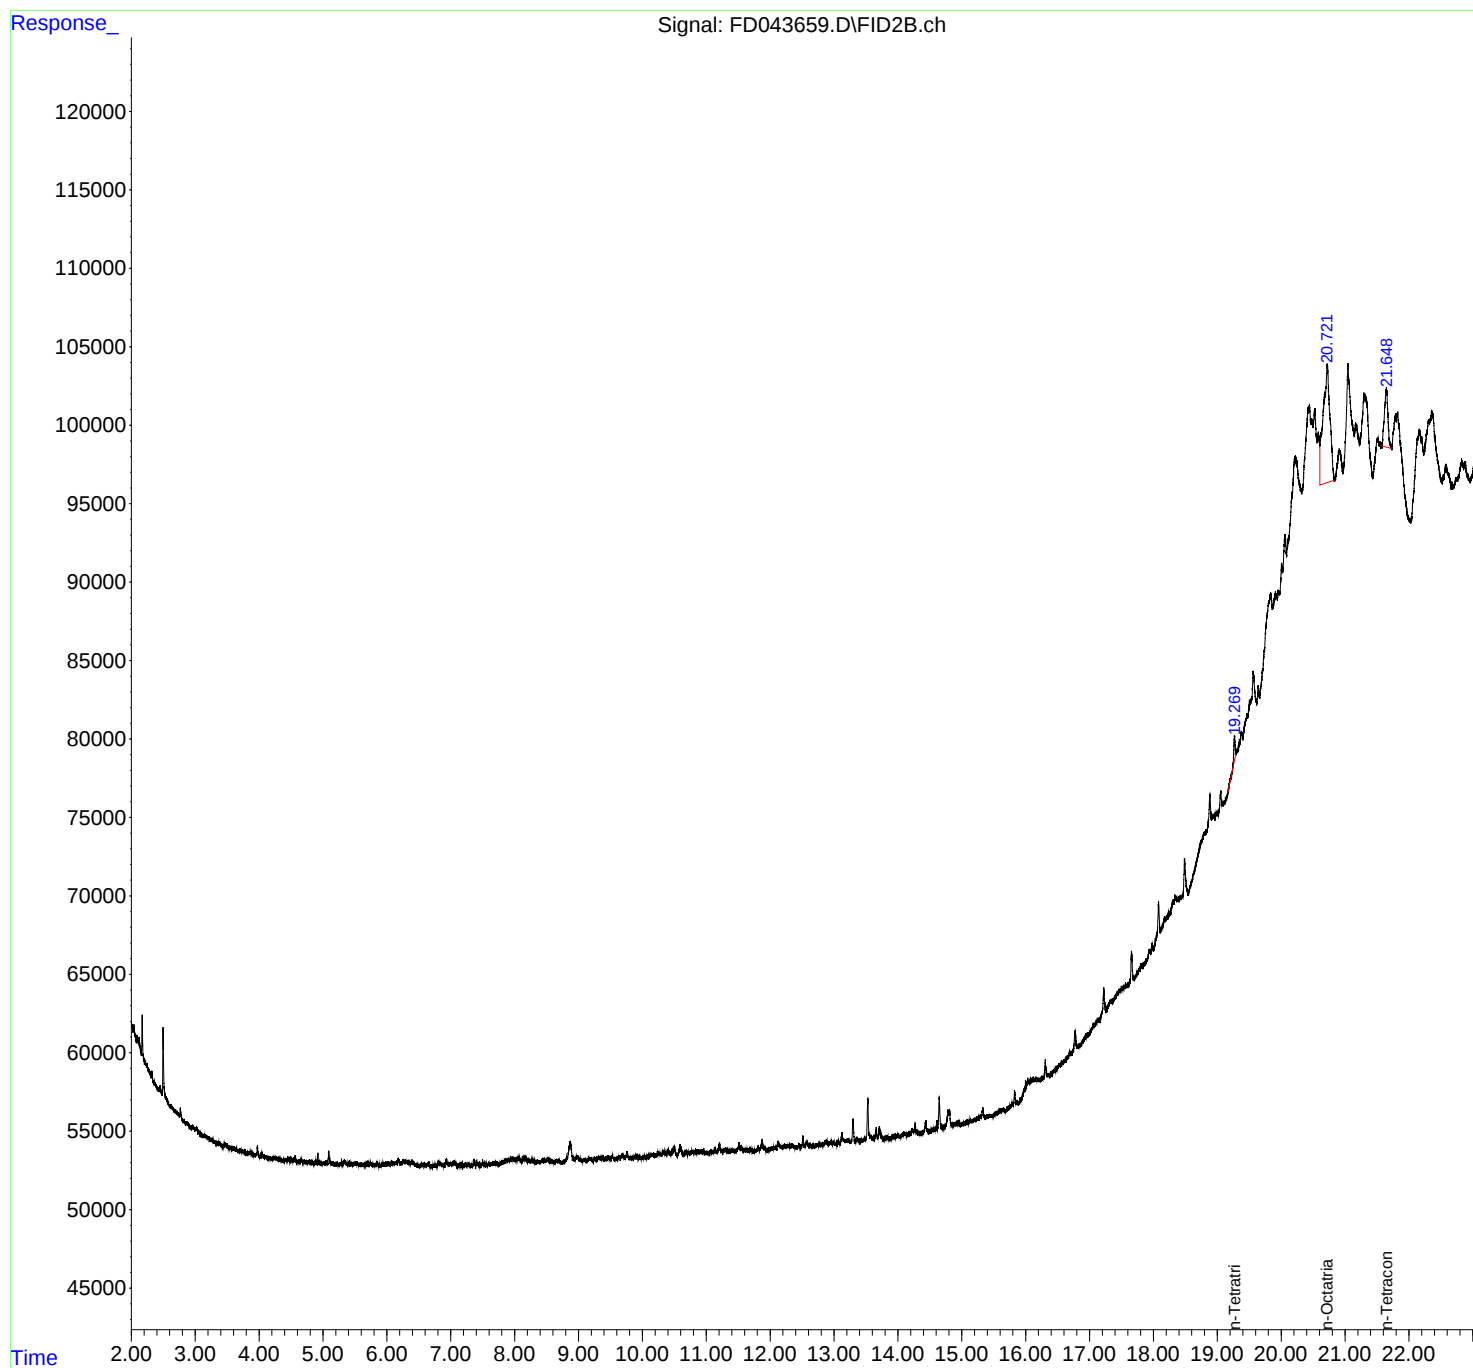


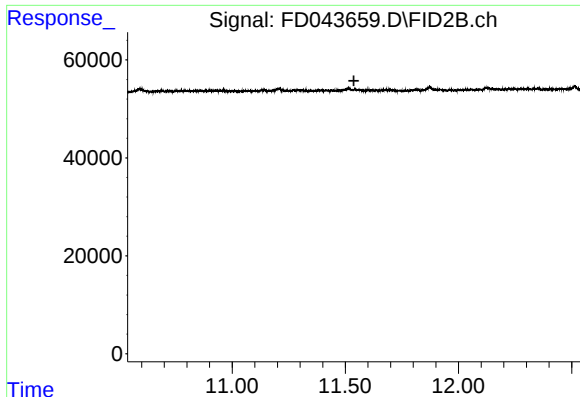

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.538 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

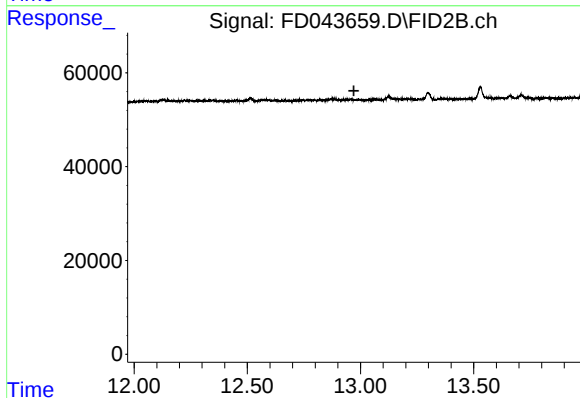


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.971 min
Response: 0
Conc: N.D.

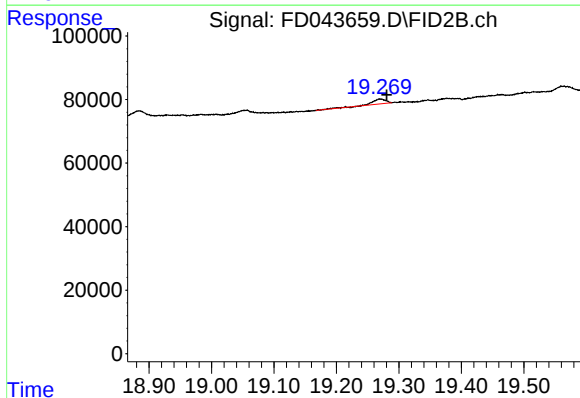


#19 n-Tetratriacontane (C34)

R.T.: 19.270 min
Delta R.T.: -0.011 min
Response: 21362
Conc: 0.17 ug/ml

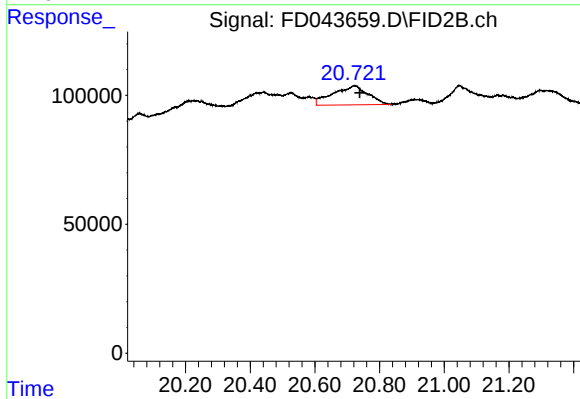

#21 n-Octatriacontane (C38)

R.T.: 20.721 min
Delta R.T.: -0.017 min
Response: 556046
Conc: 4.70 ug/ml

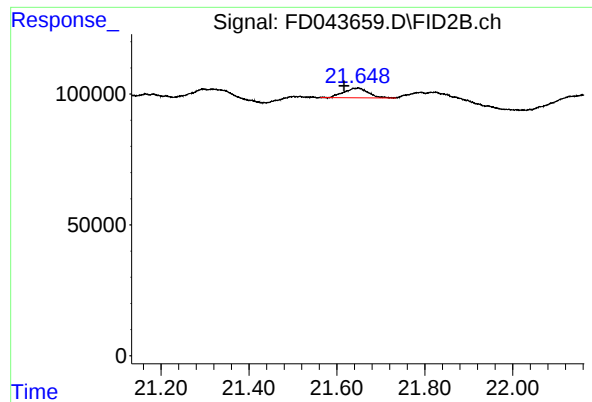

#22 n-Tetracontane (C40)

R.T.: 21.649 min
Delta R.T.: 0.033 min
Response: 142103
Conc: 1.26 ug/ml

Instrument :

FID_D

ClientSampleId :