

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD082520AL\
 Data File : FD034521.D
 Signal(s) : FID2B.CH
 Acq On : 25 Aug 2020 18:36
 Operator : DD\AJ
 Sample : L3784-10
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 RO-24

Integration File: autoint1.e
 Quant Time: Aug 26 02:36:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 073120.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 03 10:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.603	3937651	30.038 ug/ml
Spiked Amount 50.000		Recovery =	60.08%
12) S 1-chlorooctadecane (S...	13.033	3106724	28.898 ug/ml
Spiked Amount 50.000		Recovery =	57.80%
Target Compounds			
6) T n-Tetradecane (C14)	8.309	178100	1.524 ug/ml
10) T n-Eicosane (C20)	12.650	158087	1.281 ug/ml
14) T n-Tetracosane (C24)	14.858	117752	0.941 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD082520AL\
Data File : FD034521.D
Signal(s) : FID2B.CH
Acq On : 25 Aug 2020 18:36
Operator : DD\AJ
Sample : L3784-10
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
RO-24

Integration File: autoint1.e
Quant Time: Aug 26 02:36:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 073120.M
Quant Title : GC Extractables
QLast Update : Mon Aug 03 10:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

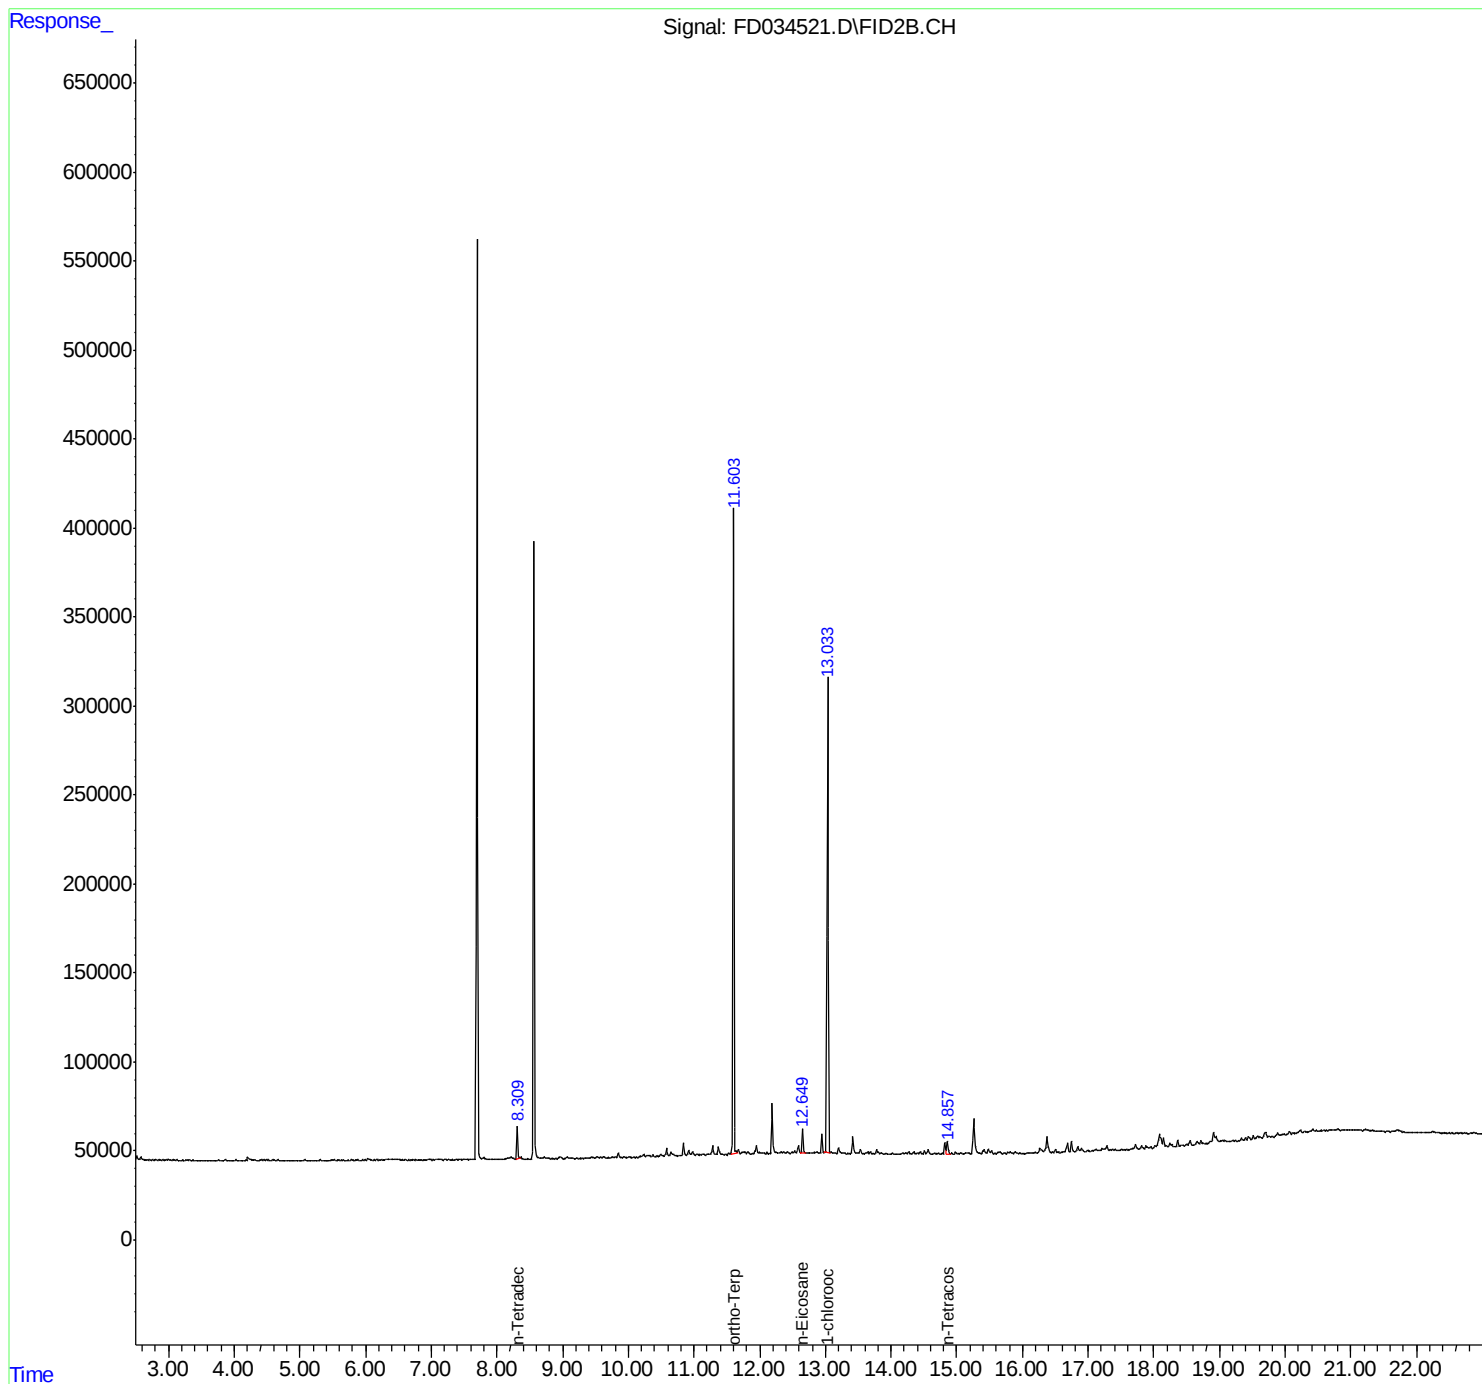


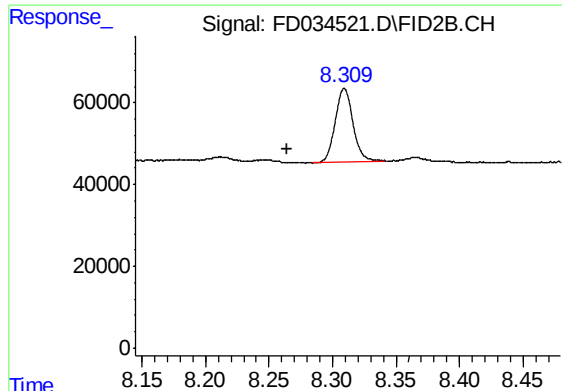

#6 n-Tetradecane (C14)


R.T.: 8.309 min
Delta R.T.: 0.045 min
Response: 178100
Conc: 1.52 ug/ml

Instrument :
FID_D
ClientSampleId :
RO-24

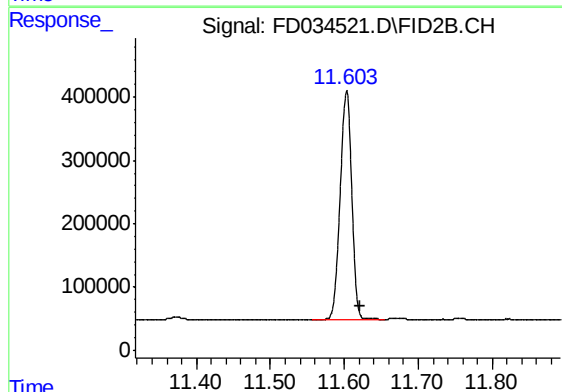


#9 ortho-Terphenyl (SURR)

R.T.: 11.603 min
Delta R.T.: -0.018 min
Response: 3937651
Conc: 30.04 ug/ml

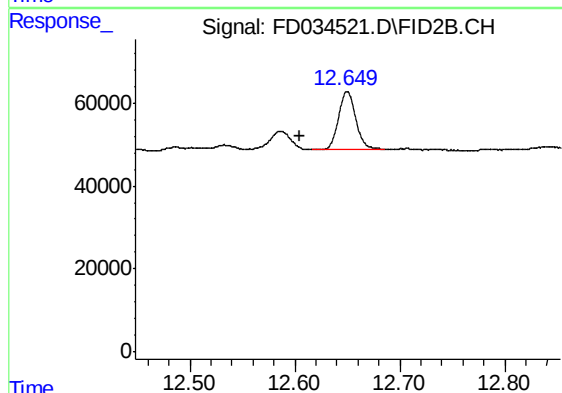


#10 n-Eicosane (C20)

R.T.: 12.650 min
Delta R.T.: 0.046 min
Response: 158087
Conc: 1.28 ug/ml

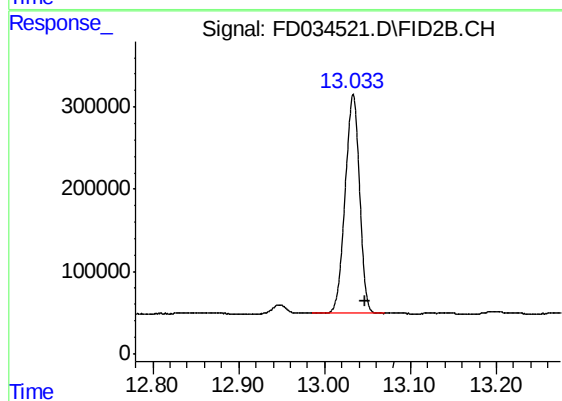

#12 1-chlorooctadecane (SURR)

R.T.: 13.033 min
Delta R.T.: -0.014 min
Response: 3106724
Conc: 28.90 ug/ml

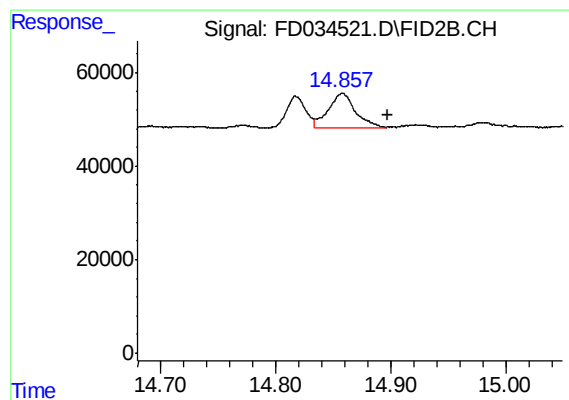

#14 n-Tetracosane (C24)

R.T.: 14.858 min
Delta R.T.: -0.040 min
Response: 117752
Conc: 0.94 ug/ml

Instrument :
FID_D
ClientSampleId :
RO-24