

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD090123AR\
Data File : FD046414.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2023 07:57
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 23:50:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 082223.M
Quant Title : GC Extractables
QLast Update : Tue Aug 22 12:26:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	Benzo[a]anthracene (C...	14.626	242754	1.725 ug/ml
15) T	Chrysene (C27.41)	14.626	242754	1.637 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD090123AR\
Data File : FD046414.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2023 07:57
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 23:50:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 082223.M
Quant Title : GC Extractables
QLast Update : Tue Aug 22 12:26:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 μ l
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18 μ m

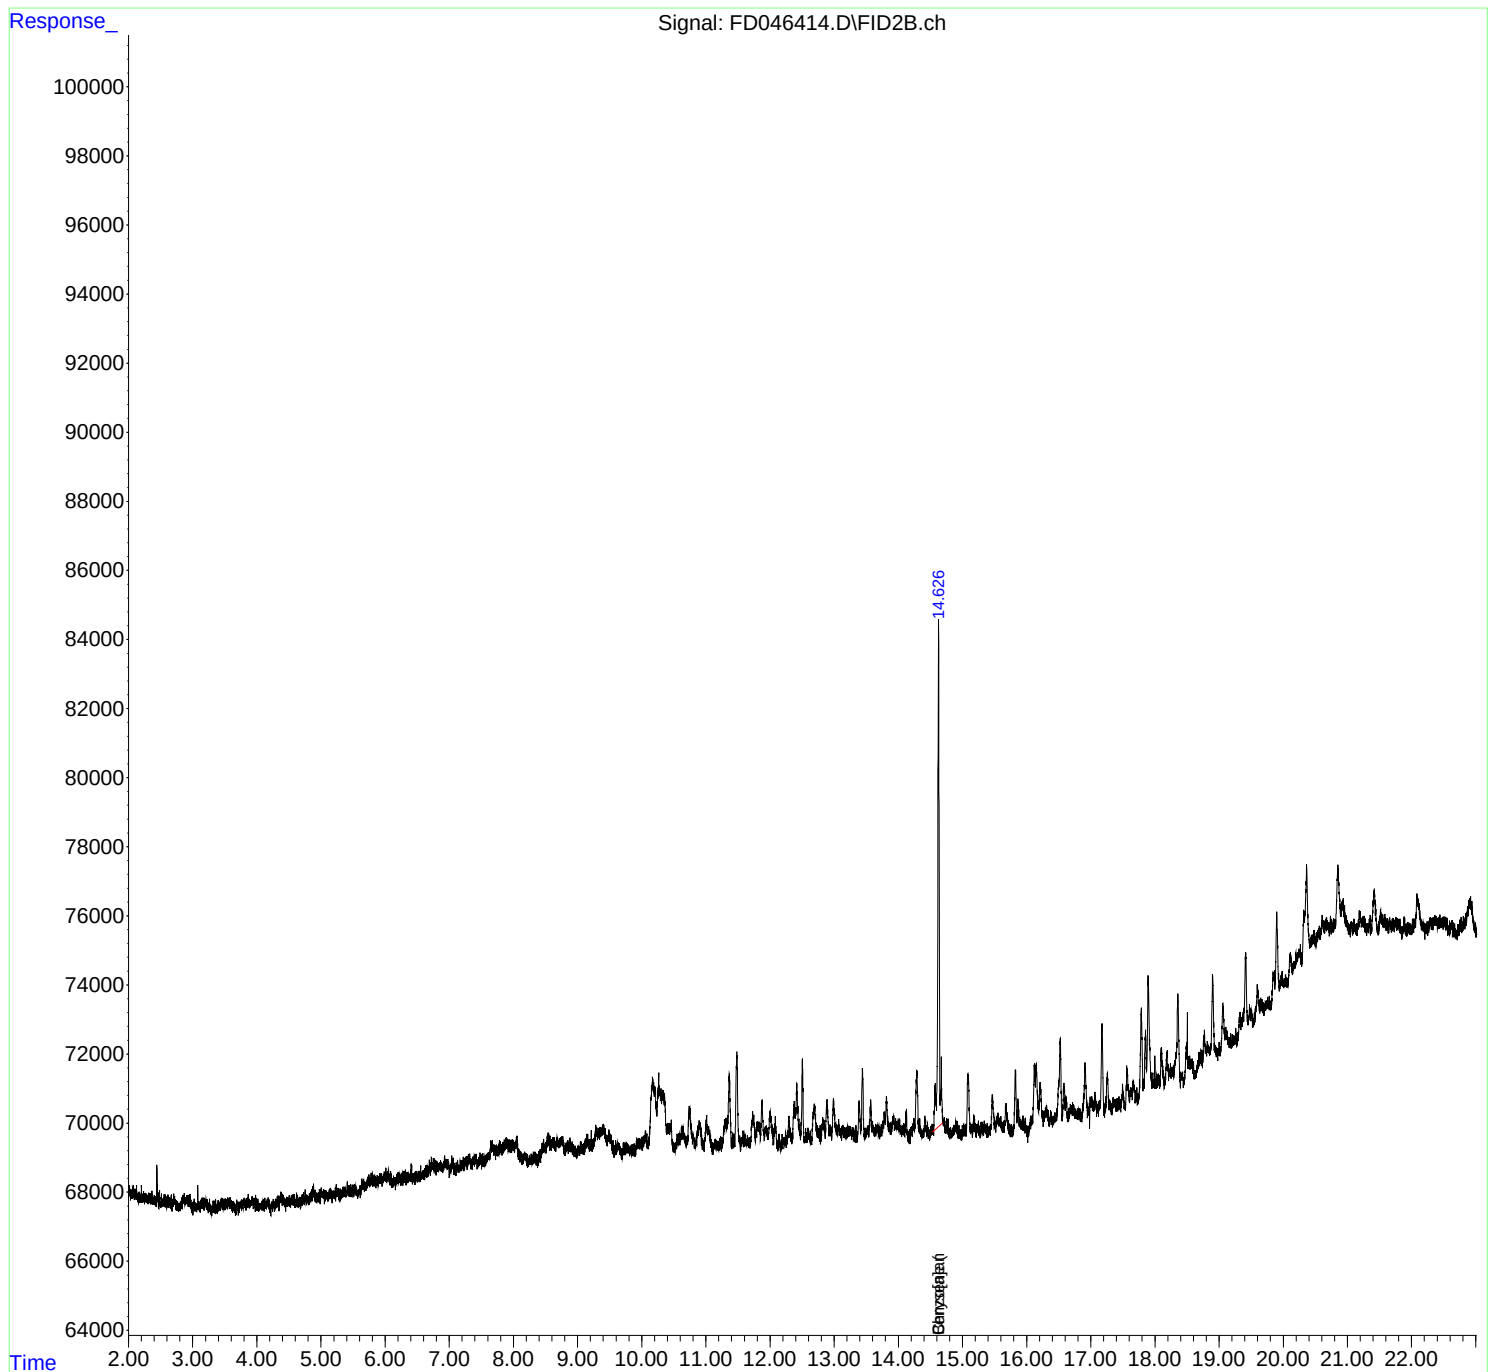


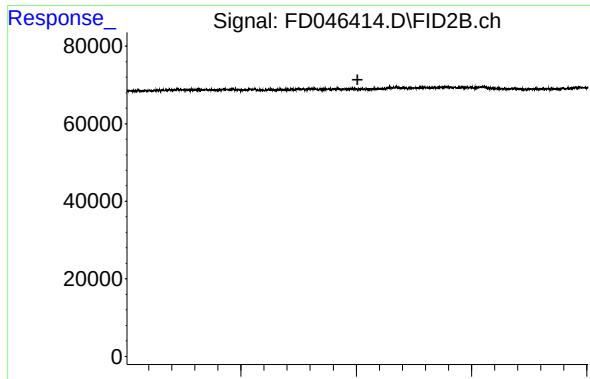

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.506 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

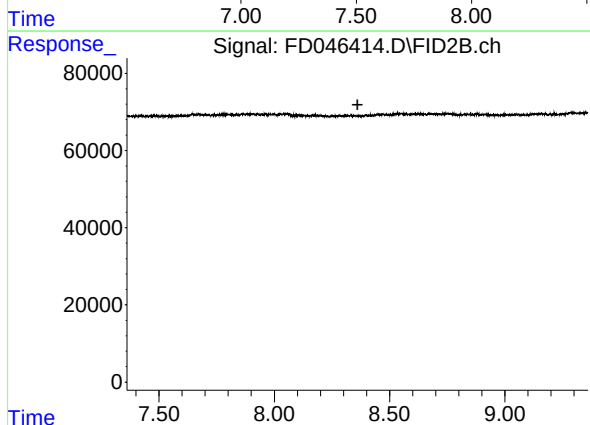


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

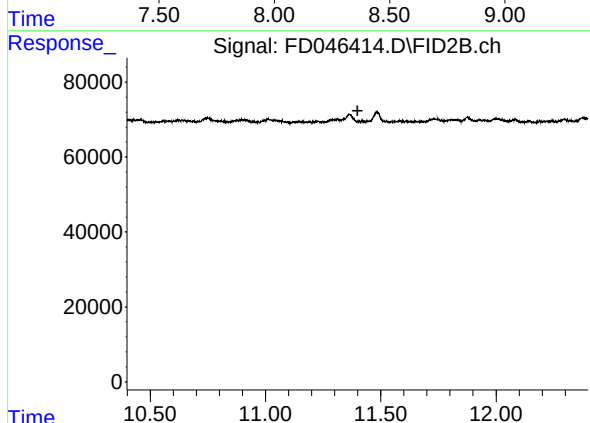


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.399 min
Response: 0
Conc: N.D.

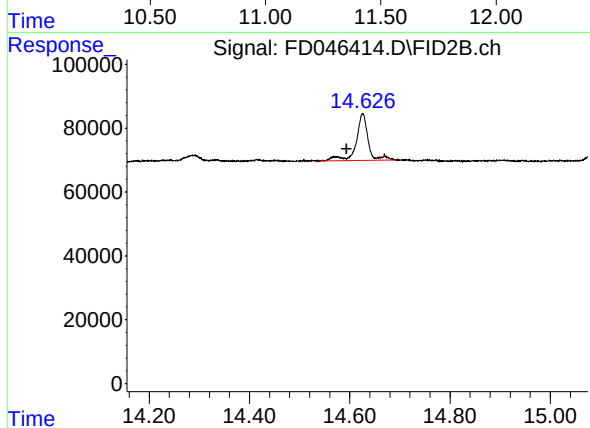

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.626 min
Delta R.T.: 0.032 min
Response: 242754
Conc: 1.73 ug/ml

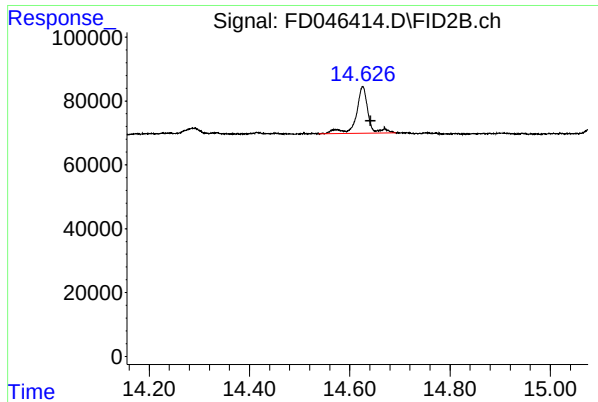

#15 Chrysene (C27.41)

R.T.: 14.626 min

Delta R.T.: -0.016 min

Response: 242754

Conc: 1.64 ug/ml

Instrument :

FID_D

ClientSampleId :