

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD090419AL\
 Data File : FD030498.D
 Signal(s) : FID2B.CH
 Acq On : 04 Sep 2019 19:57
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Sep 05 02:32:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 090319.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 04 04:22:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.615	77782	0.654 ug/ml
18) T	n-Dotriacontane (C32)	18.448	413748	3.608 ug/ml
19) T	n-Tetratriacontane (C34)	19.216	302961	2.791 ug/ml
20) T	n-Hexatriacontane (C36)	19.939	418871	4.081 ug/ml
21) T	n-Octatriacontane (C38)	20.605f	1647578	16.980 ug/ml
22) T	n-Tetracontane (C40)	21.546	374320	3.651 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD090419AL\
Data File : FD030498.D
Signal(s) : FID2B.CH
Acq On : 04 Sep 2019 19:57
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampled :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 05 02:32:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 090319.M
Quant Title : GC Extractables
QLast Update : Wed Sep 04 04:22:49 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

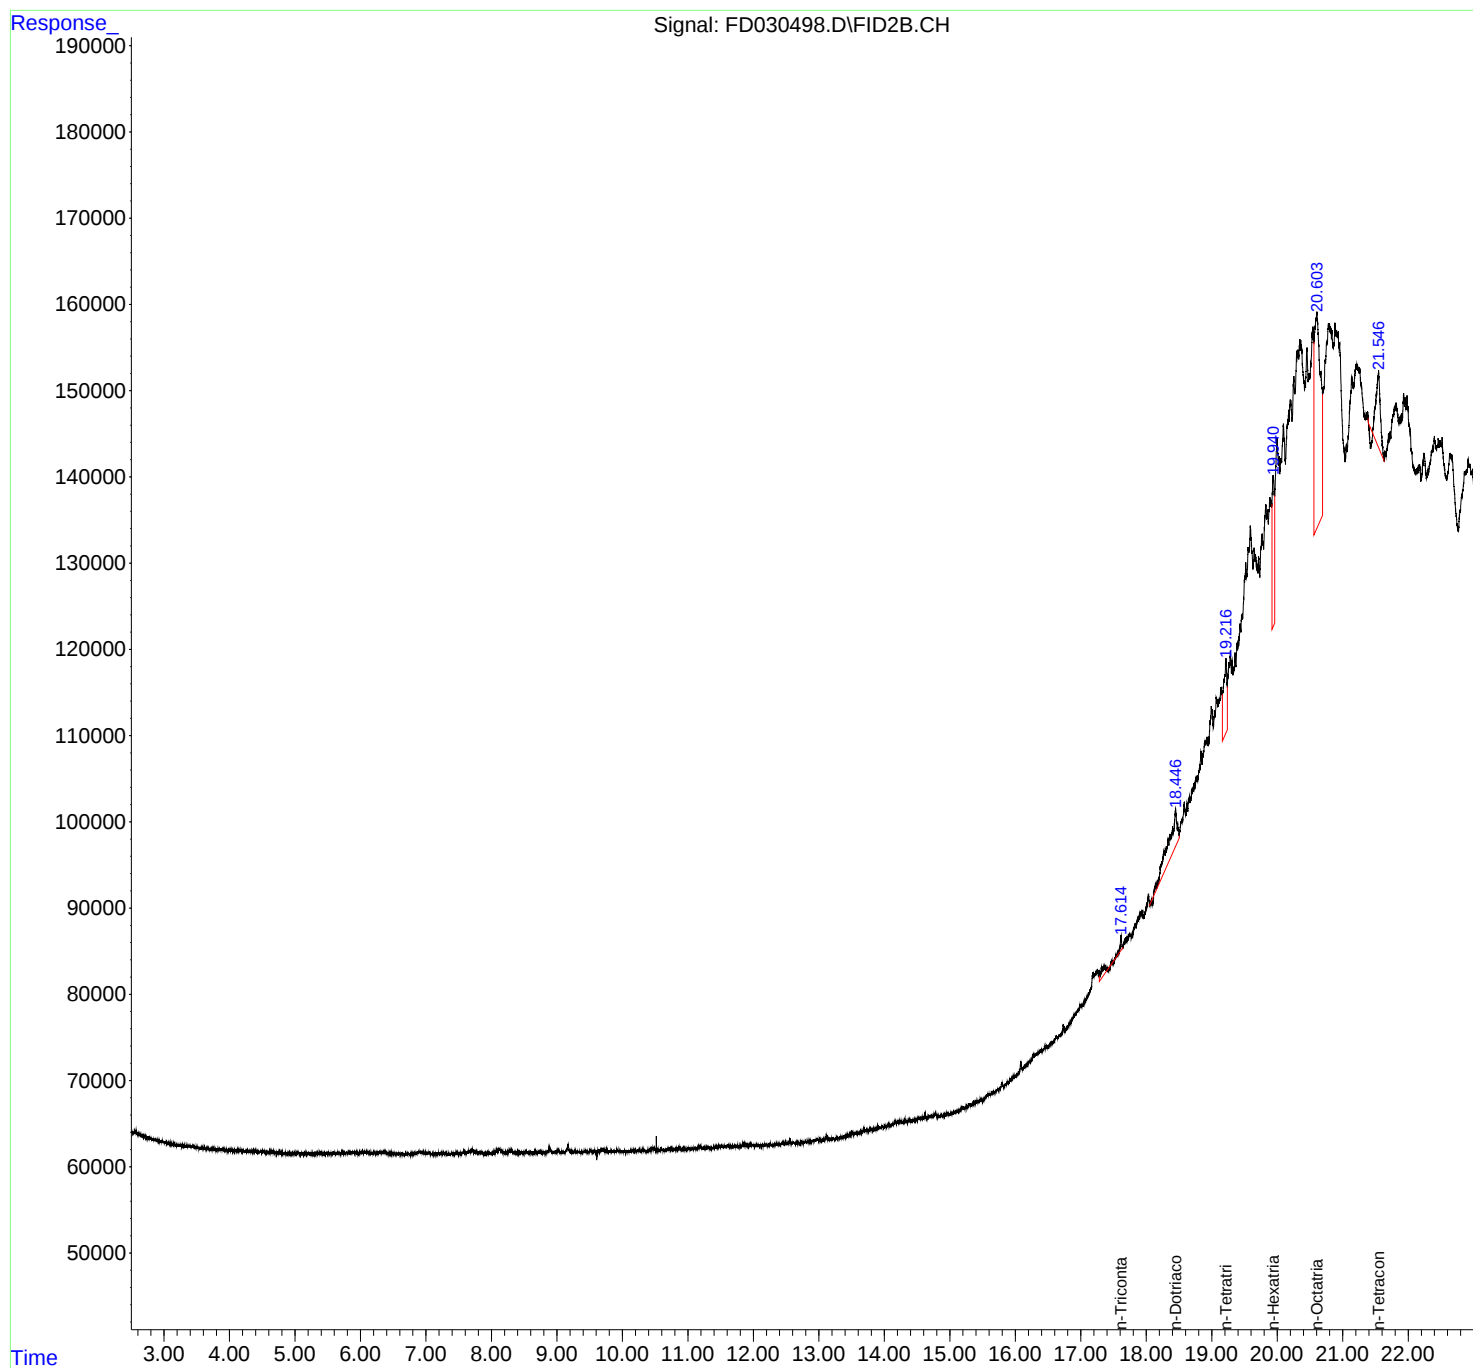


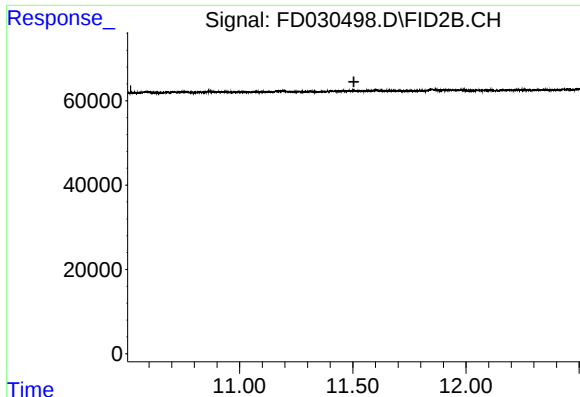

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.505 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
I.BLK

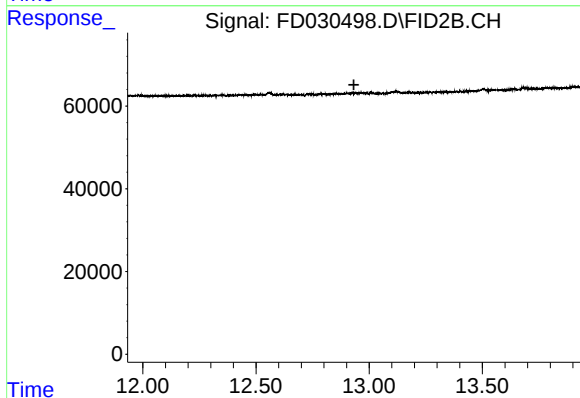


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.932 min
Response: 0
Conc: N.D.

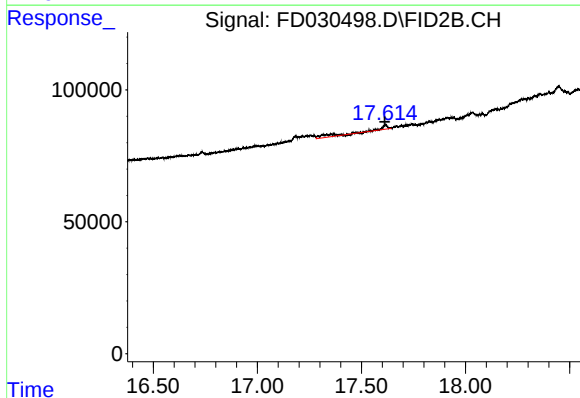


#17 n-Tricontane (C30)

R.T.: 17.615 min
Delta R.T.: 0.004 min
Response: 77782
Conc: 0.65 ug/ml

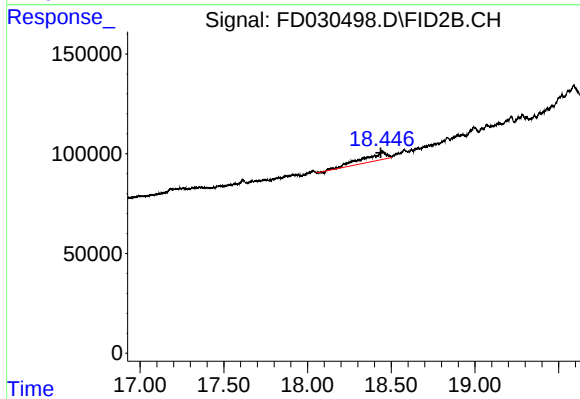

#18 n-Dotriacontane (C32)


R.T.: 18.448 min
Delta R.T.: 0.011 min
Response: 413748
Conc: 3.61 ug/ml

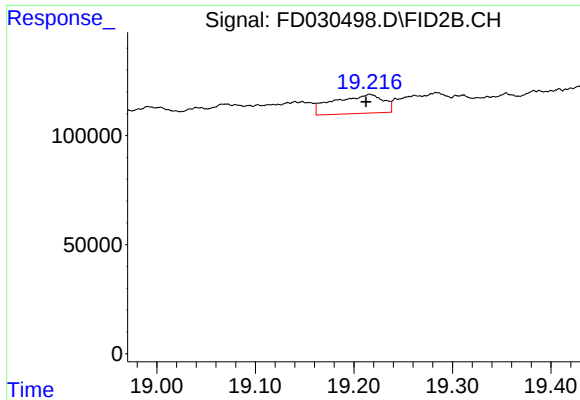

#19 n-Tetratriacontane (C34)


R.T.: 19.216 min
Delta R.T.: 0.004 min
Response: 302961
Conc: 2.79 ug/ml

Instrument :
FID_D
ClientSampleId :
I.BLK

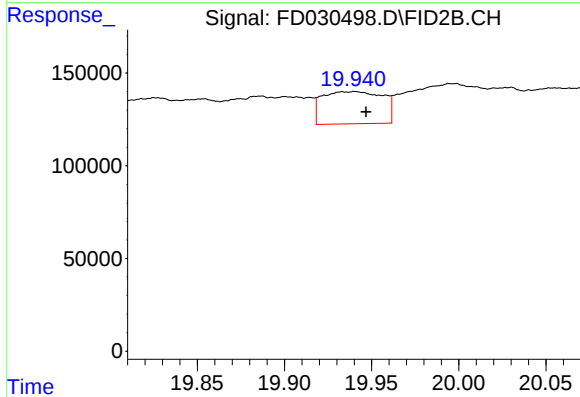


#20 n-Hexatriacontane (C36)

R.T.: 19.939 min
Delta R.T.: -0.008 min
Response: 418871
Conc: 4.08 ug/ml

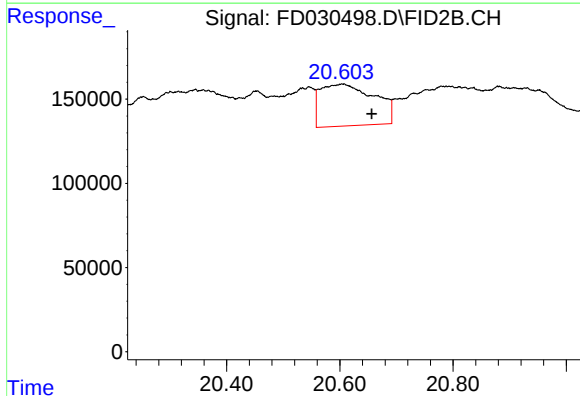

#21 n-Octatriacontane (C38)

R.T.: 20.605 min
Delta R.T.: -0.051 min
Response: 1647578
Conc: 16.98 ug/ml

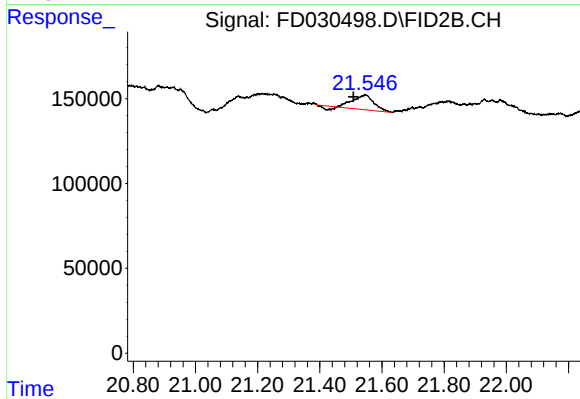

#22 n-Tetracontane (C40)

R.T.: 21.546 min
Delta R.T.: 0.037 min
Response: 374320
Conc: 3.65 ug/ml