

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD090623AR\
Data File : FD046442.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2023 08:43
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 13:37:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 082223.M
Quant Title : GC Extractables
QLast Update : Tue Aug 22 12:26:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	Benzo[a]anthracene (C...	14.628	171776	1.221 ug/ml
15) T	Chrysene (C27.41)	14.628	171776	1.158 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD090623AR\
Data File : FD046442.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2023 08:43
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 13:37:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 082223.M
Quant Title : GC Extractables
QLast Update : Tue Aug 22 12:26:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

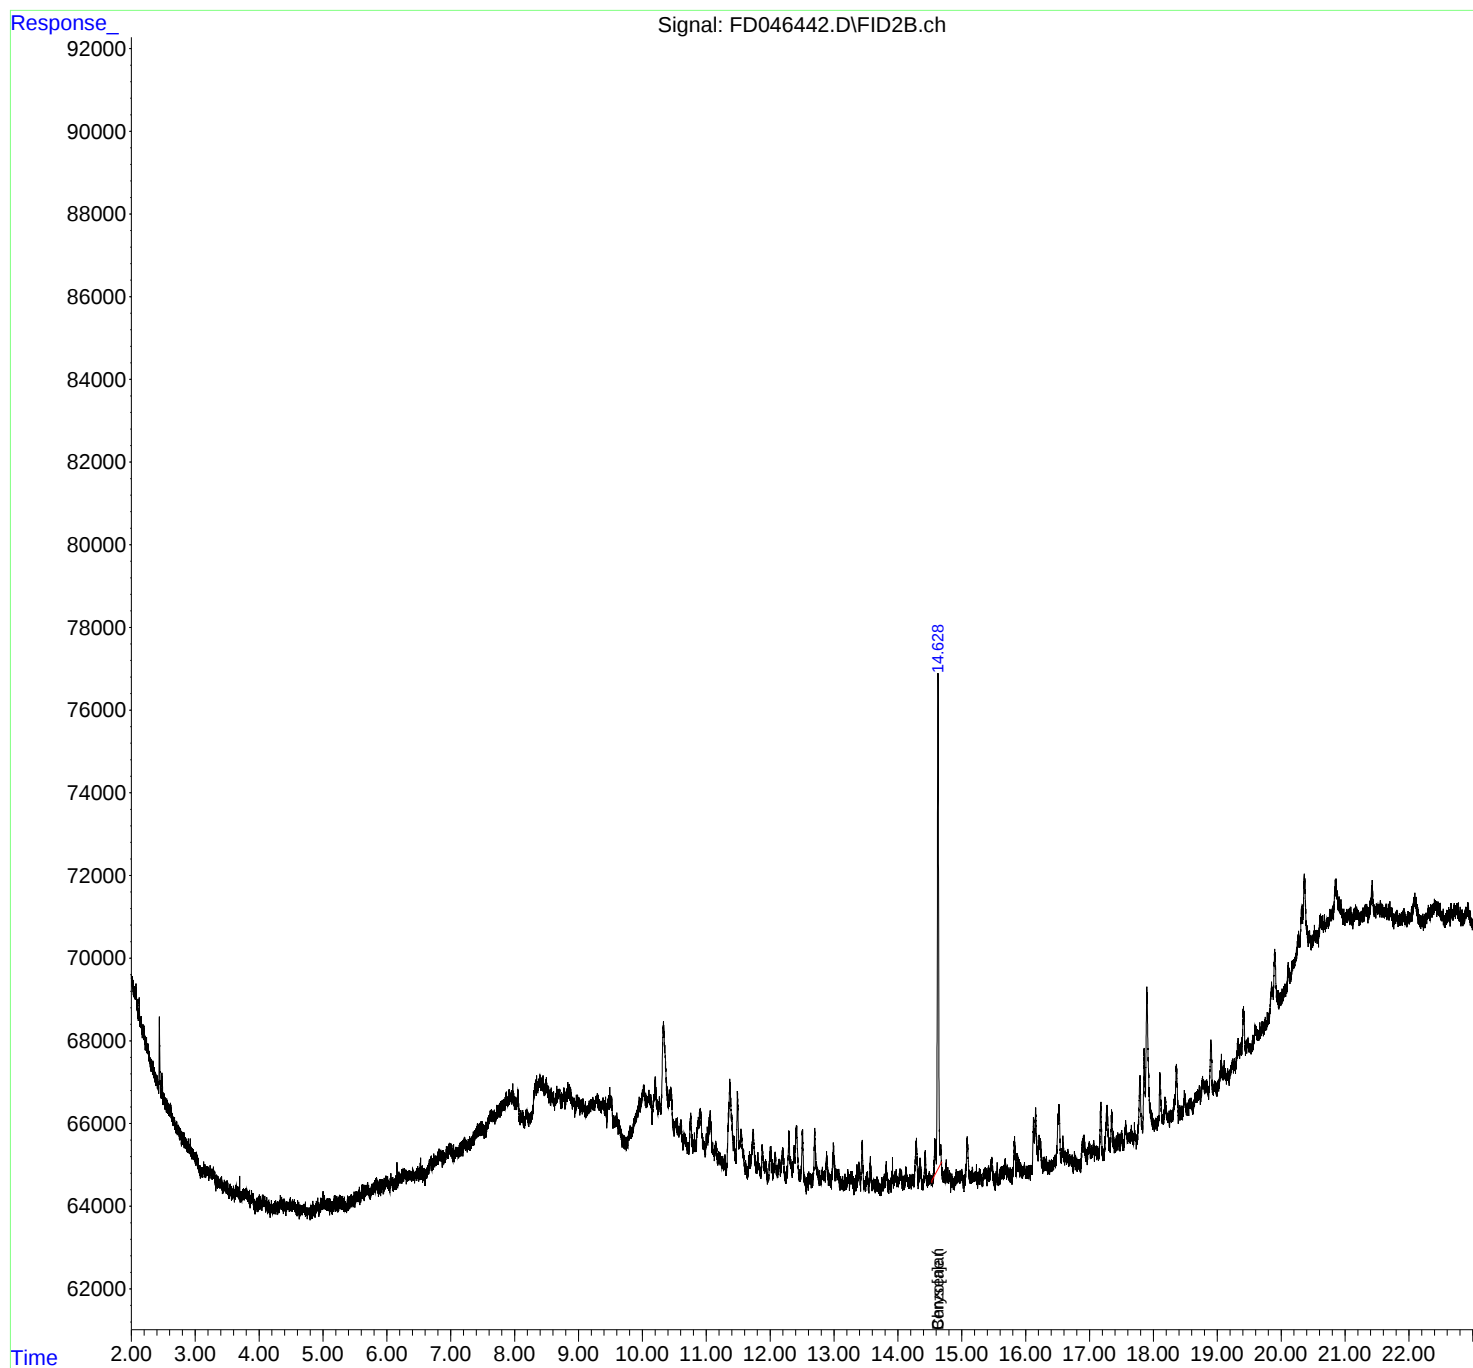


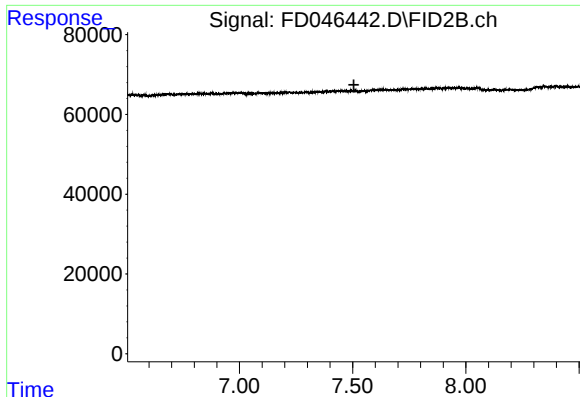

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.506 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

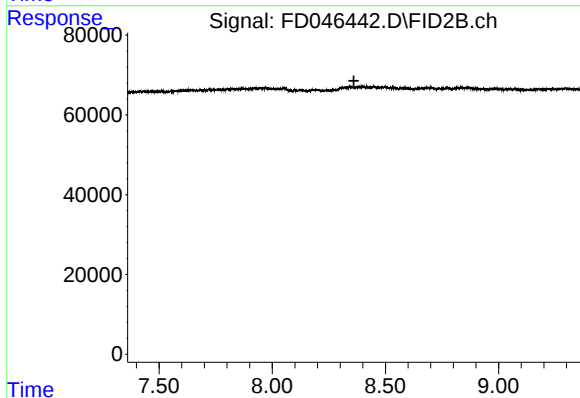


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

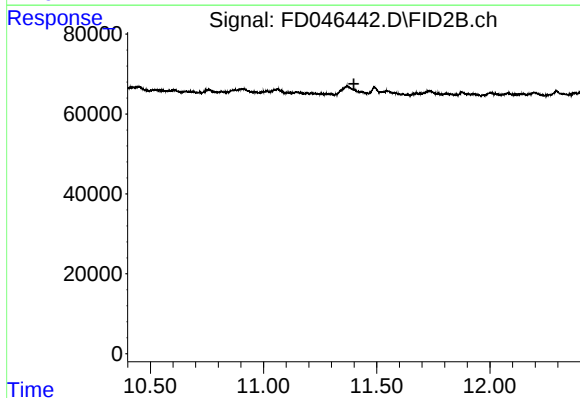


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.399 min
Response: 0
Conc: N.D.

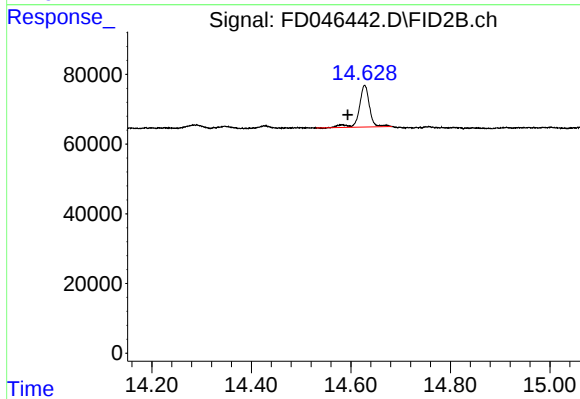

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.628 min
Delta R.T.: 0.034 min
Response: 171776
Conc: 1.22 ug/ml

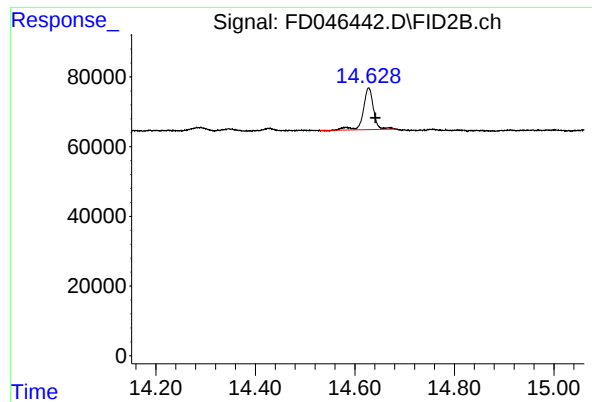

#15 Chrysene (C27.41)

R.T.: 14.628 min
Delta R.T.: -0.014 min
Response: 171776
Conc: 1.16 ug/ml

Instrument :

FID_D

ClientSampleId :