

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD091923AR\
Data File : FD046537.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2023 10:57
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 12:09:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:47:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	17.919f	35290	0.282 ug/ml
20) T	Dibenz[a,h]anthracene...	17.919	35290	0.265 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD091923AR\
Data File : FD046537.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2023 10:57
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 12:09:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:47:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

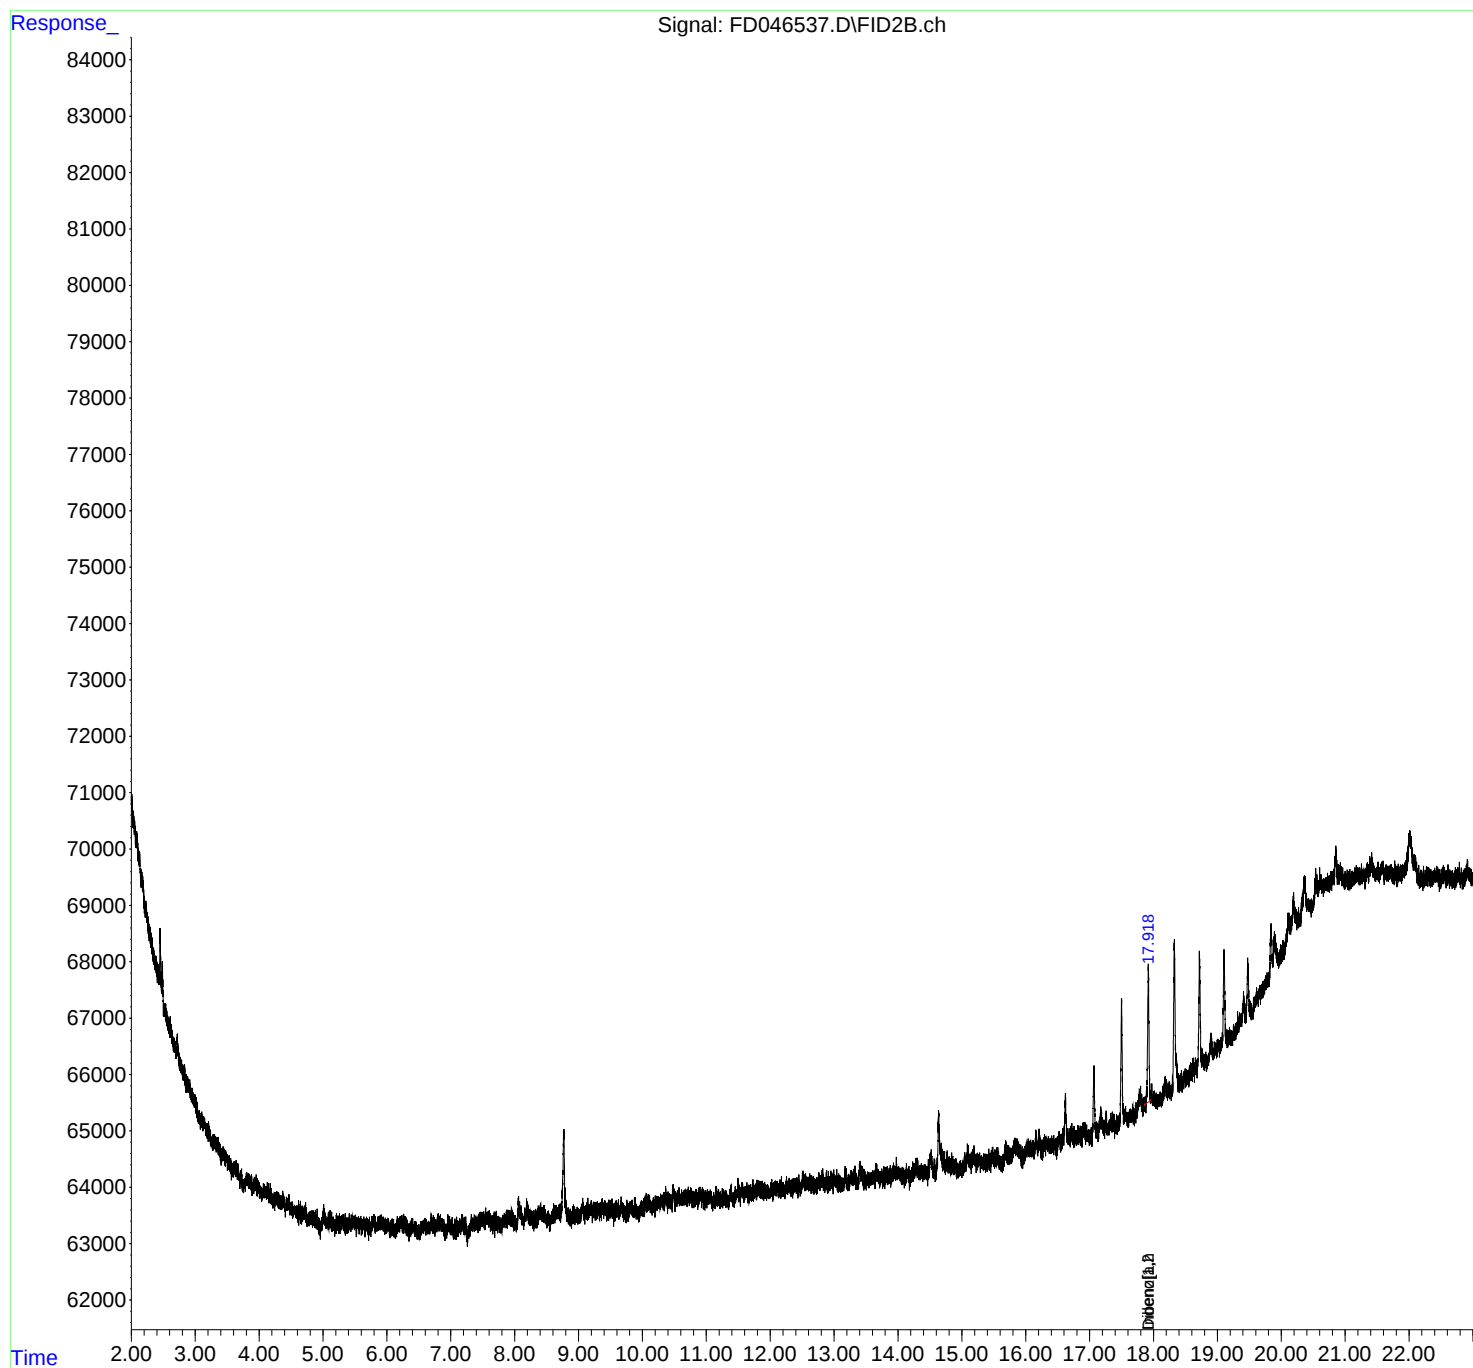


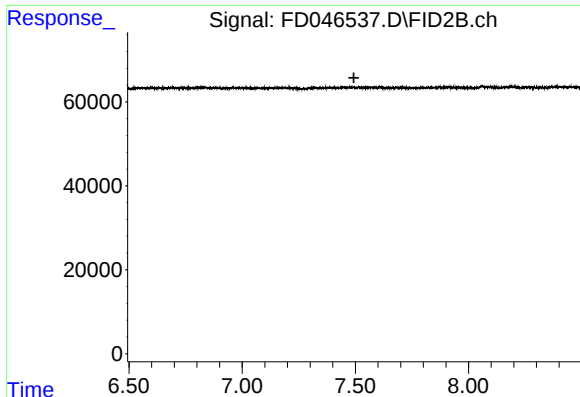

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

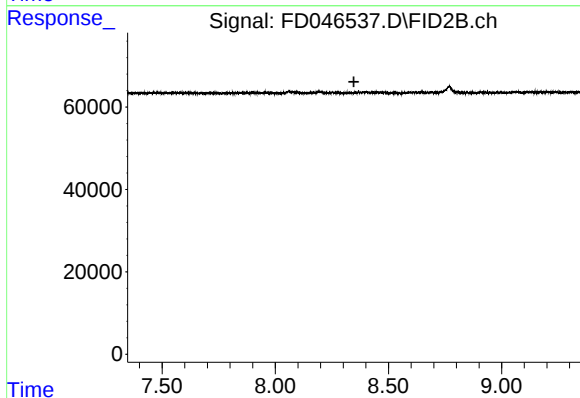


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.347 min
Response: 0
Conc: N.D.

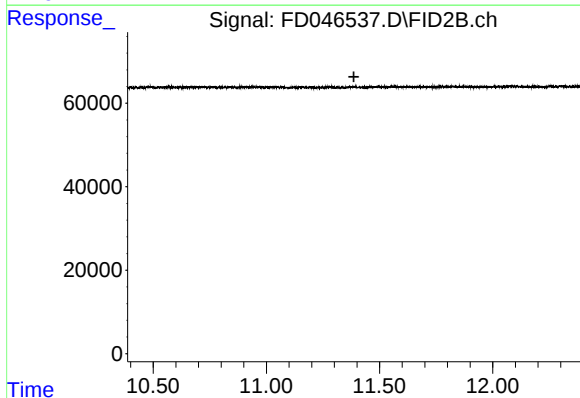


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.386 min
Response: 0
Conc: N.D.

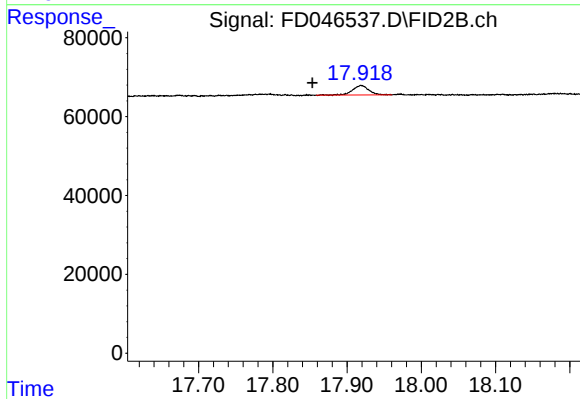

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.919 min
Delta R.T.: 0.066 min
Response: 35290
Conc: 0.28 ug/ml

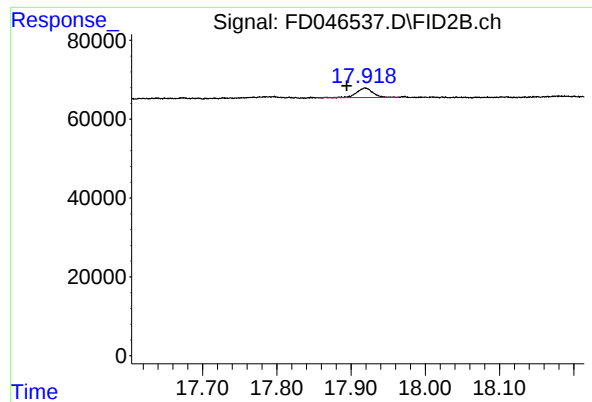

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.919 min
Delta R.T.: 0.025 min
Response: 35290
Conc: 0.27 ug/ml

Instrument :

FID_D

ClientSampleId :