

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091823\
 Data File : P0098081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 15:26
 Operator : YP/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 13:23:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 02:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.508	3.621	44186	36977	0.015	0.025 #
2)	SA Decachlor...	10.345	8.642	108773	-16596	0.063	N.D. #
Target Compounds							
3)	L1 AR-1016-1	5.678	4.703	126406	131842	1.409	2.520 #
4)	L1 AR-1016-2	5.706	4.703	74891	131842	0.578	1.858 #
5)	L1 AR-1016-3	5.761	4.913	47766	575605	0.601	14.854 #
6)	L1 AR-1016-4	5.864	4.913	176784	575605	2.781	18.296 #
7)	L1 AR-1016-5	6.158	5.166	192000	1309924	3.124	32.388 #
8)	L2 AR-1221-1	4.727	3.809	42492	42301	1.162	2.131 #
9)	L2 AR-1221-2	4.796	3.929	66397	99536	2.468	6.470 #
10)	L2 AR-1221-3	4.865	3.995	71340	104571	0.889	2.389 #
11)	L3 AR-1232-1	4.865	3.995	71340	104571	1.089	2.861 #
12)	L3 AR-1232-2	5.405	4.703	20089	131842	0.615	4.034 #
13)	L3 AR-1232-3	5.706	4.886	74891	178779	1.275	10.250 #
14)	L3 AR-1232-4	5.864	5.014	176784	2415984	6.407	147.686 #
15)	L3 AR-1232-5	5.995	5.166	58988	1309924	2.579	74.377 #
16)	L4 AR-1242-1	5.678	4.703	126406	131842	1.567	2.837 #
17)	L4 AR-1242-2	5.706	4.703	74891	131842	0.654	2.096 #
18)	L4 AR-1242-3	5.761	4.886	47766	178779	0.677	5.208 #
19)	L4 AR-1242-4	5.864	5.014	176784	2415984	3.142	68.127 #
20)	L4 AR-1242-5	6.642	5.536	5826327	2389831	98.131	57.505 #
21)	L5 AR-1248-1	5.678	4.703	126406	131842	2.149	3.835 #
22)	L5 AR-1248-2	5.968	4.913f	114868	575605	1.388	12.389 #
23)	L5 AR-1248-3	6.158	5.014	192000	2415984	2.141	48.651 #
24)	L5 AR-1248-4	6.545	5.166	3957316	1309924	40.599	23.032 #
25)	L5 AR-1248-5	6.642	5.536	5826327	2389831	57.974	42.976 #
26)	L6 AR-1254-1	6.545	5.536	3957316	2389831	40.143	30.325
27)	L6 AR-1254-2	6.738	5.653	724629	281659	4.939	4.076
28)	L6 AR-1254-3	7.134	6.059	5181020	721893	34.206	6.862 #
29)	L6 AR-1254-4	7.436	6.287	2685548	211255	24.823	3.301 #
30)	L6 AR-1254-5	7.871	6.711	475675	277268	4.294	3.174 #
31)	L7 AR-1260-1	7.296	6.194	709745	1327236	6.489	17.915 #
32)	L7 AR-1260-2	7.579	6.366	1758003	1968715	13.992	22.811 #
33)	L7 AR-1260-3	7.883f	6.536	68873	252604	0.777	3.105 #
34)	L7 AR-1260-4	8.127	7.010	347229	36731	3.492	0.566 #
35)	L7 AR-1260-5	8.430f	7.231	2196422	92633	10.840	0.656 #
36)	L8 AR-1262-1	7.883	6.808	68873	152261	0.504	4.199 #
37)	L8 AR-1262-2	8.430f	7.010	2196422	36731	9.216	0.488 #
38)	L8 AR-1262-3	8.791	7.538	150974	2692044	0.957	45.396 #
39)	L8 AR-1262-4	8.873	7.592	106637	36300	1.423	0.351 #
40)	L8 AR-1262-5	9.545	8.086	311942	31506	3.896	0.658 #
41)	L9 AR-1268-1	8.791	7.538	150974	2692044	0.550	15.399 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091823\
 Data File : P0098081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 15:26
 Operator : YP/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 13:23:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 02:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.873	7.592	106637	36300	0.435	0.245 #
43) L9	AR-1268-3	9.118	7.903	87500	28887	0.411	0.838 #
44) L9	AR-1268-4	9.545	8.086	311942	31506	3.450	0.580 #
45) L9	AR-1268-5	9.992	8.388	181474	24091	0.261	0.067 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO091823\
Data File : PO098081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2023 15:26
Operator : YP/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 13:23:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 02:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

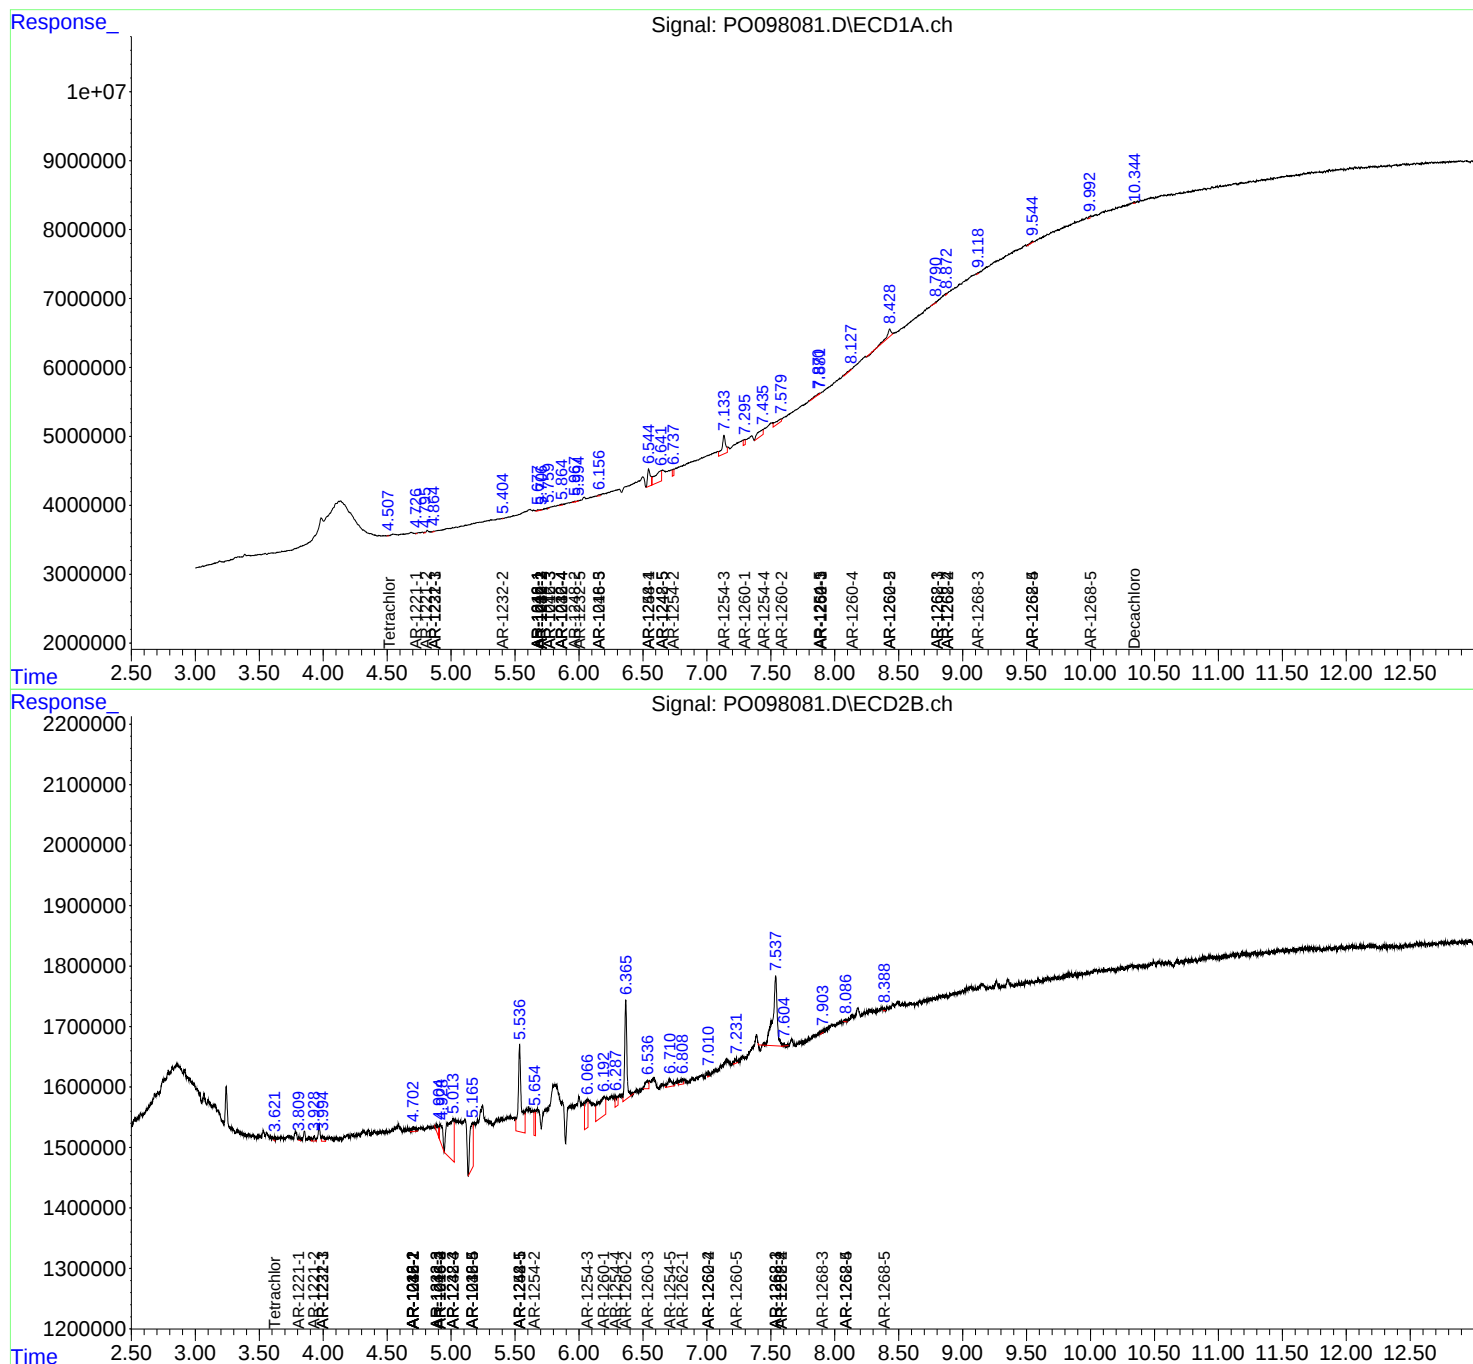


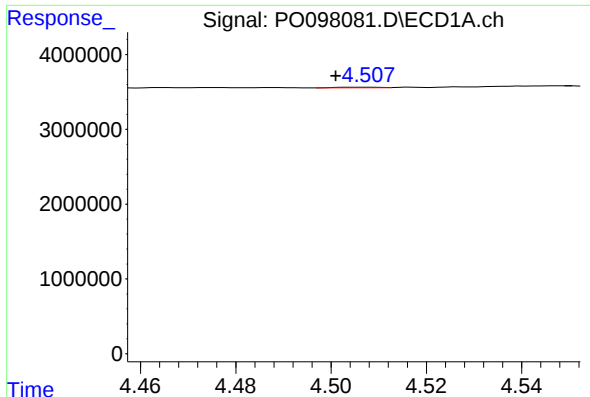

#1 Tetrachloro-m-xylene


R.T.: 4.508 min
Delta R.T.: 0.007 min
Response: 44186
Conc: 0.02 ng/ml

Instrument :
FID_D
ClientSampleId :

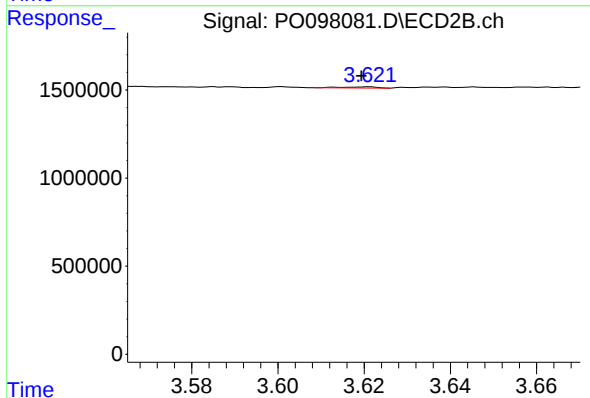


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: 0.001 min
Response: 36977
Conc: 0.03 ng/ml

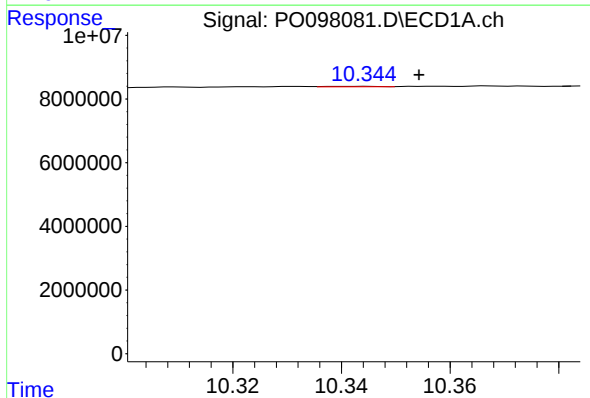


#2 Decachlorobiphenyl

R.T.: 10.345 min
Delta R.T.: -0.010 min
Response: 108773
Conc: 0.06 ng/ml

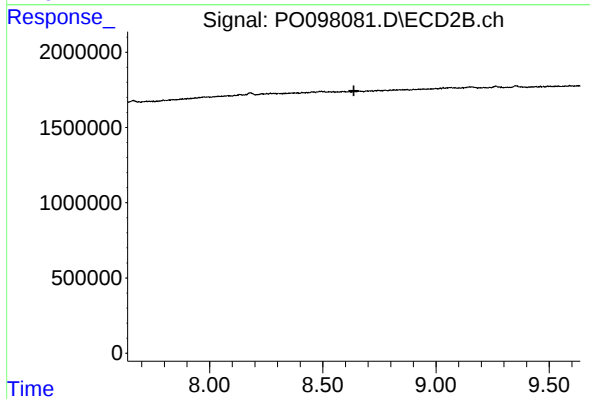

#2 Decachlorobiphenyl


R.T.: 8.642 min
Delta R.T.: 0.006 min
Response: -16596
Conc: N.D.

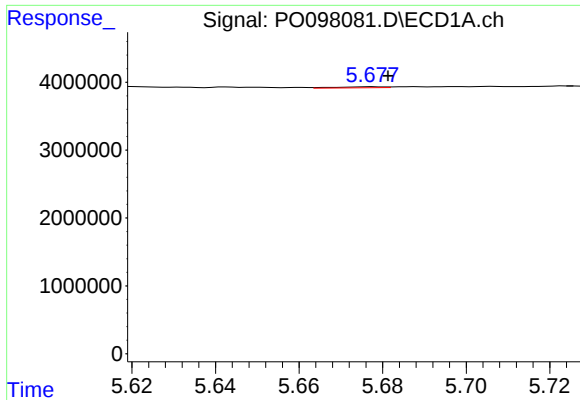

#3 AR-1016-1


R.T.: 5.678 min
Delta R.T.: -0.004 min
Response: 126406
Conc: 1.41 ng/ml

Instrument :
FID_D
ClientSampleId :

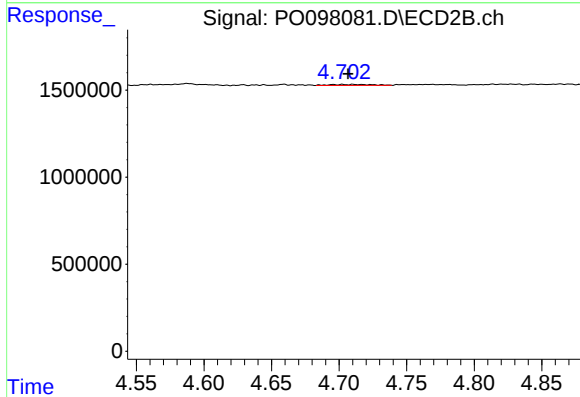


#3 AR-1016-1

R.T.: 4.703 min
Delta R.T.: -0.004 min
Response: 131842
Conc: 2.52 ng/ml

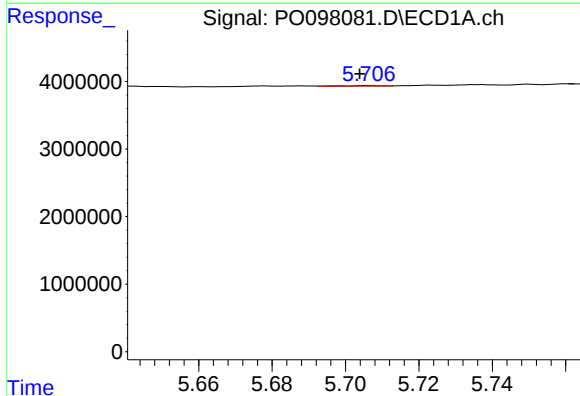


#4 AR-1016-2

R.T.: 5.706 min
Delta R.T.: 0.003 min
Response: 74891
Conc: 0.58 ng/ml

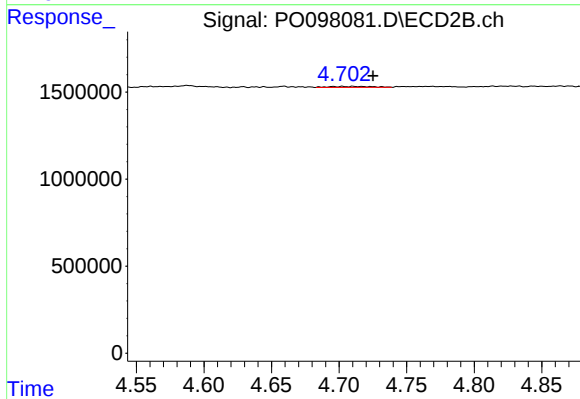

#4 AR-1016-2


R.T.: 4.703 min
Delta R.T.: -0.023 min
Response: 131842
Conc: 1.86 ng/ml

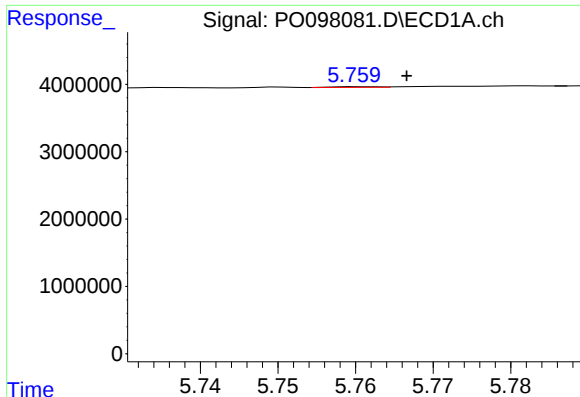

#5 AR-1016-3


R.T.: 5.761 min
Delta R.T.: -0.006 min
Response: 47766
Conc: 0.60 ng/ml

Instrument :
FID_D
ClientSampleId :

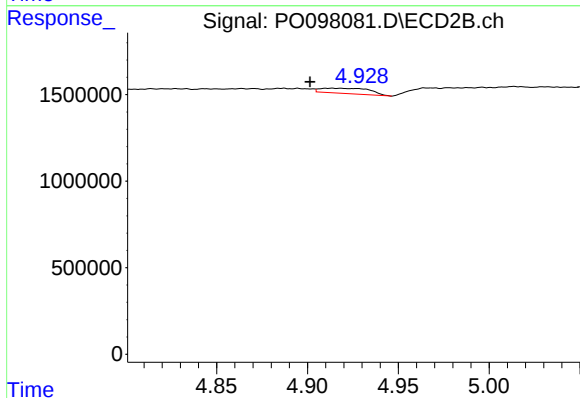


#5 AR-1016-3

R.T.: 4.913 min
Delta R.T.: 0.012 min
Response: 575605
Conc: 14.85 ng/ml

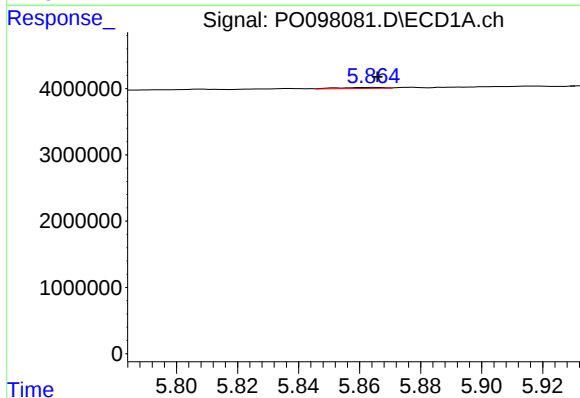


#6 AR-1016-4

R.T.: 5.864 min
Delta R.T.: -0.002 min
Response: 176784
Conc: 2.78 ng/ml

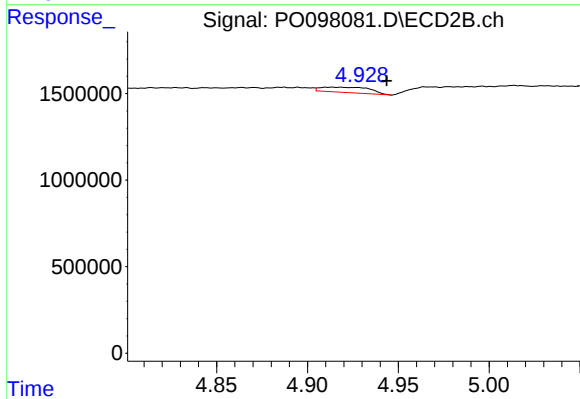

#6 AR-1016-4


R.T.: 4.913 min
Delta R.T.: -0.030 min
Response: 575605
Conc: 18.30 ng/ml

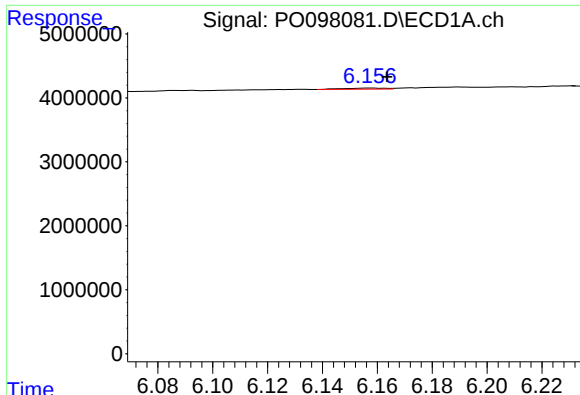

#7 AR-1016-5


R.T.: 6.158 min
Delta R.T.: -0.006 min
Response: 192000
Conc: 3.12 ng/ml

Instrument :
FID_D
ClientSampleId :

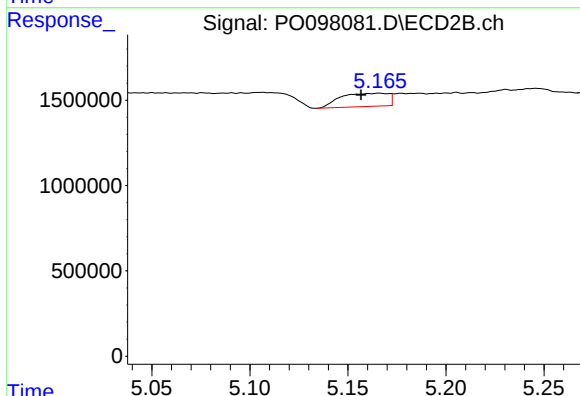


#7 AR-1016-5

R.T.: 5.166 min
Delta R.T.: 0.009 min
Response: 1309924
Conc: 32.39 ng/ml

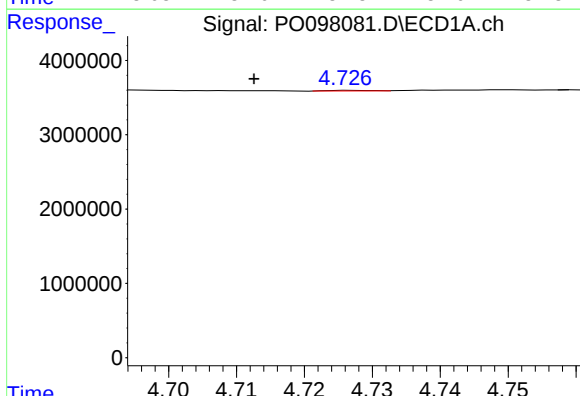


#8 AR-1221-1

R.T.: 4.727 min
Delta R.T.: 0.014 min
Response: 42492
Conc: 1.16 ng/ml

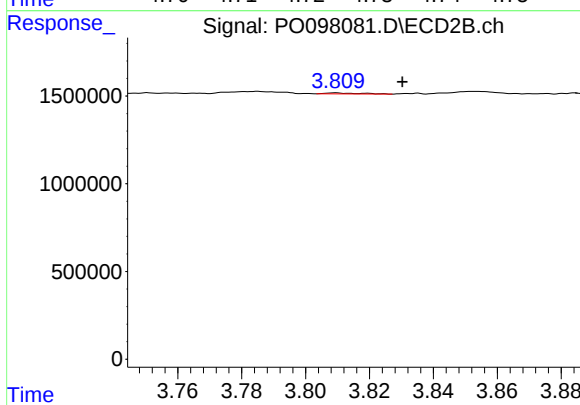

#8 AR-1221-1


R.T.: 3.809 min
Delta R.T.: -0.021 min
Response: 42301
Conc: 2.13 ng/ml

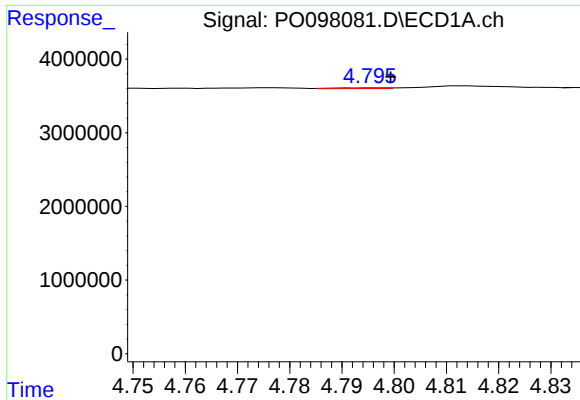

#9 AR-1221-2


R.T.: 4.796 min
Delta R.T.: -0.003 min
Response: 66397
Conc: 2.47 ng/ml

Instrument :
FID_D
ClientSampleId :

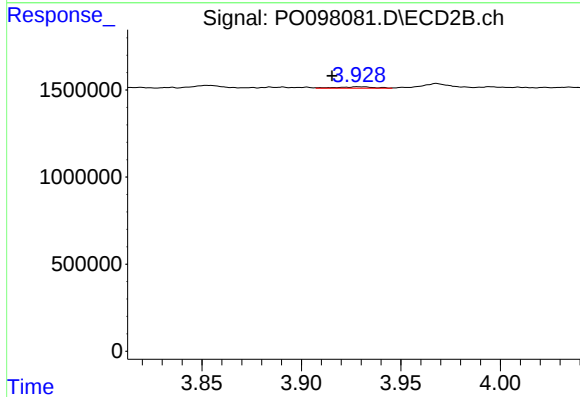


#9 AR-1221-2

R.T.: 3.929 min
Delta R.T.: 0.014 min
Response: 99536
Conc: 6.47 ng/ml

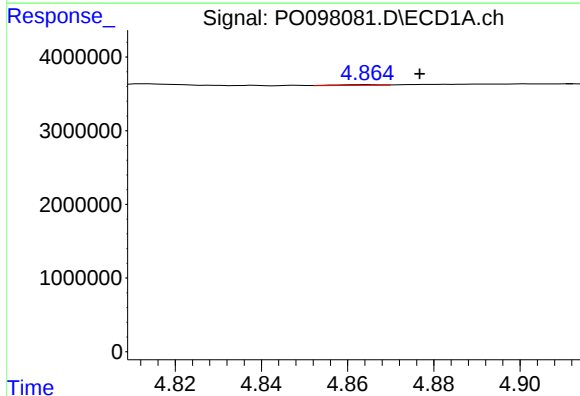


#10 AR-1221-3

R.T.: 4.865 min
Delta R.T.: -0.012 min
Response: 71340
Conc: 0.89 ng/ml

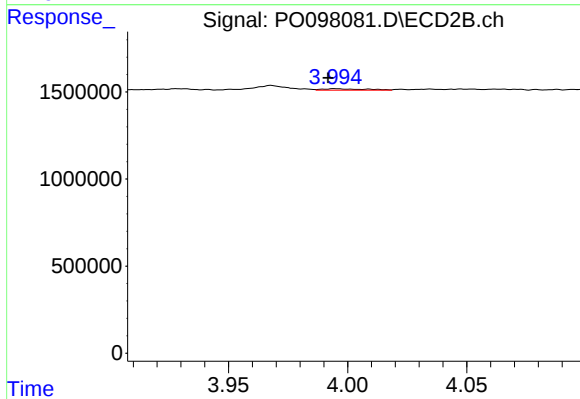

#10 AR-1221-3


R.T.: 3.995 min
Delta R.T.: 0.003 min
Response: 104571
Conc: 2.39 ng/ml

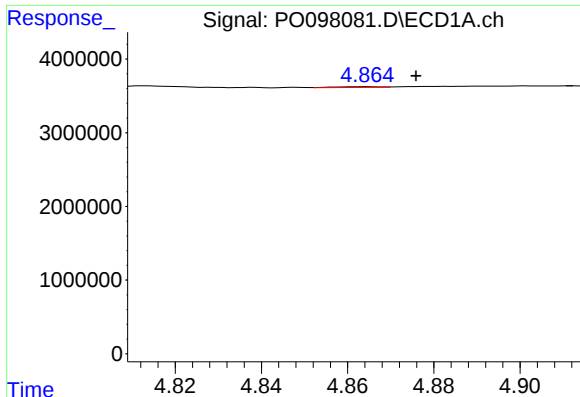

#11 AR-1232-1


R.T.: 4.865 min
Delta R.T.: -0.011 min
Response: 71340
Conc: 1.09 ng/ml

Instrument :
FID_D
ClientSampleId :

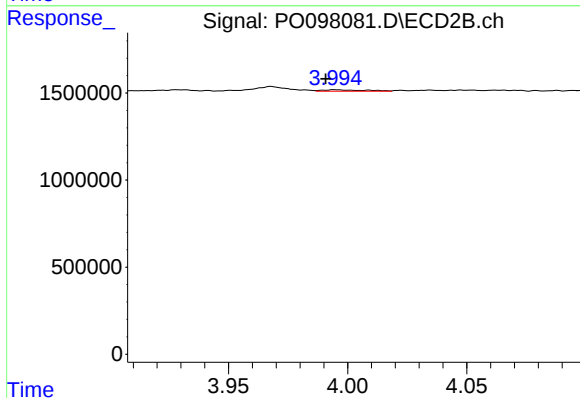


#11 AR-1232-1

R.T.: 3.995 min
Delta R.T.: 0.004 min
Response: 104571
Conc: 2.86 ng/ml

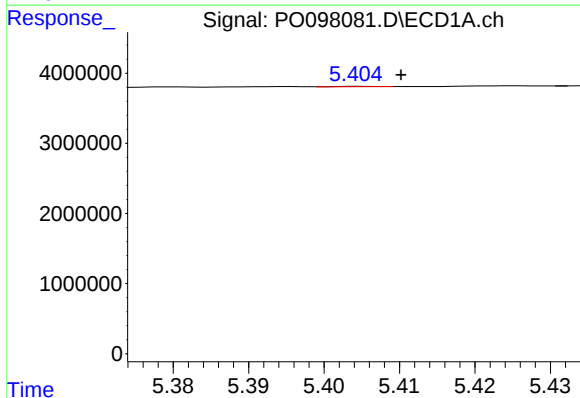


#12 AR-1232-2

R.T.: 5.405 min
Delta R.T.: -0.006 min
Response: 20089
Conc: 0.61 ng/ml

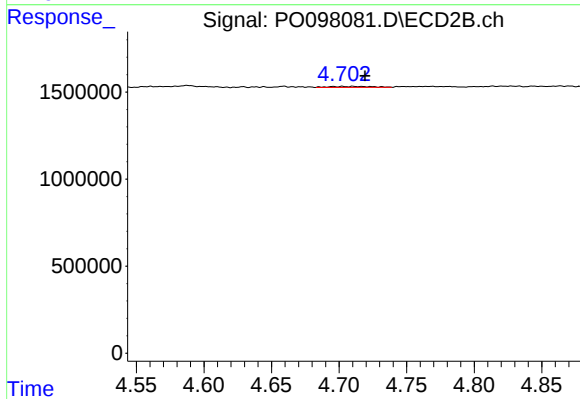

#12 AR-1232-2


R.T.: 4.703 min
Delta R.T.: -0.017 min
Response: 131842
Conc: 4.03 ng/ml

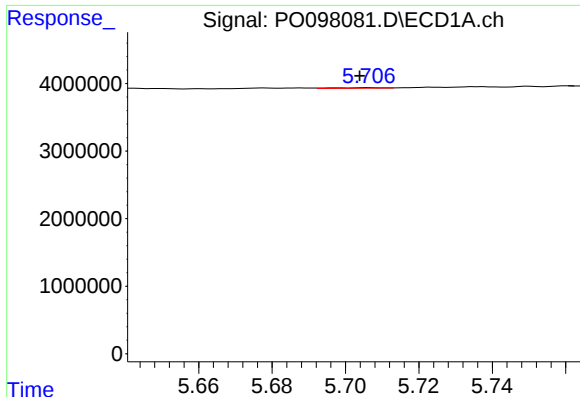

#13 AR-1232-3


R.T.: 5.706 min
Delta R.T.: 0.003 min
Response: 74891
Conc: 1.28 ng/ml

Instrument :
FID_D
ClientSampleId :

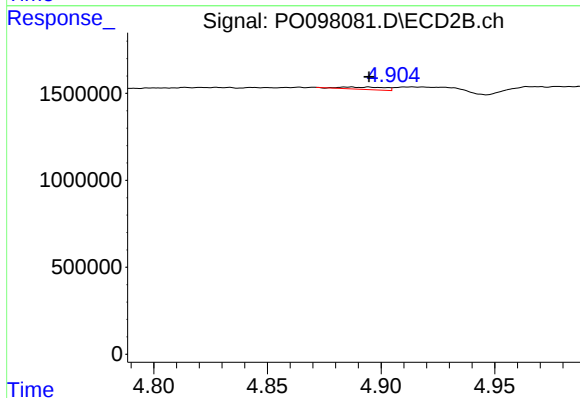


#13 AR-1232-3

R.T.: 4.886 min
Delta R.T.: -0.009 min
Response: 178779
Conc: 10.25 ng/ml

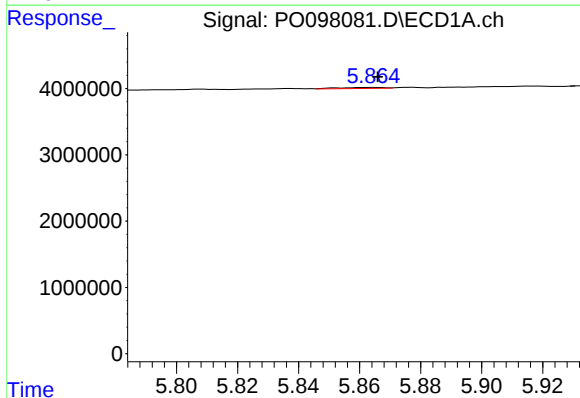


#14 AR-1232-4

R.T.: 5.864 min
Delta R.T.: -0.002 min
Response: 176784
Conc: 6.41 ng/ml

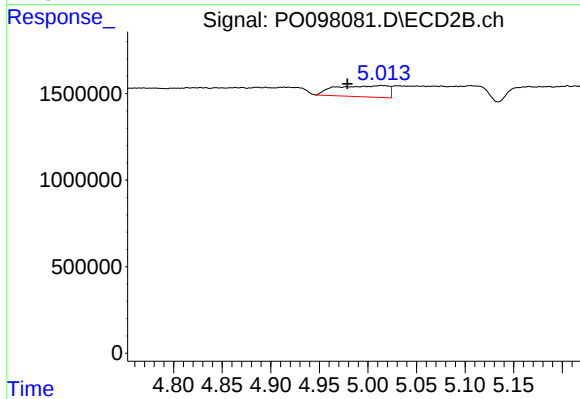

#14 AR-1232-4


R.T.: 5.014 min
Delta R.T.: 0.035 min
Response: 2415984
Conc: 147.69 ng/ml

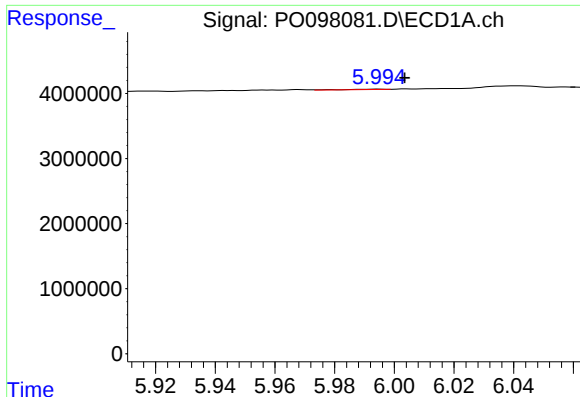

#15 AR-1232-5


R.T.: 5.995 min
Delta R.T.: -0.009 min
Response: 58988
Conc: 2.58 ng/ml

Instrument :
FID_D
ClientSampleId :

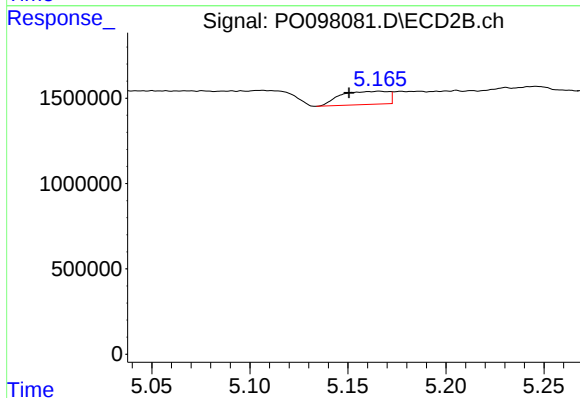


#15 AR-1232-5

R.T.: 5.166 min
Delta R.T.: 0.016 min
Response: 1309924
Conc: 74.38 ng/ml

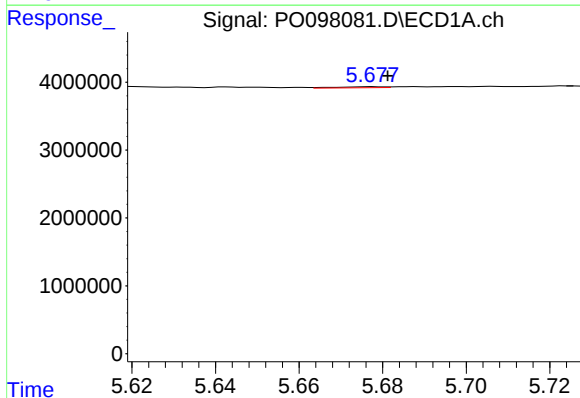


#16 AR-1242-1

R.T.: 5.678 min
Delta R.T.: -0.004 min
Response: 126406
Conc: 1.57 ng/ml

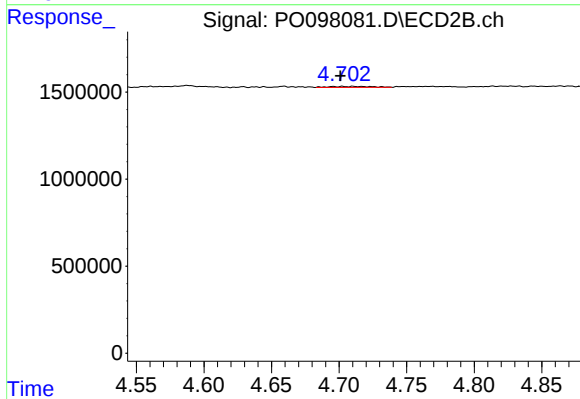

#16 AR-1242-1


R.T.: 4.703 min
Delta R.T.: 0.002 min
Response: 131842
Conc: 2.84 ng/ml

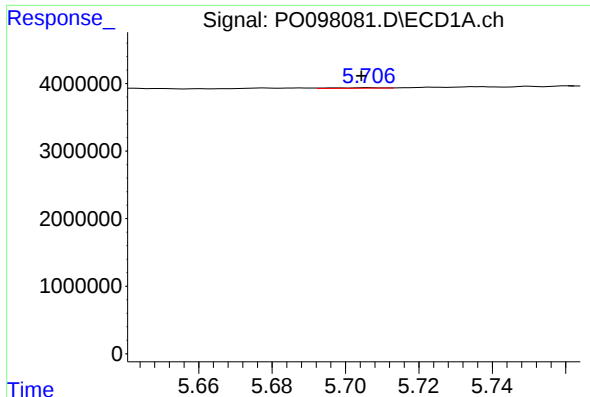

#17 AR-1242-2


R.T.: 5.706 min
Delta R.T.: 0.002 min
Response: 74891
Conc: 0.65 ng/ml

Instrument :
FID_D
ClientSampleId :

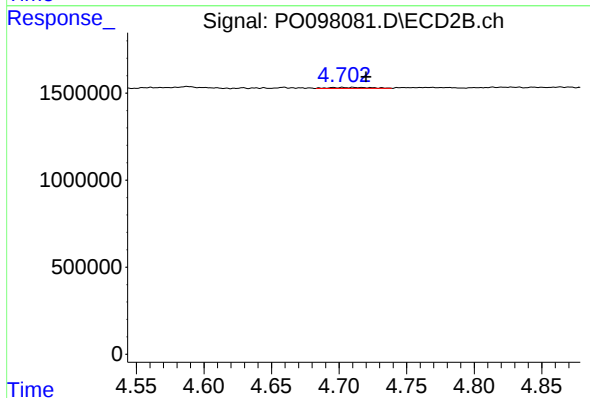


#17 AR-1242-2

R.T.: 4.703 min
Delta R.T.: -0.017 min
Response: 131842
Conc: 2.10 ng/ml

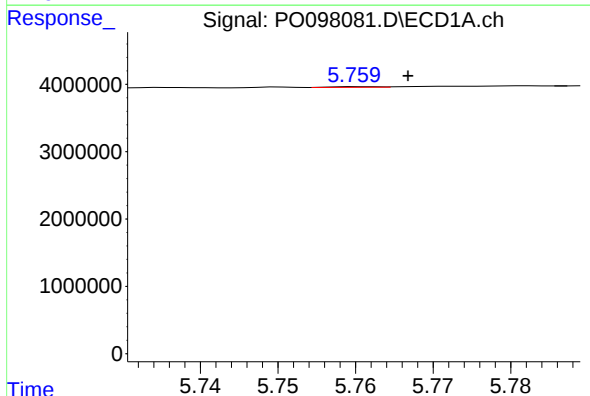


#18 AR-1242-3

R.T.: 5.761 min
Delta R.T.: -0.006 min
Response: 47766
Conc: 0.68 ng/ml

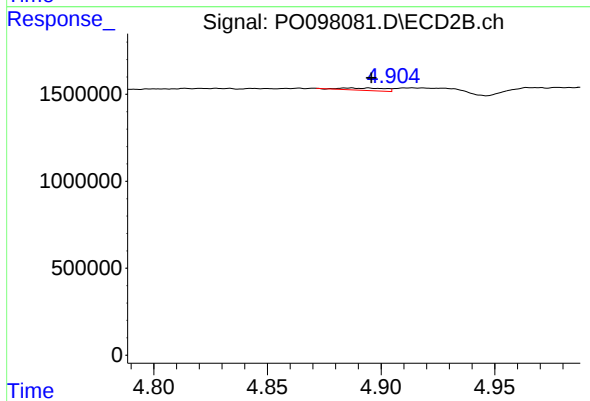

#18 AR-1242-3


R.T.: 4.886 min
Delta R.T.: -0.010 min
Response: 178779
Conc: 5.21 ng/ml

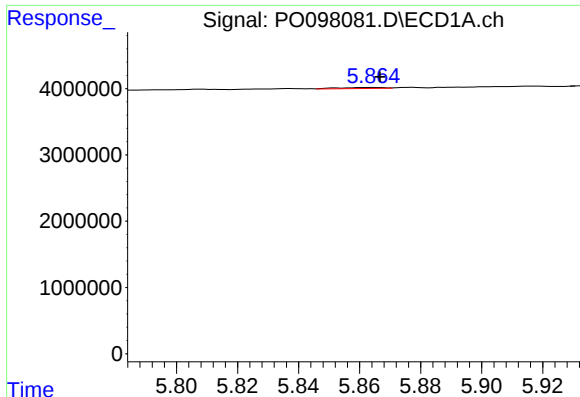

#19 AR-1242-4


R.T.: 5.864 min
Delta R.T.: -0.003 min
Response: 176784
Conc: 3.14 ng/ml

Instrument :
FID_D
ClientSampleId :

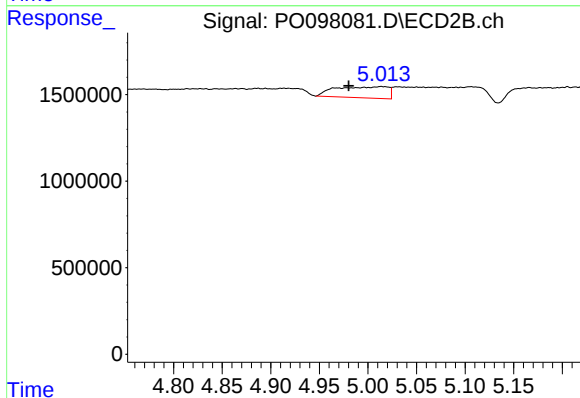


#19 AR-1242-4

R.T.: 5.014 min
Delta R.T.: 0.034 min
Response: 2415984
Conc: 68.13 ng/ml

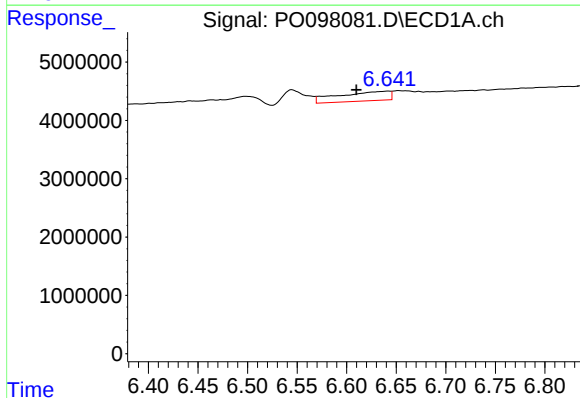


#20 AR-1242-5

R.T.: 6.642 min
Delta R.T.: 0.032 min
Response: 5826327
Conc: 98.13 ng/ml

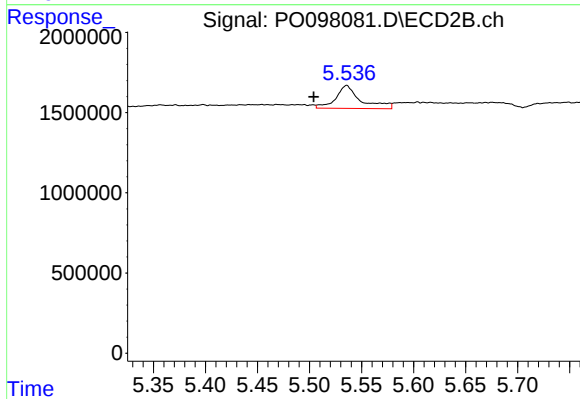

#20 AR-1242-5


R.T.: 5.536 min
Delta R.T.: 0.032 min
Response: 2389831
Conc: 57.50 ng/ml

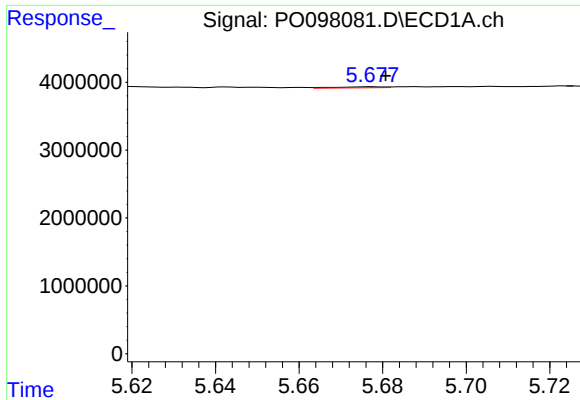

#21 AR-1248-1


R.T.: 5.678 min
Delta R.T.: -0.003 min
Response: 126406
Conc: 2.15 ng/ml

Instrument :
FID_D
ClientSampleId :

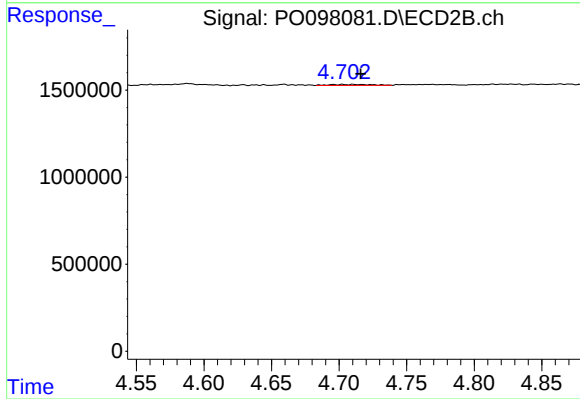


#21 AR-1248-1

R.T.: 4.703 min
Delta R.T.: -0.013 min
Response: 131842
Conc: 3.83 ng/ml

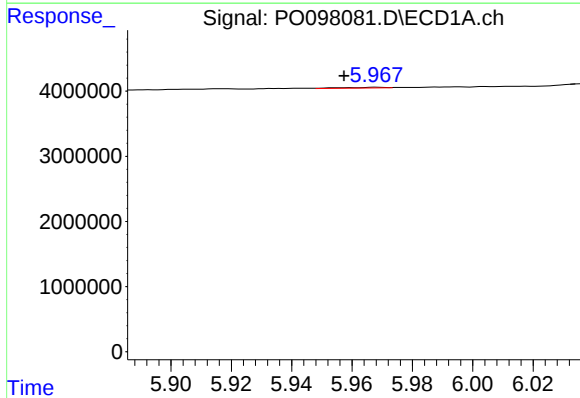


#22 AR-1248-2

R.T.: 5.968 min
Delta R.T.: 0.011 min
Response: 114868
Conc: 1.39 ng/ml

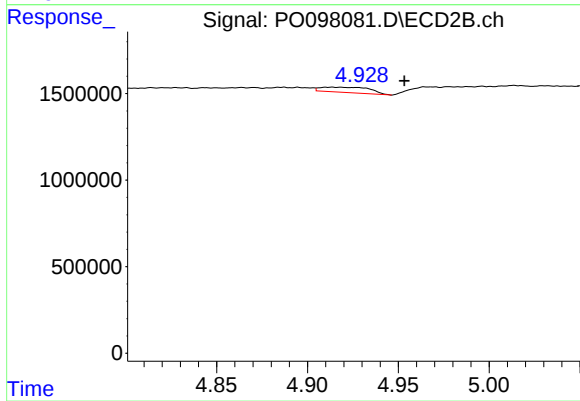

#22 AR-1248-2


R.T.: 4.913 min
Delta R.T.: -0.040 min
Response: 575605
Conc: 12.39 ng/ml

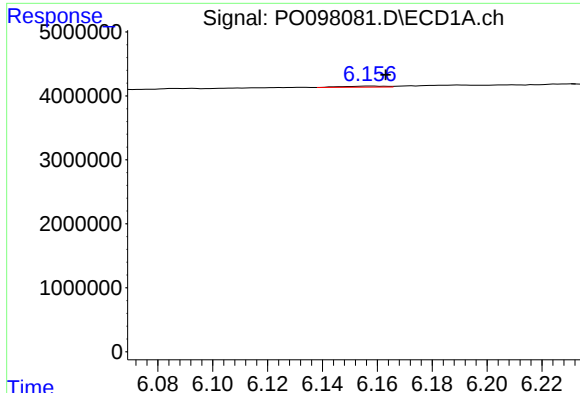

#23 AR-1248-3


R.T.: 6.158 min
Delta R.T.: -0.005 min
Response: 192000
Conc: 2.14 ng/ml

Instrument :
FID_D
ClientSampleId :

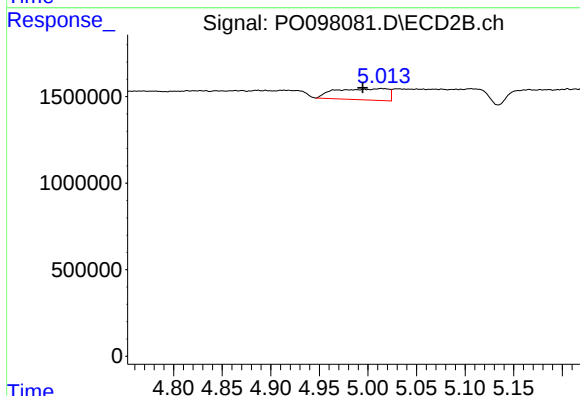


#23 AR-1248-3

R.T.: 5.014 min
Delta R.T.: 0.019 min
Response: 2415984
Conc: 48.65 ng/ml

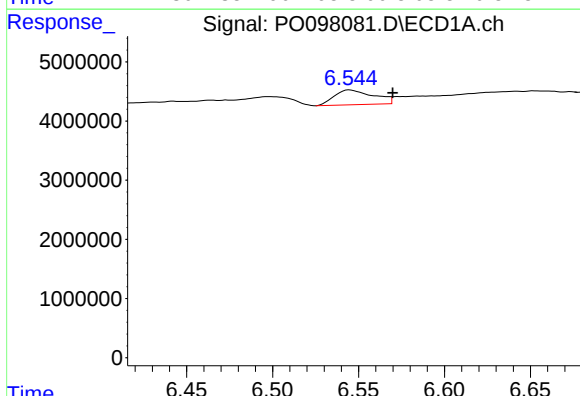


#24 AR-1248-4

R.T.: 6.545 min
Delta R.T.: -0.025 min
Response: 3957316
Conc: 40.60 ng/ml

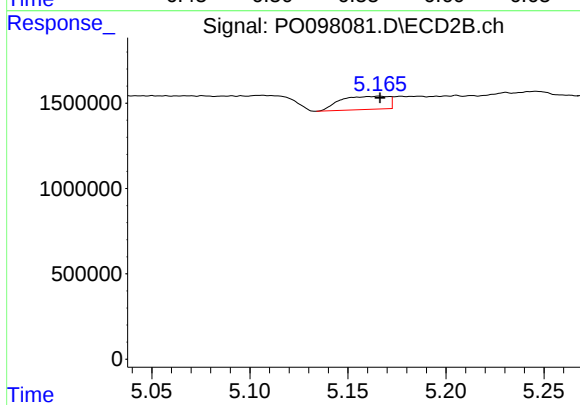

#24 AR-1248-4


R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 1309924
Conc: 23.03 ng/ml

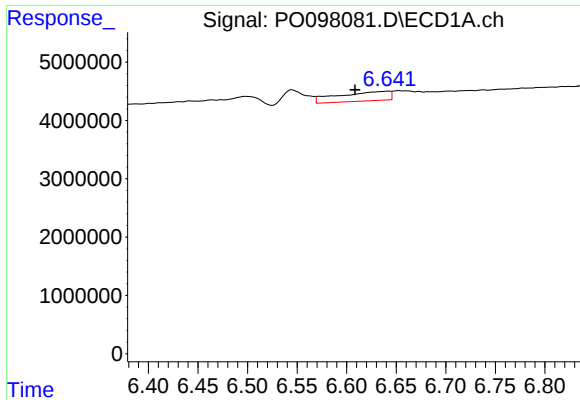

#25 AR-1248-5


R.T.: 6.642 min
Delta R.T.: 0.033 min
Response: 5826327
Conc: 57.97 ng/ml

Instrument :
FID_D
ClientSampleId :

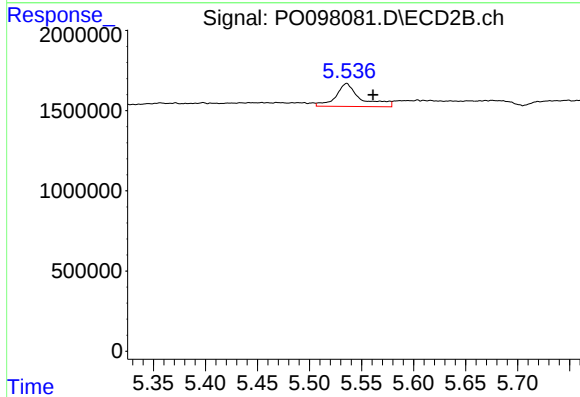


#25 AR-1248-5

R.T.: 5.536 min
Delta R.T.: -0.025 min
Response: 2389831
Conc: 42.98 ng/ml

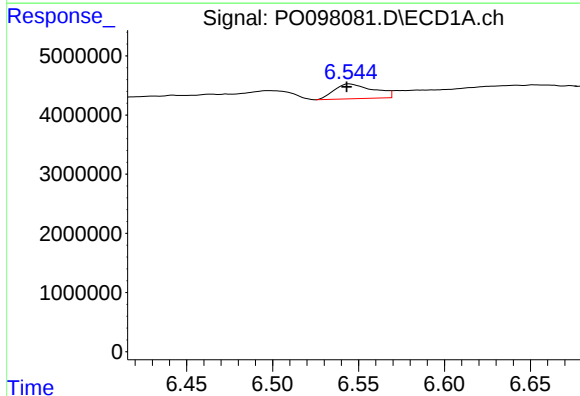


#26 AR-1254-1

R.T.: 6.545 min
Delta R.T.: 0.002 min
Response: 3957316
Conc: 40.14 ng/ml

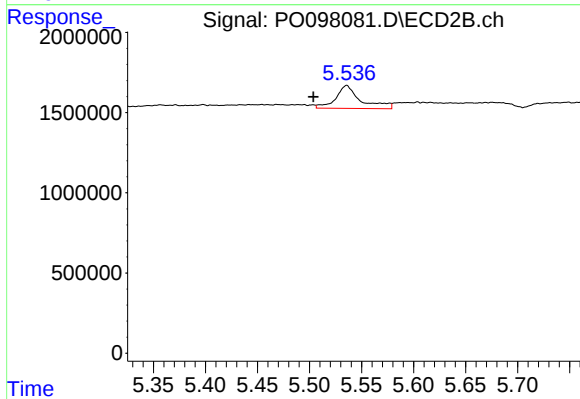

#26 AR-1254-1


R.T.: 5.536 min
Delta R.T.: 0.032 min
Response: 2389831
Conc: 30.33 ng/ml

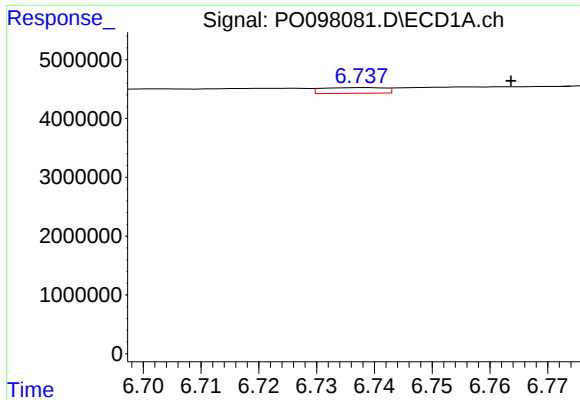

#27 AR-1254-2


R.T.: 6.738 min
Delta R.T.: -0.025 min
Response: 724629
Conc: 4.94 ng/ml

Instrument :
FID_D
ClientSampleId :

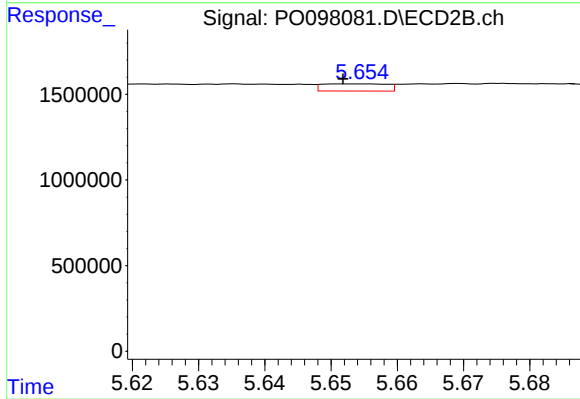


#27 AR-1254-2

R.T.: 5.653 min
Delta R.T.: 0.002 min
Response: 281659
Conc: 4.08 ng/ml

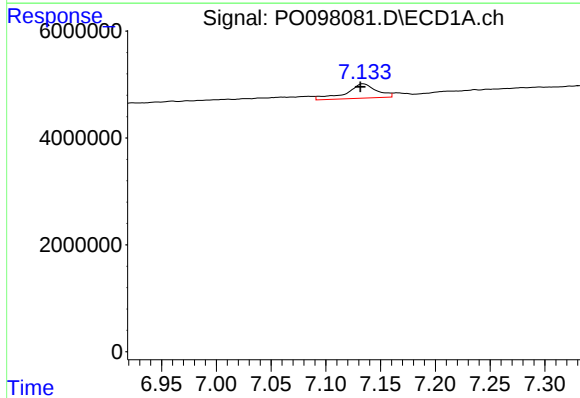


#28 AR-1254-3

R.T.: 7.134 min
Delta R.T.: 0.002 min
Response: 5181020
Conc: 34.21 ng/ml

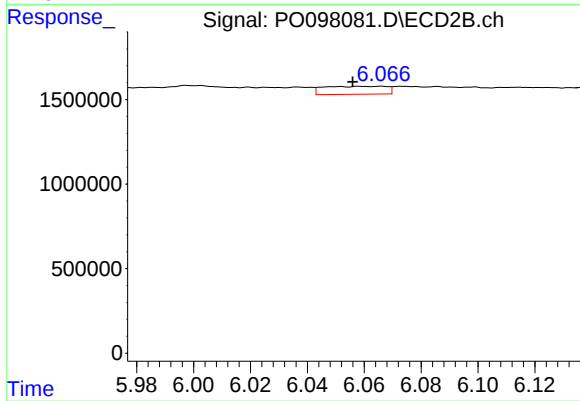

#28 AR-1254-3


R.T.: 6.059 min
Delta R.T.: 0.003 min
Response: 721893
Conc: 6.86 ng/ml

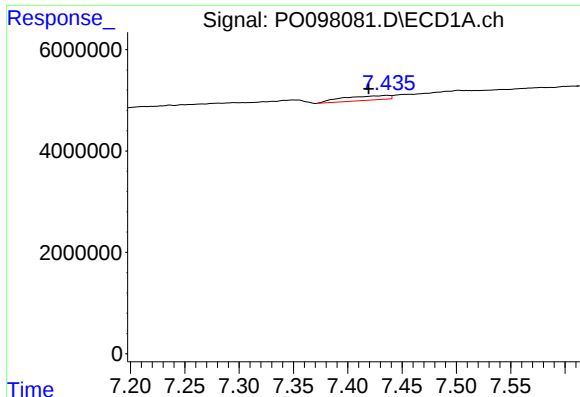

#29 AR-1254-4


R.T.: 7.436 min
Delta R.T.: 0.017 min
Response: 2685548
Conc: 24.82 ng/ml

Instrument :
FID_D
ClientSampleId :

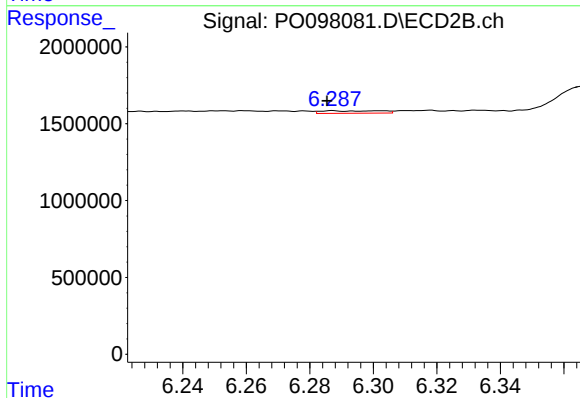


#29 AR-1254-4

R.T.: 6.287 min
Delta R.T.: 0.002 min
Response: 211255
Conc: 3.30 ng/ml

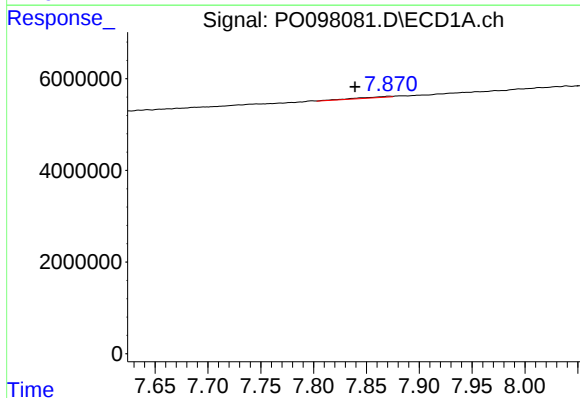


#30 AR-1254-5

R.T.: 7.871 min
Delta R.T.: 0.032 min
Response: 475675
Conc: 4.29 ng/ml

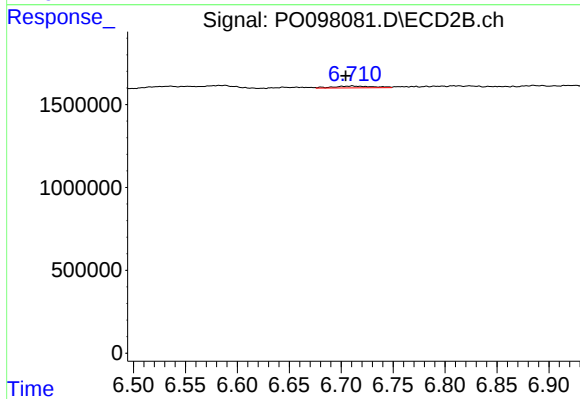

#30 AR-1254-5


R.T.: 6.711 min
Delta R.T.: 0.007 min
Response: 277268
Conc: 3.17 ng/ml

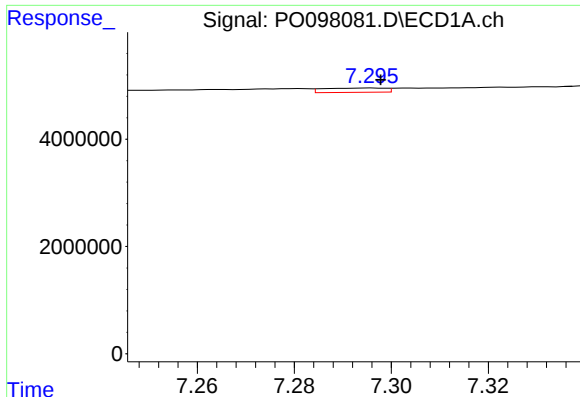

#31 AR-1260-1


R.T.: 7.296 min
Delta R.T.: -0.002 min
Response: 709745
Conc: 6.49 ng/ml

Instrument :
FID_D
ClientSampleId :

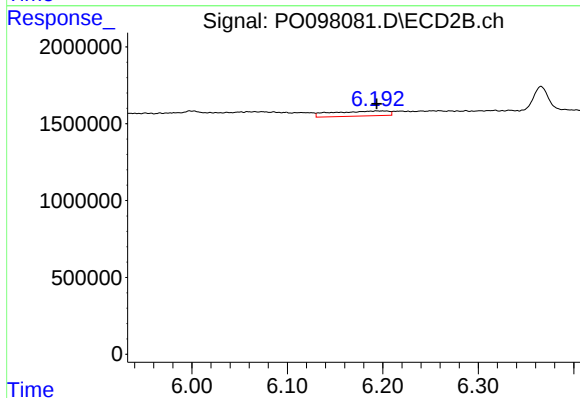


#31 AR-1260-1

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 1327236
Conc: 17.91 ng/ml

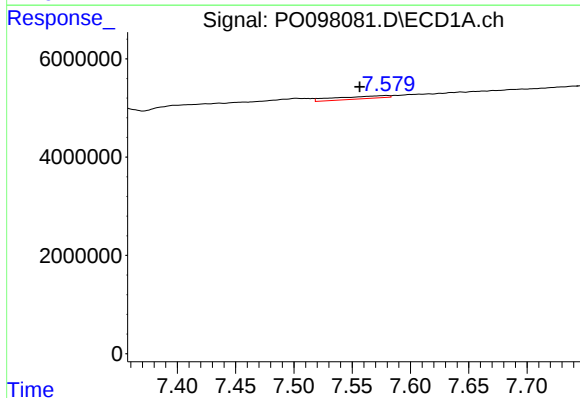


#32 AR-1260-2

R.T.: 7.579 min
Delta R.T.: 0.023 min
Response: 1758003
Conc: 13.99 ng/ml

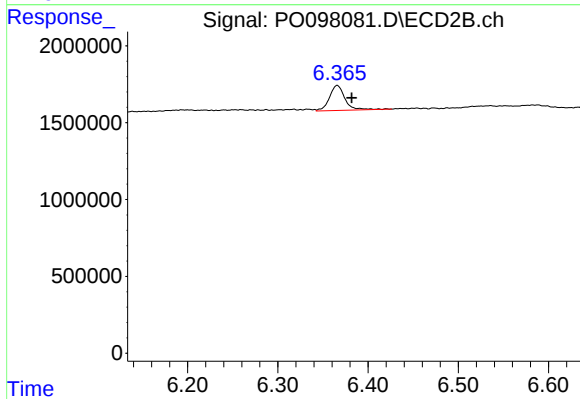

#32 AR-1260-2


R.T.: 6.366 min
Delta R.T.: -0.016 min
Response: 1968715
Conc: 22.81 ng/ml

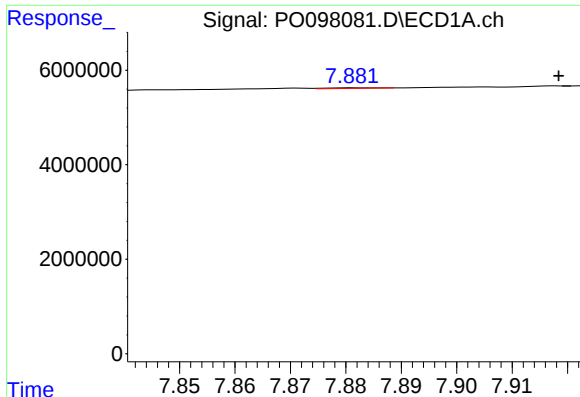

#33 AR-1260-3


R.T.: 7.883 min
Delta R.T.: -0.036 min
Response: 68873
Conc: 0.78 ng/ml

Instrument :
FID_D
ClientSampleId :

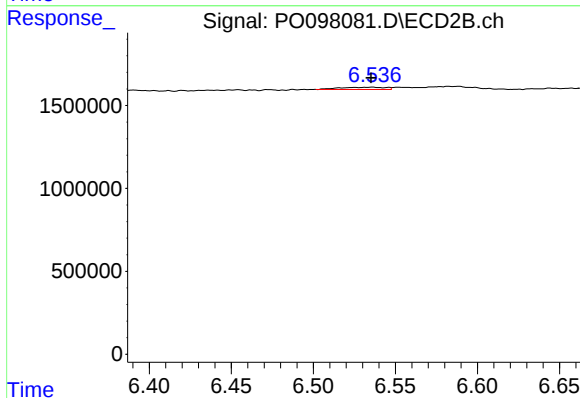


#33 AR-1260-3

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 252604
Conc: 3.11 ng/ml

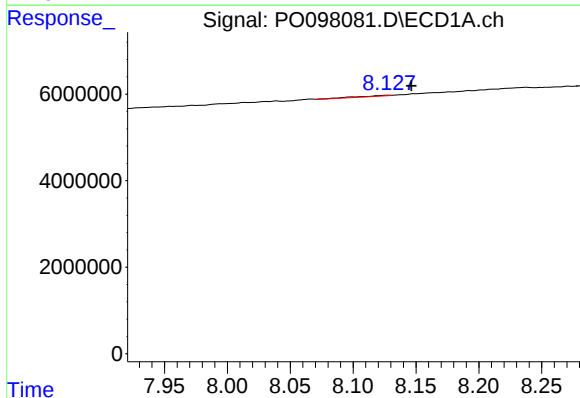


#34 AR-1260-4

R.T.: 8.127 min
Delta R.T.: -0.019 min
Response: 347229
Conc: 3.49 ng/ml

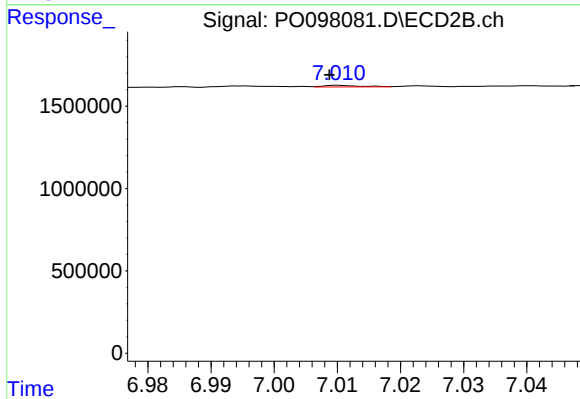

#34 AR-1260-4


R.T.: 7.010 min
Delta R.T.: 0.002 min
Response: 36731
Conc: 0.57 ng/ml

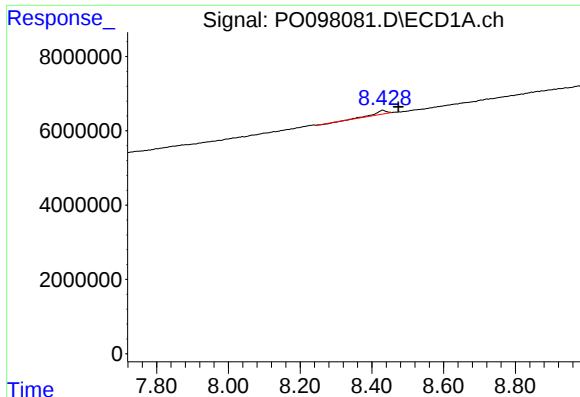

#35 AR-1260-5


R.T.: 8.430 min
Delta R.T.: -0.045 min
Response: 2196422
Conc: 10.84 ng/ml

Instrument :
FID_D
ClientSampleId :

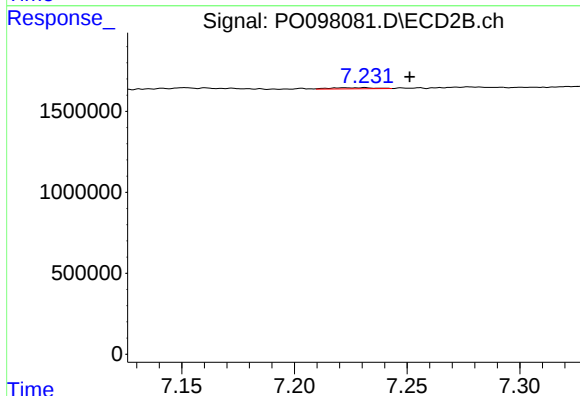


#35 AR-1260-5

R.T.: 7.231 min
Delta R.T.: -0.020 min
Response: 92633
Conc: 0.66 ng/ml

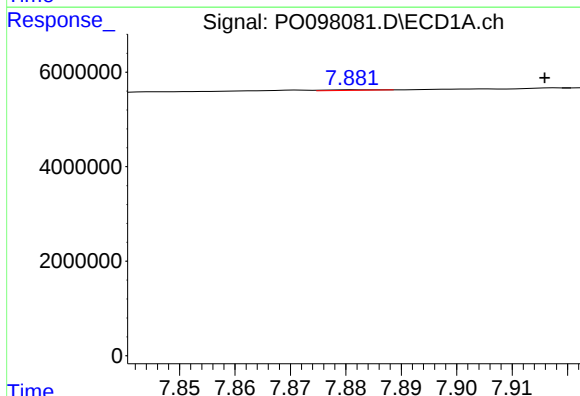


#36 AR-1262-1

R.T.: 7.883 min
Delta R.T.: -0.033 min
Response: 68873
Conc: 0.50 ng/ml

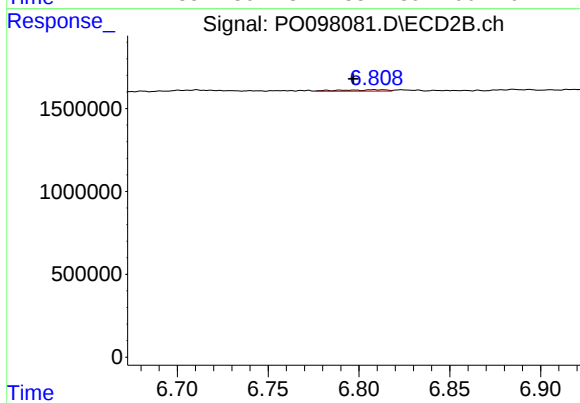

#36 AR-1262-1


R.T.: 6.808 min
Delta R.T.: 0.011 min
Response: 152261
Conc: 4.20 ng/ml

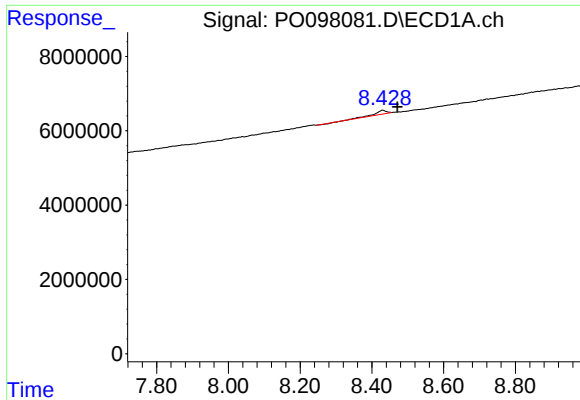

#37 AR-1262-2


R.T.: 8.430 min
Delta R.T.: -0.042 min
Response: 2196422
Conc: 9.22 ng/ml

Instrument :
FID_D
ClientSampleId :

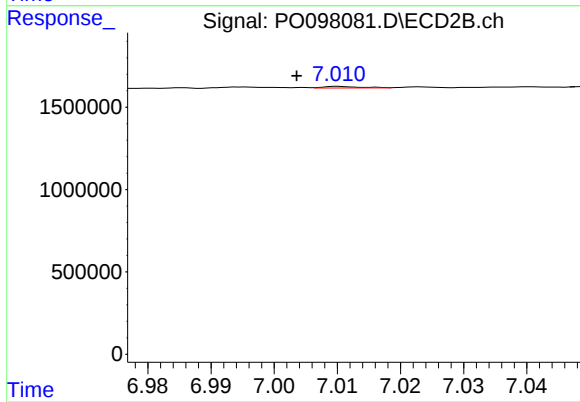


#37 AR-1262-2

R.T.: 7.010 min
Delta R.T.: 0.007 min
Response: 36731
Conc: 0.49 ng/ml

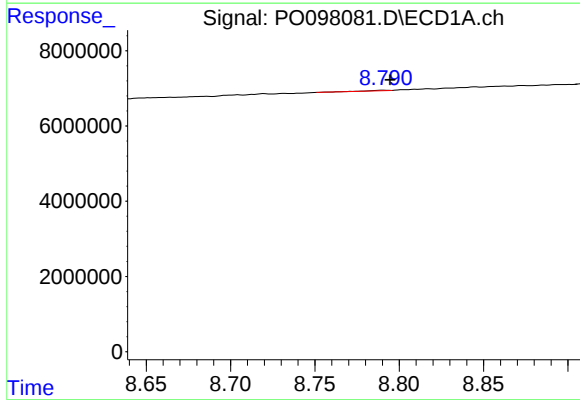


#38 AR-1262-3

R.T.: 8.791 min
Delta R.T.: -0.004 min
Response: 150974
Conc: 0.96 ng/ml

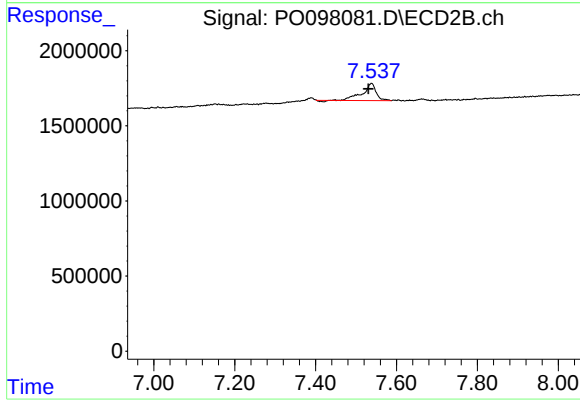

#38 AR-1262-3


R.T.: 7.538 min
Delta R.T.: 0.008 min
Response: 2692044
Conc: 45.40 ng/ml

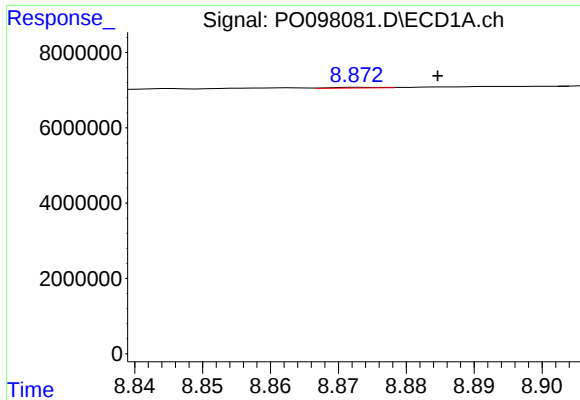

#39 AR-1262-4


R.T.: 8.873 min
Delta R.T.: -0.011 min
Response: 106637
Conc: 1.42 ng/ml

Instrument :
FID_D
ClientSampleId :

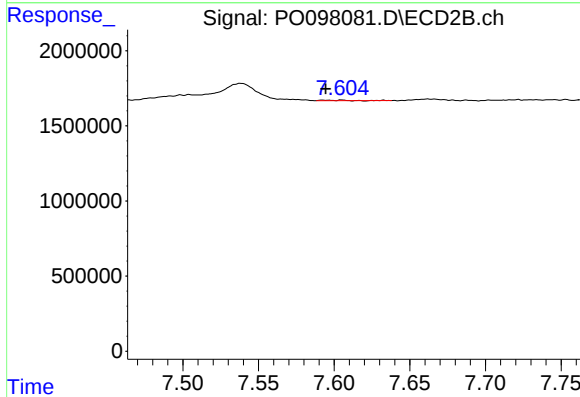


#39 AR-1262-4

R.T.: 7.592 min
Delta R.T.: -0.002 min
Response: 36300
Conc: 0.35 ng/ml

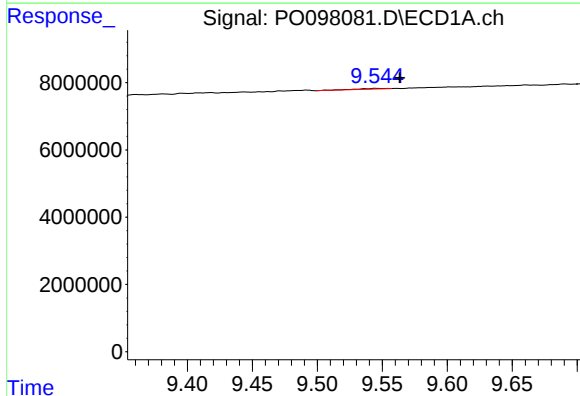


#40 AR-1262-5

R.T.: 9.545 min
Delta R.T.: -0.018 min
Response: 311942
Conc: 3.90 ng/ml

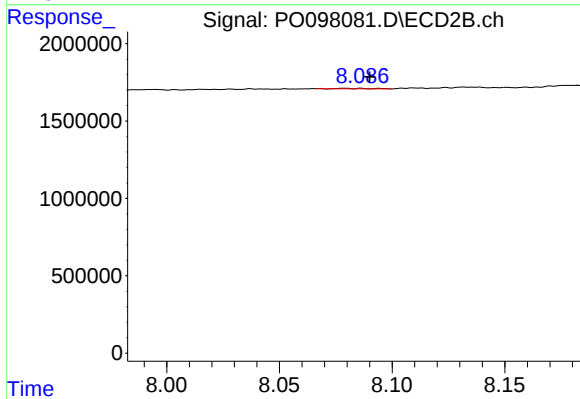

#40 AR-1262-5


R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 31506
Conc: 0.66 ng/ml

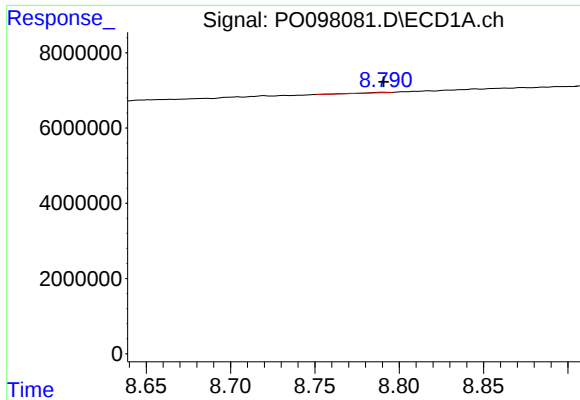

#41 AR-1268-1


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 150974
Conc: 0.55 ng/ml

Instrument :
FID_D
ClientSampleId :

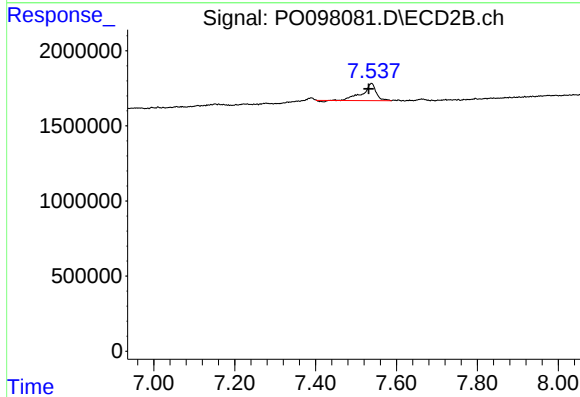


#41 AR-1268-1

R.T.: 7.538 min
Delta R.T.: 0.007 min
Response: 2692044
Conc: 15.40 ng/ml

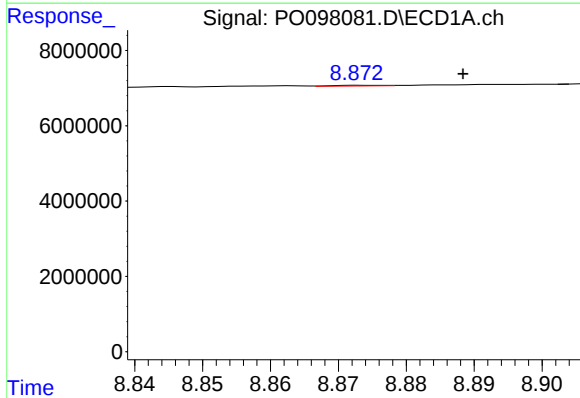


#42 AR-1268-2

R.T.: 8.873 min
Delta R.T.: -0.015 min
Response: 106637
Conc: 0.43 ng/ml

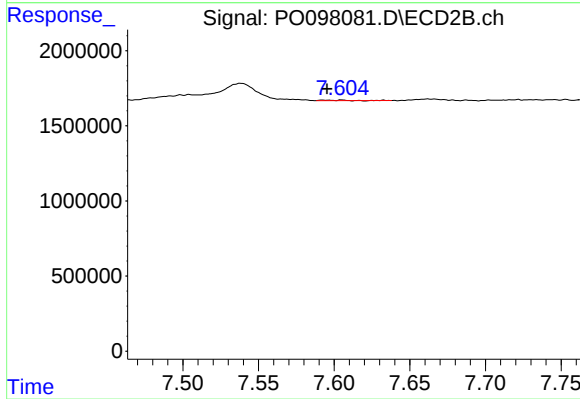

#42 AR-1268-2


R.T.: 7.592 min
Delta R.T.: -0.003 min
Response: 36300
Conc: 0.24 ng/ml

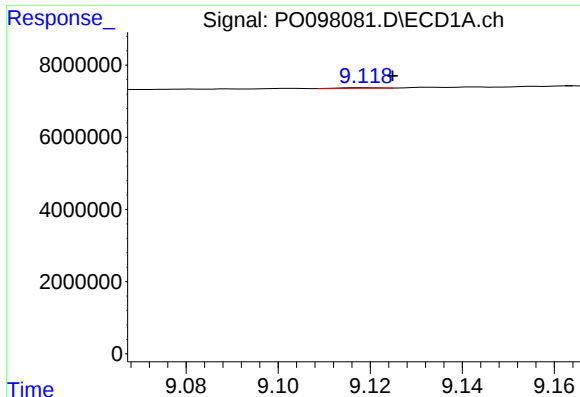

#43 AR-1268-3


R.T.: 9.118 min
Delta R.T.: -0.006 min
Response: 87500
Conc: 0.41 ng/ml

Instrument :
FID_D
ClientSampleId :

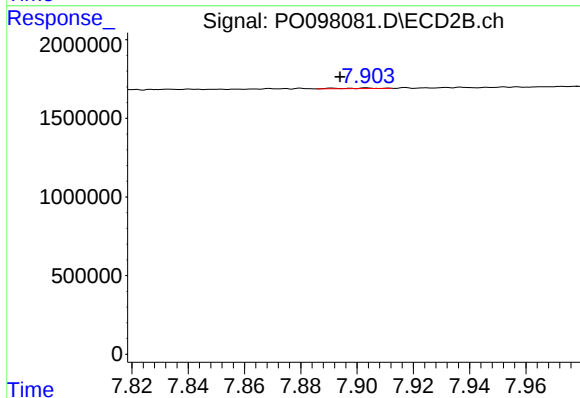


#43 AR-1268-3

R.T.: 7.903 min
Delta R.T.: 0.009 min
Response: 28887
Conc: 0.84 ng/ml

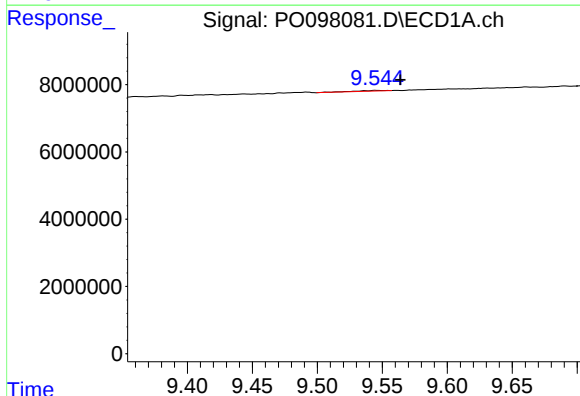


#44 AR-1268-4

R.T.: 9.545 min
Delta R.T.: -0.019 min
Response: 311942
Conc: 3.45 ng/ml

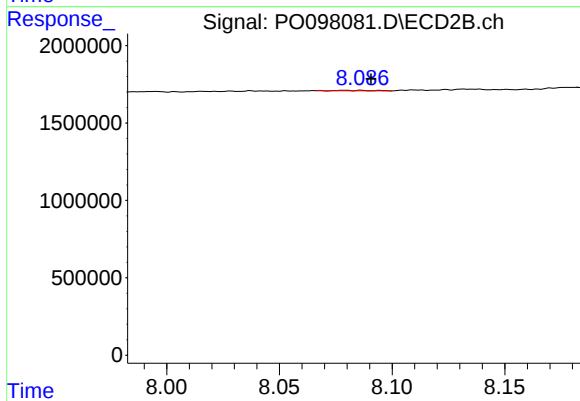

#44 AR-1268-4


R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 31506
Conc: 0.58 ng/ml

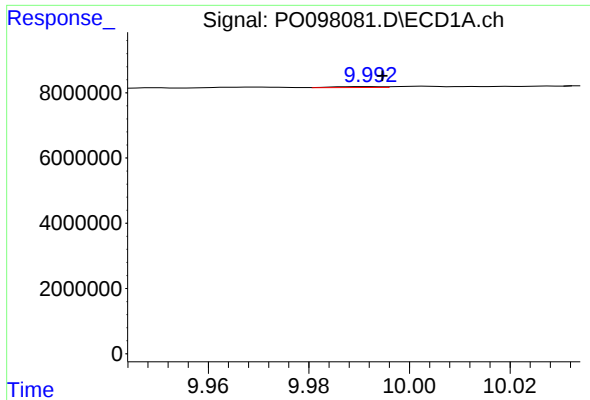

#45 AR-1268-5

R.T.: 9.992 min
Delta R.T.: -0.003 min
Response: 181474
Conc: 0.26 ng/ml

Instrument :
FID_D
ClientSampleId :

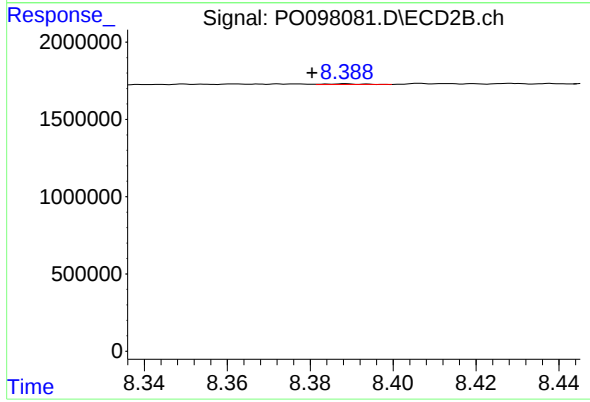

#45 AR-1268-5

R.T.: 8.388 min
Delta R.T.: 0.008 min
Response: 24091
Conc: 0.07 ng/ml