

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD091924AR\
Data File : FD048347.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2024 05:27
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 20 07:05:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 090624.M
Quant Title : GC Extractables
QLast Update : Fri Sep 06 11:53:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T benzo[b]fluoranthene ...	16.059	26639	0.179 ug/ml
17) T Bnezo[k]fluoranthene ...	16.059	26639	0.173 ug/ml
20) T Dibenz[a,h]anthracene...	17.824	198107	1.298 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD091924AR\
Data File : FD048347.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2024 05:27
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 20 07:05:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 090624.M
Quant Title : GC Extractables
QLast Update : Fri Sep 06 11:53:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

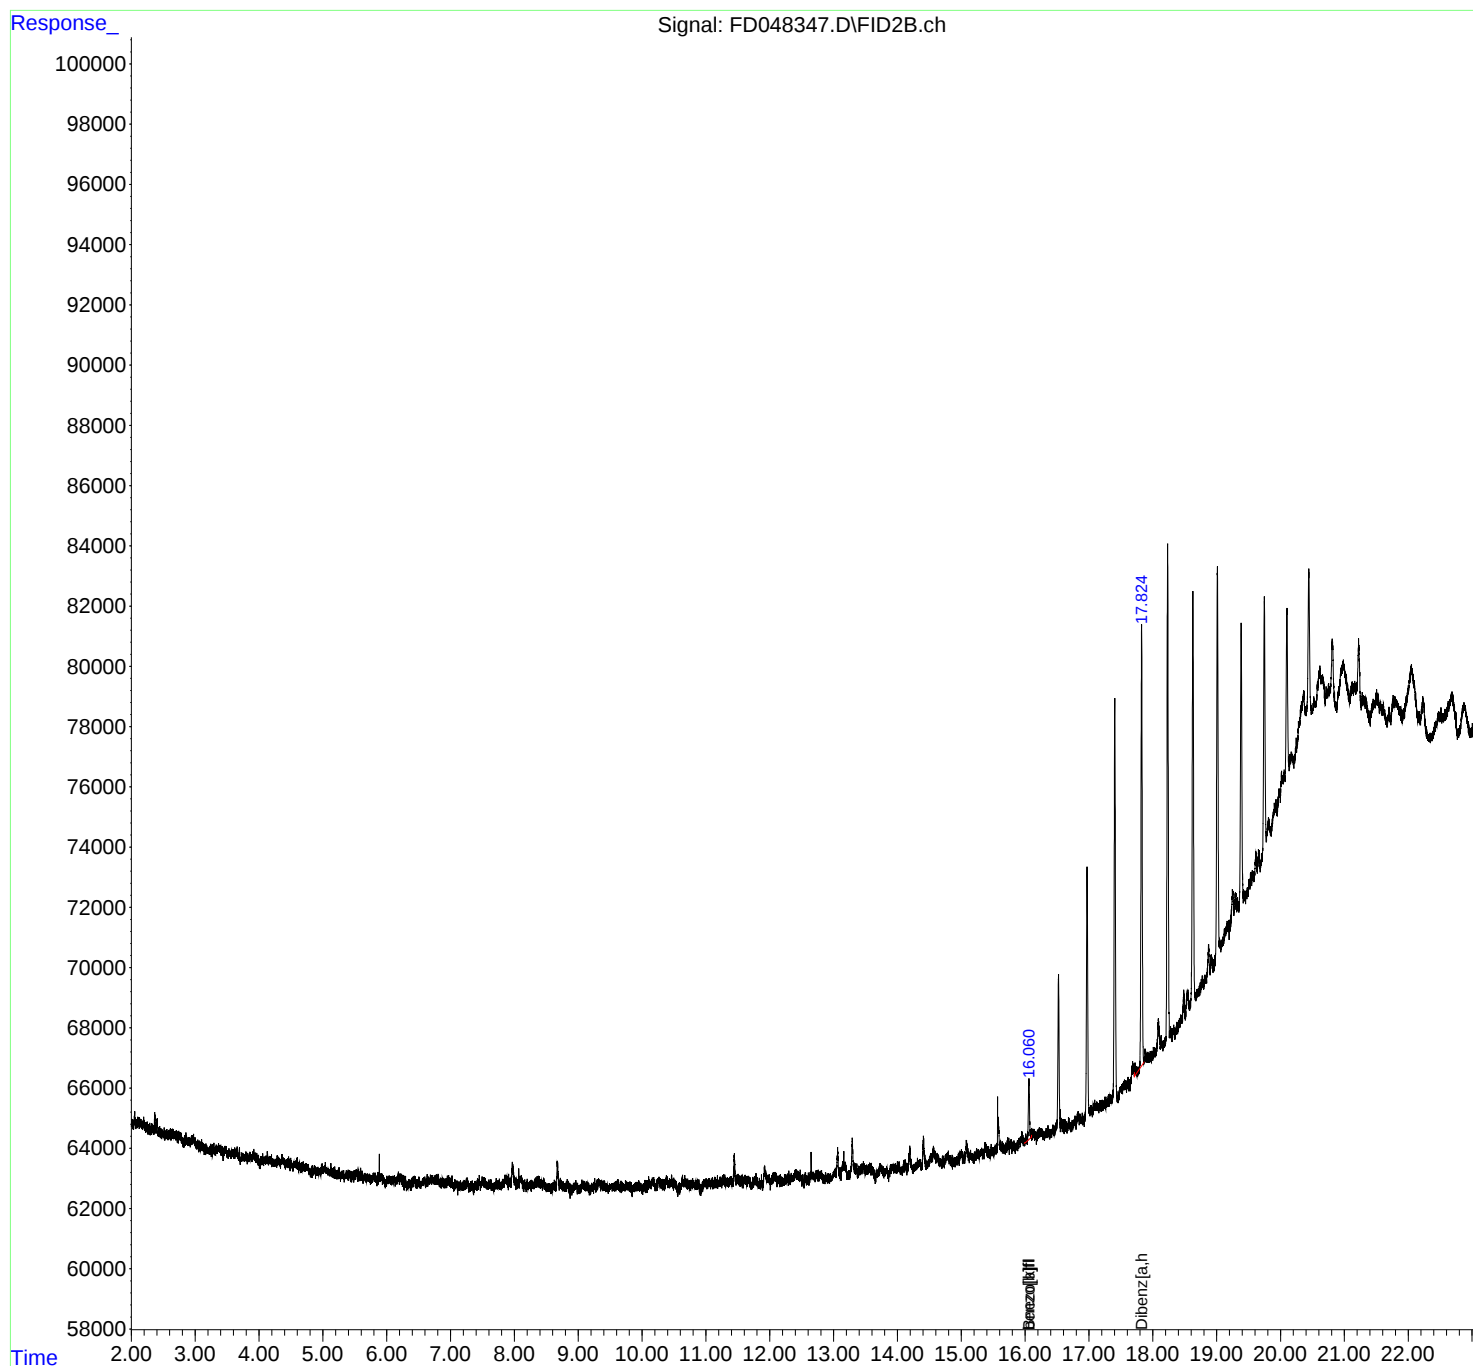


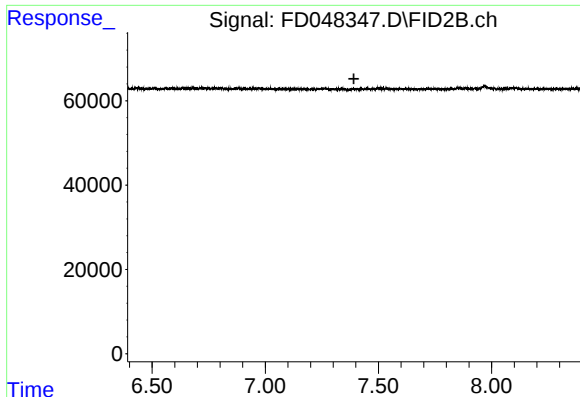

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

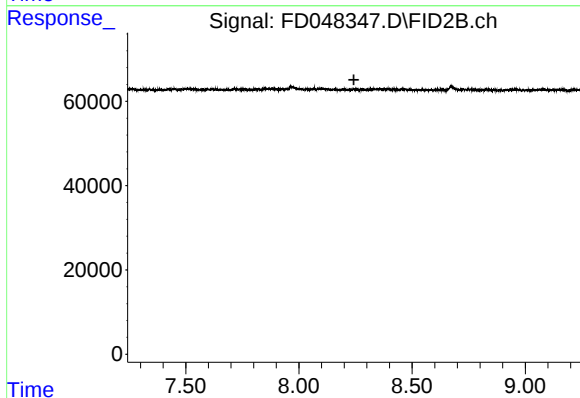


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

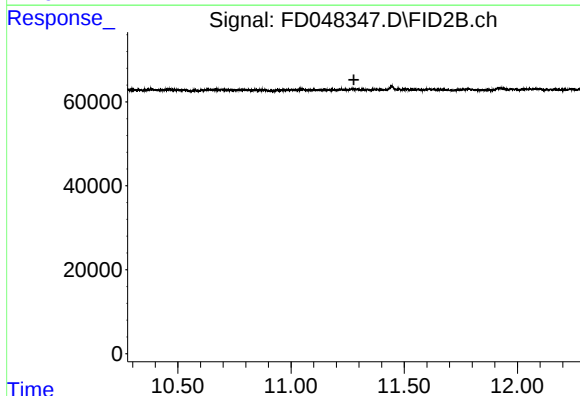


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.277 min
Response: 0
Conc: N.D.

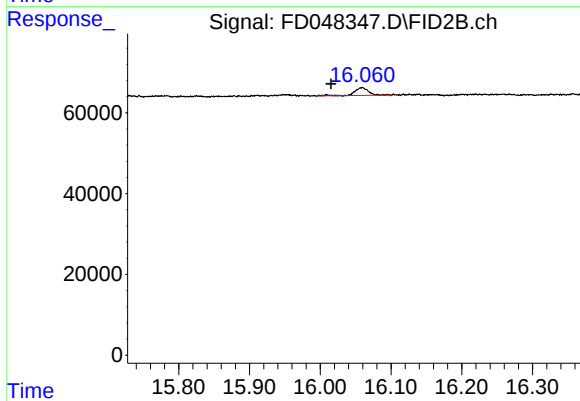

#16 benzo[b]fluoranthene (C30.41)


R.T.: 16.059 min
Delta R.T.: 0.044 min
Response: 26639
Conc: 0.18 ug/ml

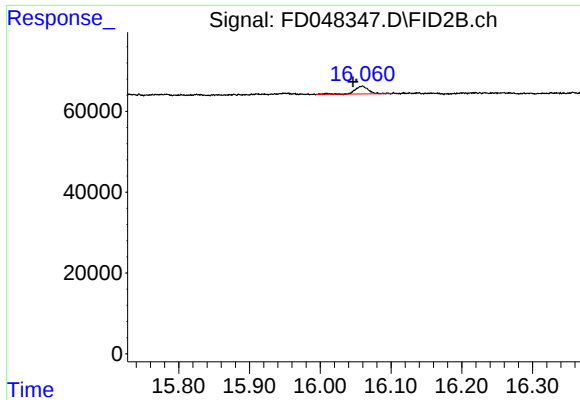

#17 Bnezo[k]fluoranthene (C30.14)

R.T.: 16.059 min
Delta R.T.: 0.013 min
Response: 26639
Conc: 0.17 ug/ml

Instrument :
FID_D
ClientSampleId :

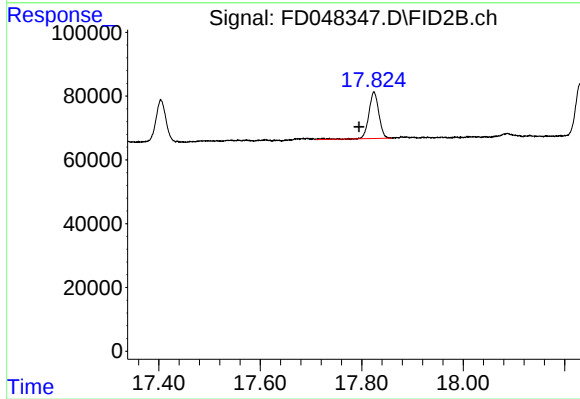

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.824 min
Delta R.T.: 0.030 min
Response: 198107
Conc: 1.30 ug/ml