

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD092723AR\
Data File : FD046600.D
Signal(s) : FID2B.ch
Acq On : 27 Sep 2023 10:57
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 27 12:16:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:47:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	Benzo[a]anthracene (C...	14.625	73189	0.524 ug/ml
15) T	Chrysene (C27.41)	14.625	73189	0.482 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD092723AR\
Data File : FD046600.D
Signal(s) : FID2B.ch
Acq On : 27 Sep 2023 10:57
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 27 12:16:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:47:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

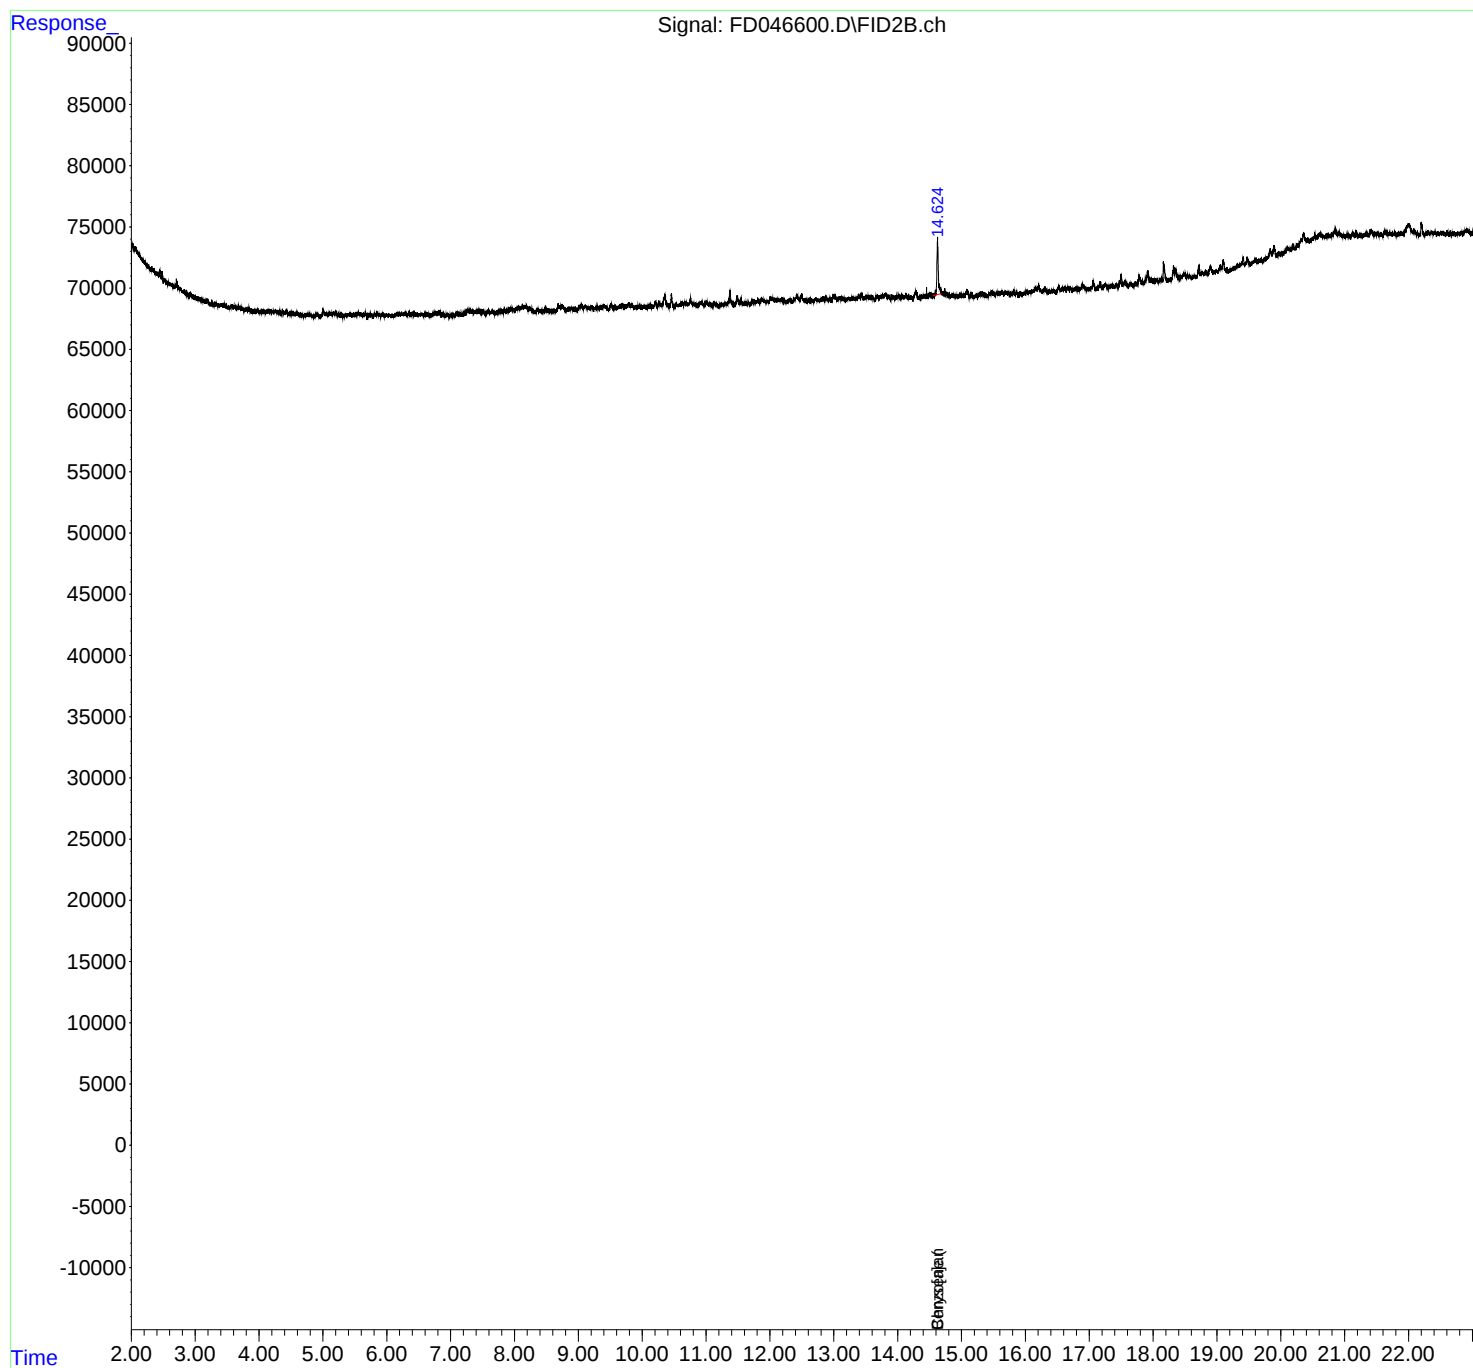


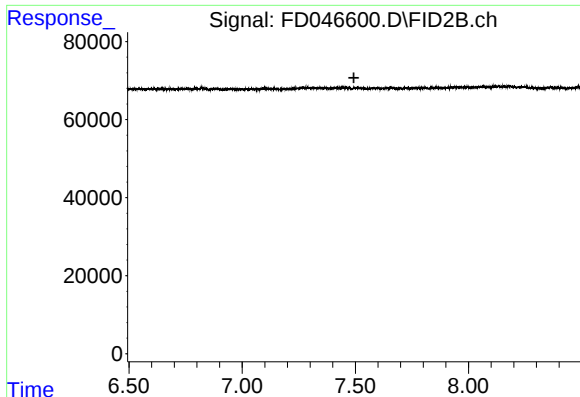

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

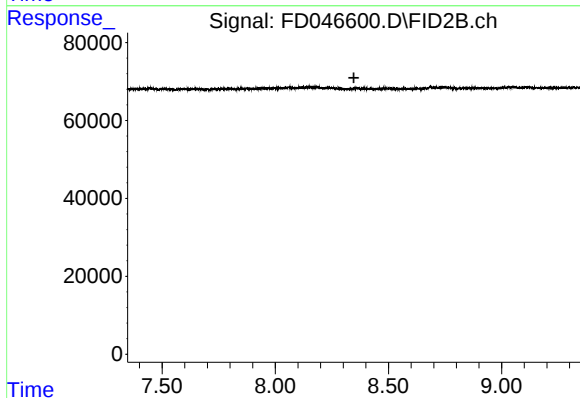


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.347 min
Response: 0
Conc: N.D.

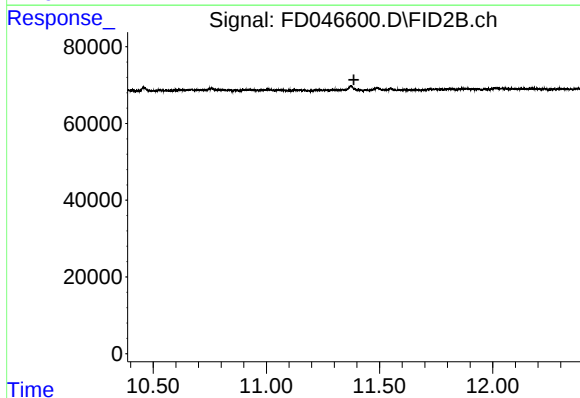


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.386 min
Response: 0
Conc: N.D.

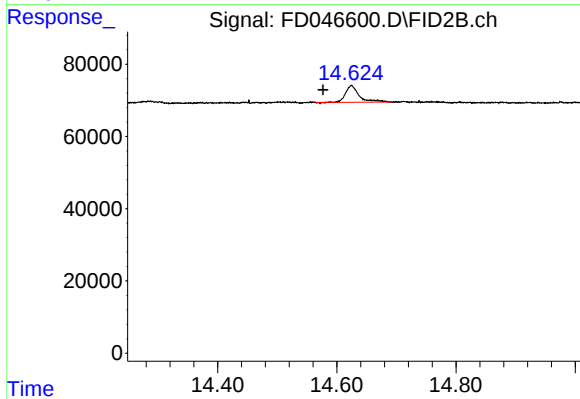

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.625 min
Delta R.T.: 0.048 min
Response: 73189
Conc: 0.52 ug/ml

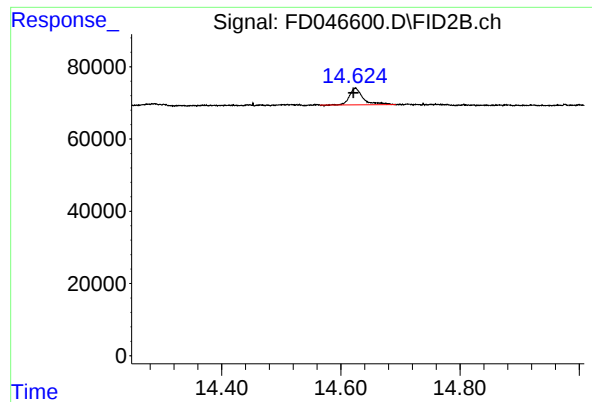

#15 Chrysene (C27.41)

R.T.: 14.625 min
Delta R.T.: 0.004 min
Response: 73189
Conc: 0.48 ug/ml

Instrument :

FID_D

ClientSampleId :