

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD100523AR\
 Data File : FD046650.D
 Signal(s) : FID2B.ch
 Acq On : 05 Oct 2023 06:34
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 05 23:51:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:47:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	Benzo[a]anthracene (C...	14.620	83856	0.601 ug/ml
15) T	Chrysene (C27.41)	14.620	83856	0.552 ug/ml
16) T	benzo[b]fluoranthene ...	16.148	59800	0.436 ug/ml
17) T	Bnezo[k]fluoranthene ...	16.148	59800	0.432 ug/ml
19) T	Indeno[1,2,3-cd]pyren...	17.908	132491	1.057 ug/ml
20) T	Dibenz[a,h]anthracene...	17.908	132491	0.996 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD100523AR\
Data File : FD046650.D
Signal(s) : FID2B.ch
Acq On : 05 Oct 2023 06:34
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 23:51:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:47:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

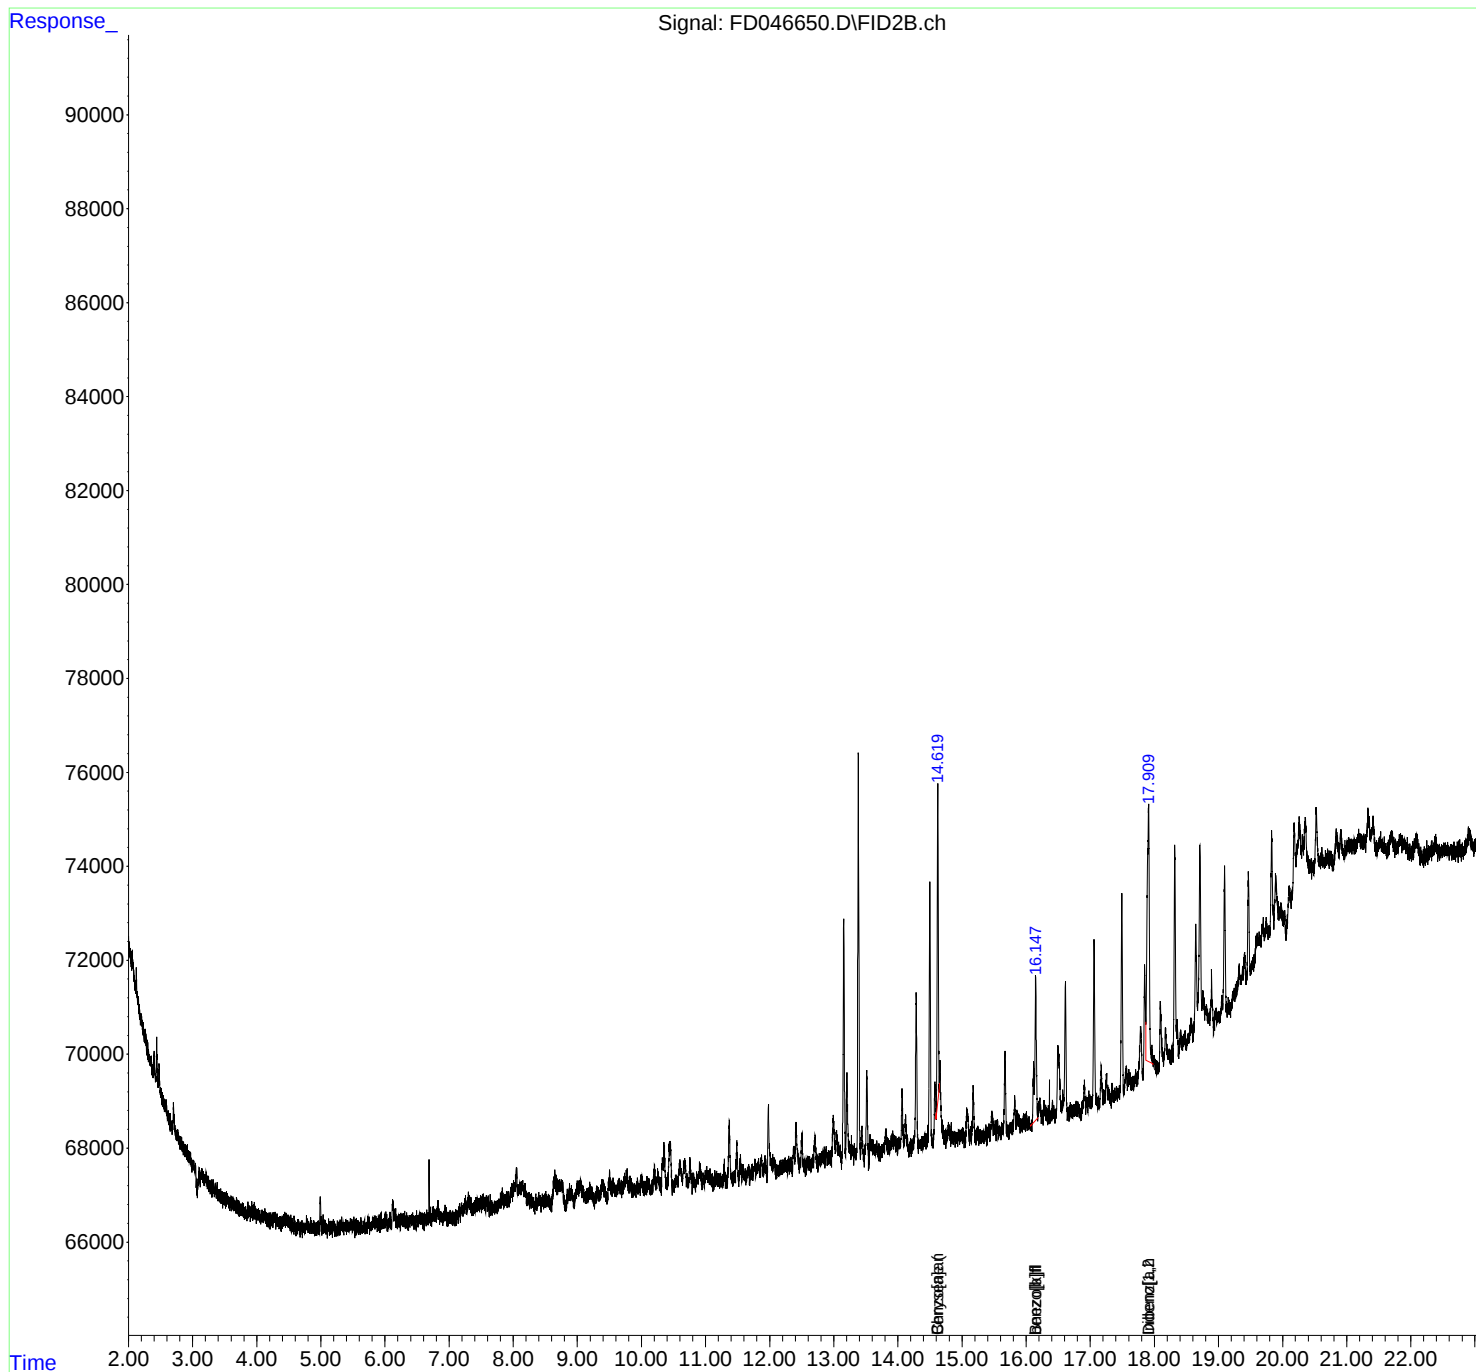


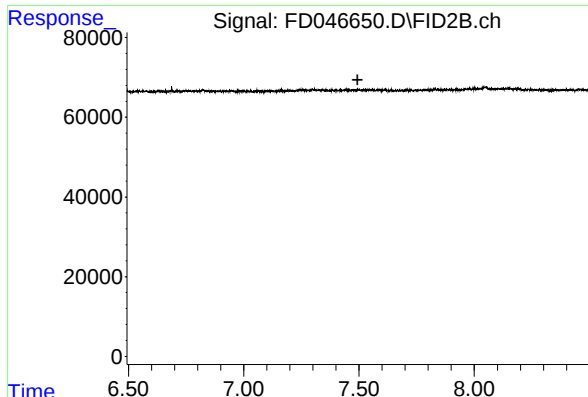

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.494 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

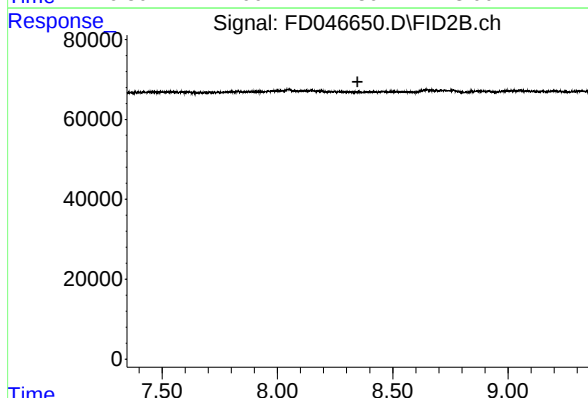


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.347 min
Response: 0
Conc: N.D.

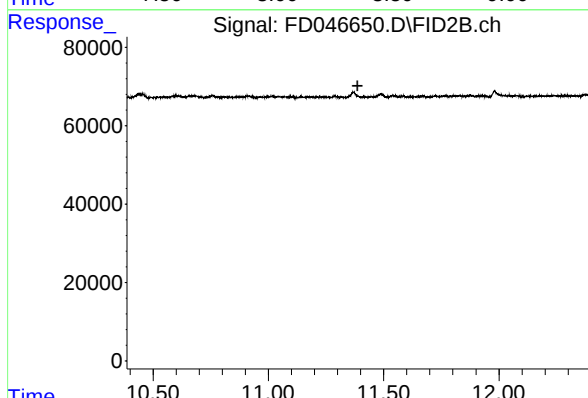


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.386 min
Response: 0
Conc: N.D.

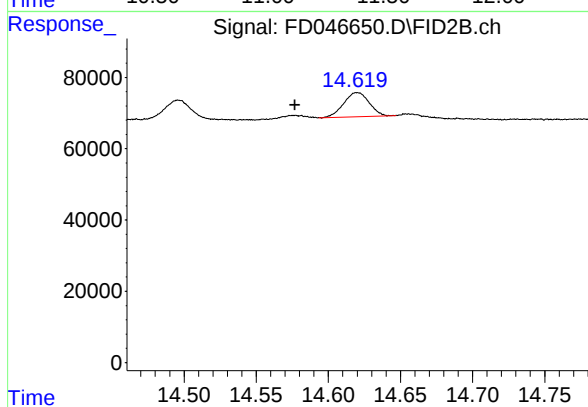

#14 Benzo[a]anthracene (C26.37)


R.T.: 14.620 min
Delta R.T.: 0.043 min
Response: 83856
Conc: 0.60 ug/ml

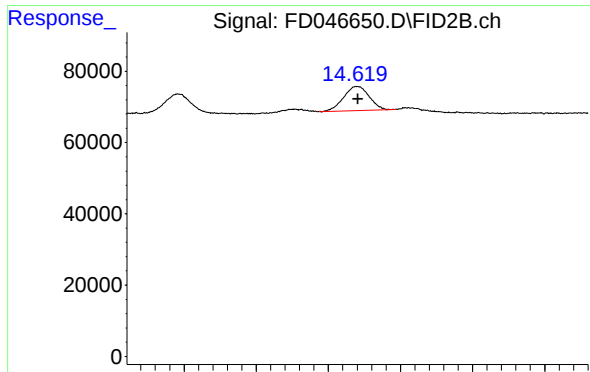

#15 Chrysene (C27.41)


R.T.: 14.620 min
Delta R.T.: 0.000 min
Response: 83856
Conc: 0.55 ug/ml

Instrument :
FID_D
ClientSampleId :

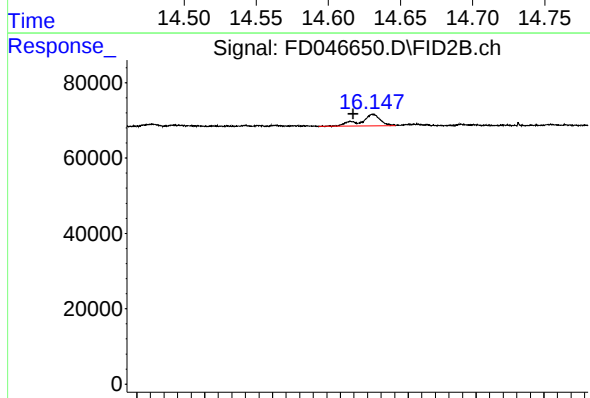


#16 benzo[b]fluoranthene (C30.41)

R.T.: 16.148 min
Delta R.T.: 0.029 min
Response: 59800
Conc: 0.44 ug/ml

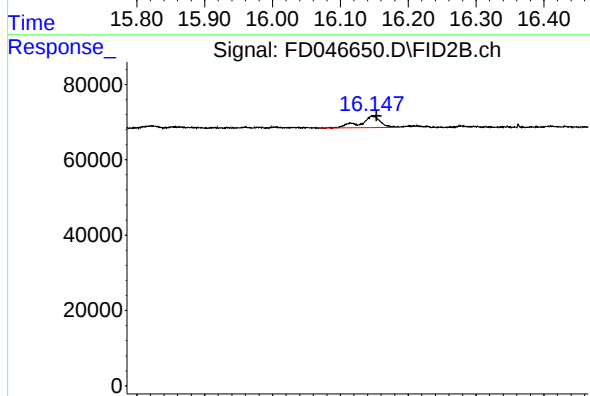


#17 Bnezo[k]fluoranthene (C30.14)

R.T.: 16.148 min
Delta R.T.: -0.006 min
Response: 59800
Conc: 0.43 ug/ml

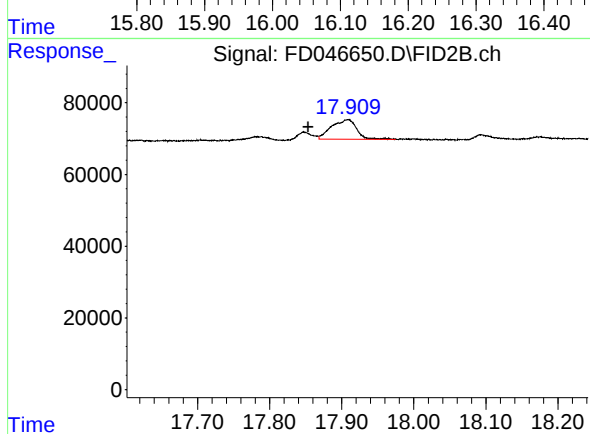

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.908 min
Delta R.T.: 0.055 min
Response: 132491
Conc: 1.06 ug/ml

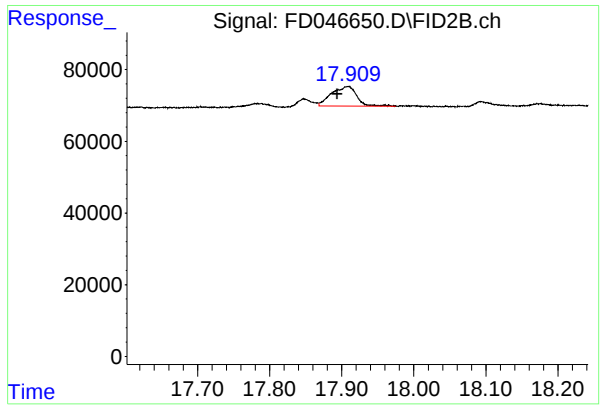

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.908 min

Delta R.T.: 0.014 min

Response: 132491

Conc: 1.00 ug/ml

Instrument :

FID_D

ClientSampleId :