

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD101023AL\
Data File : FD046706.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 07:40
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 00:21:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 05:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.621	225022	1.228 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD101023AL\
Data File : FD046706.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 07:40
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 00:21:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 05:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

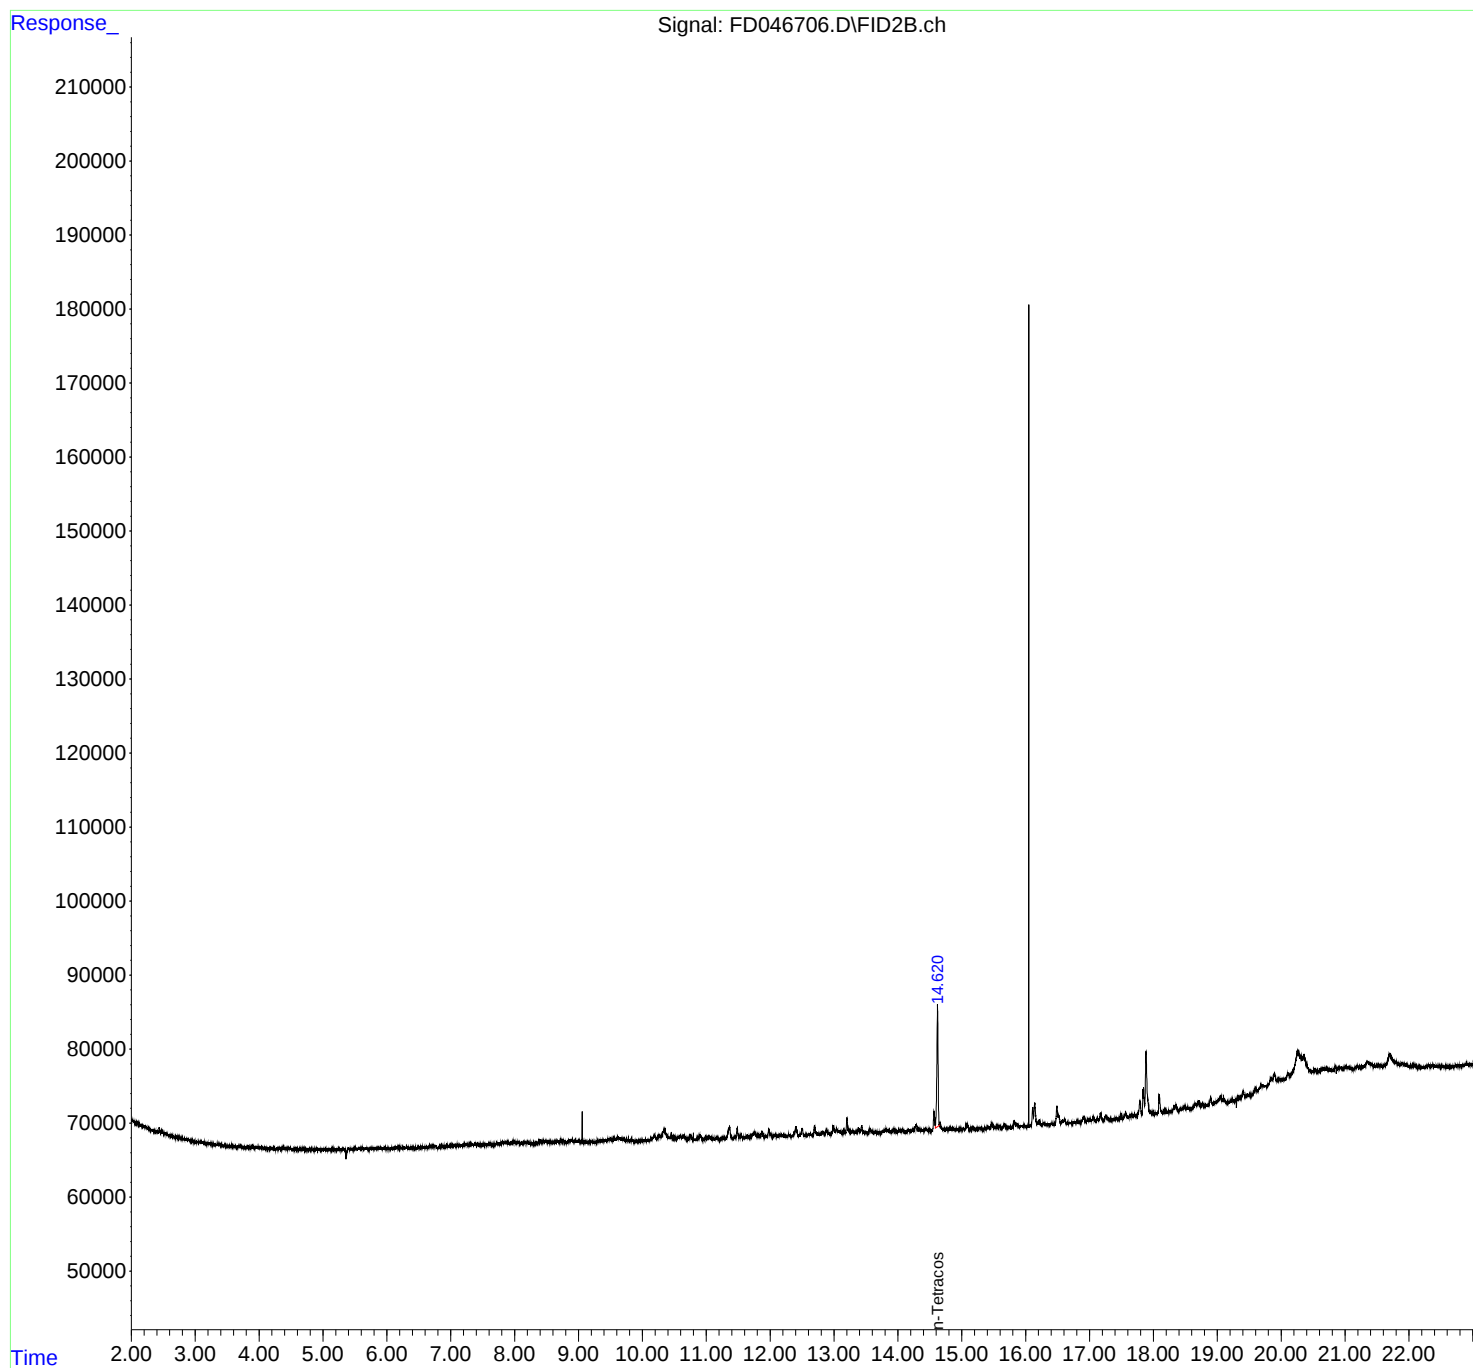


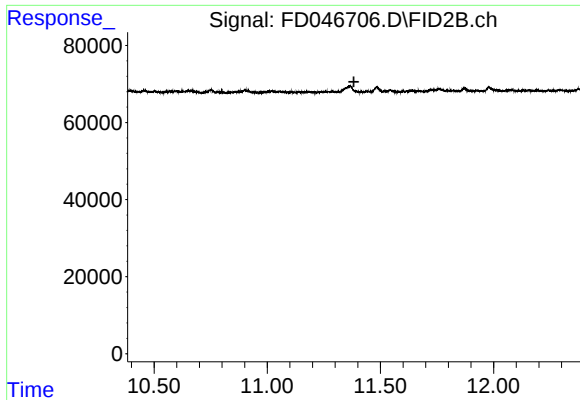

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T. : 11.383 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

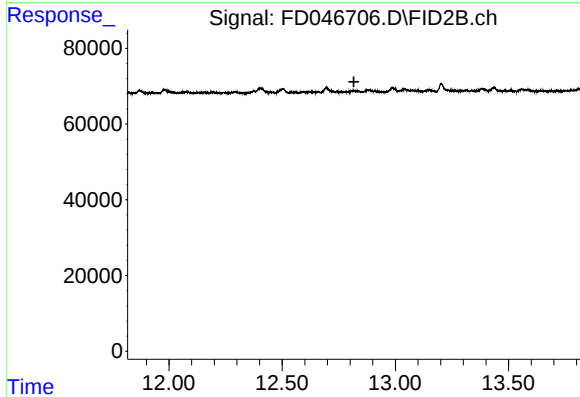

#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T. : 12.817 min
Response: 0
Conc: N.D.

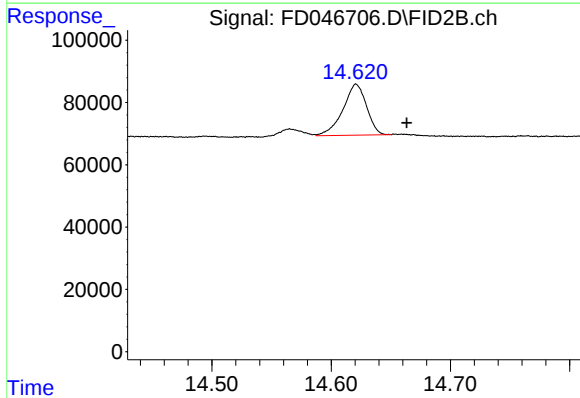

#14 n-Tetracosane (C24)

R.T.: 14.621 min
Delta R.T.: -0.043 min
Response: 225022
Conc: 1.23 ug/ml