

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD101023AR\
Data File : FD046723.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 19:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 02:54:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 02:49:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T Benzo[a]anthracene (C...	14.501f	57929	0.396 ug/ml
20) T Dibenz[a,h]anthracene...	17.912	65398	0.463 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD101023AR\
Data File : FD046723.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 19:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 02:54:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 02:49:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

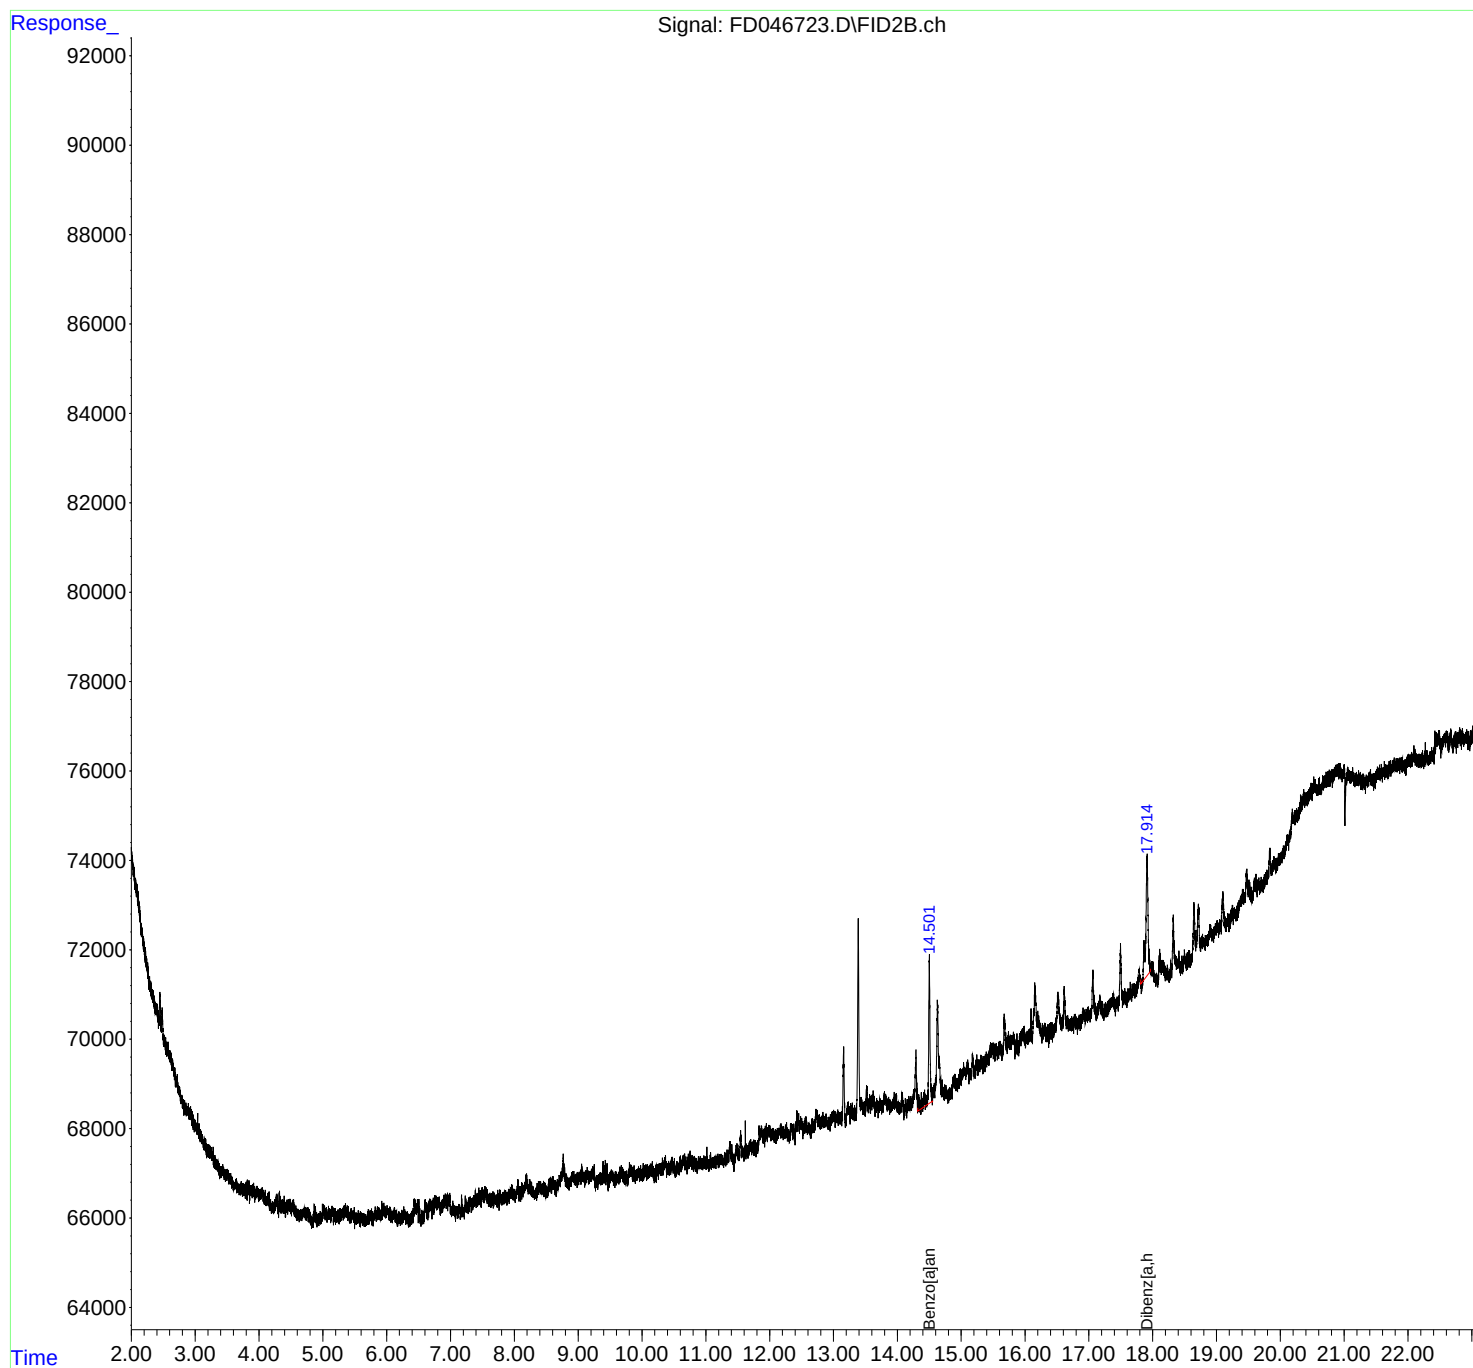


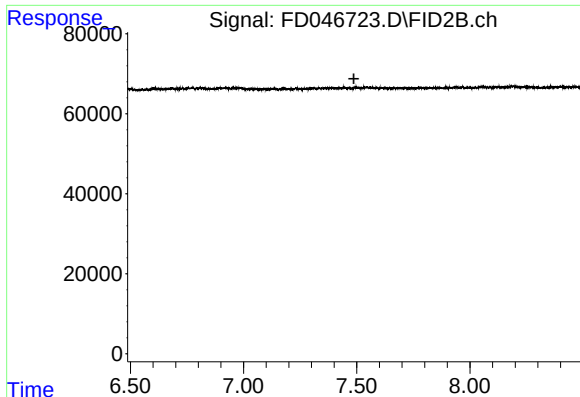

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

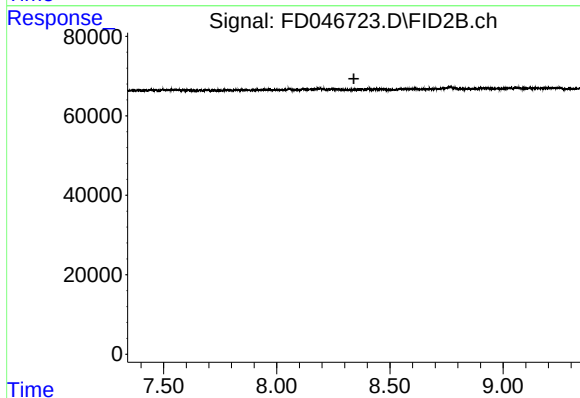


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

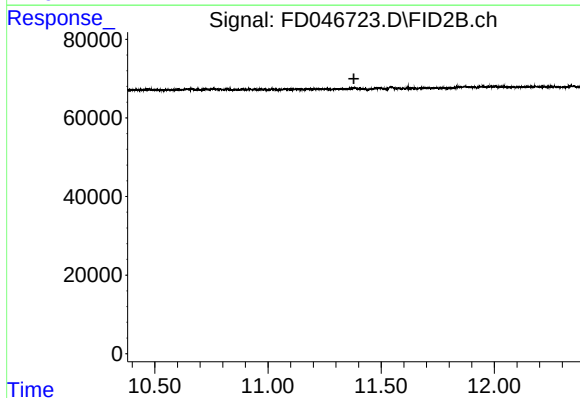


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.379 min
Response: 0
Conc: N.D.

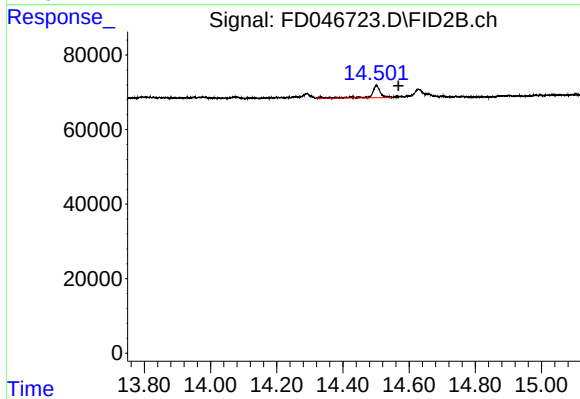

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.501 min
Delta R.T.: -0.066 min
Response: 57929
Conc: 0.40 ug/ml

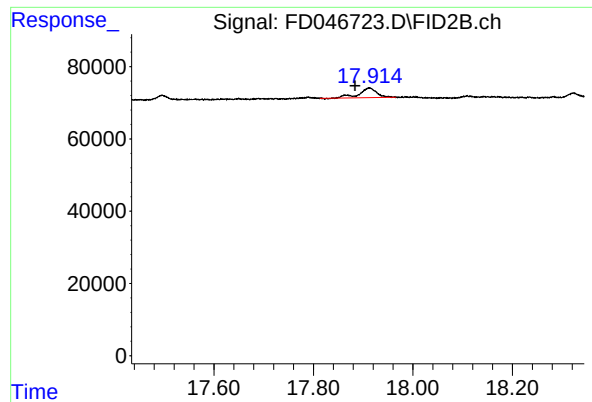

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.912 min
Delta R.T.: 0.029 min
Response: 65398
Conc: 0.46 ug/ml

Instrument :

FID_D

ClientSampleId :