

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD101323AR\
Data File : FD046760.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2023 06:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 07:04:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 02:49:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	Benzo[a]anthracene (C...	14.626f	43769	0.299 ug/ml
15) T	Chrysene (C27.41)	14.626	43769	0.272 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD101323AR\
Data File : FD046760.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2023 06:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 07:04:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 02:49:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

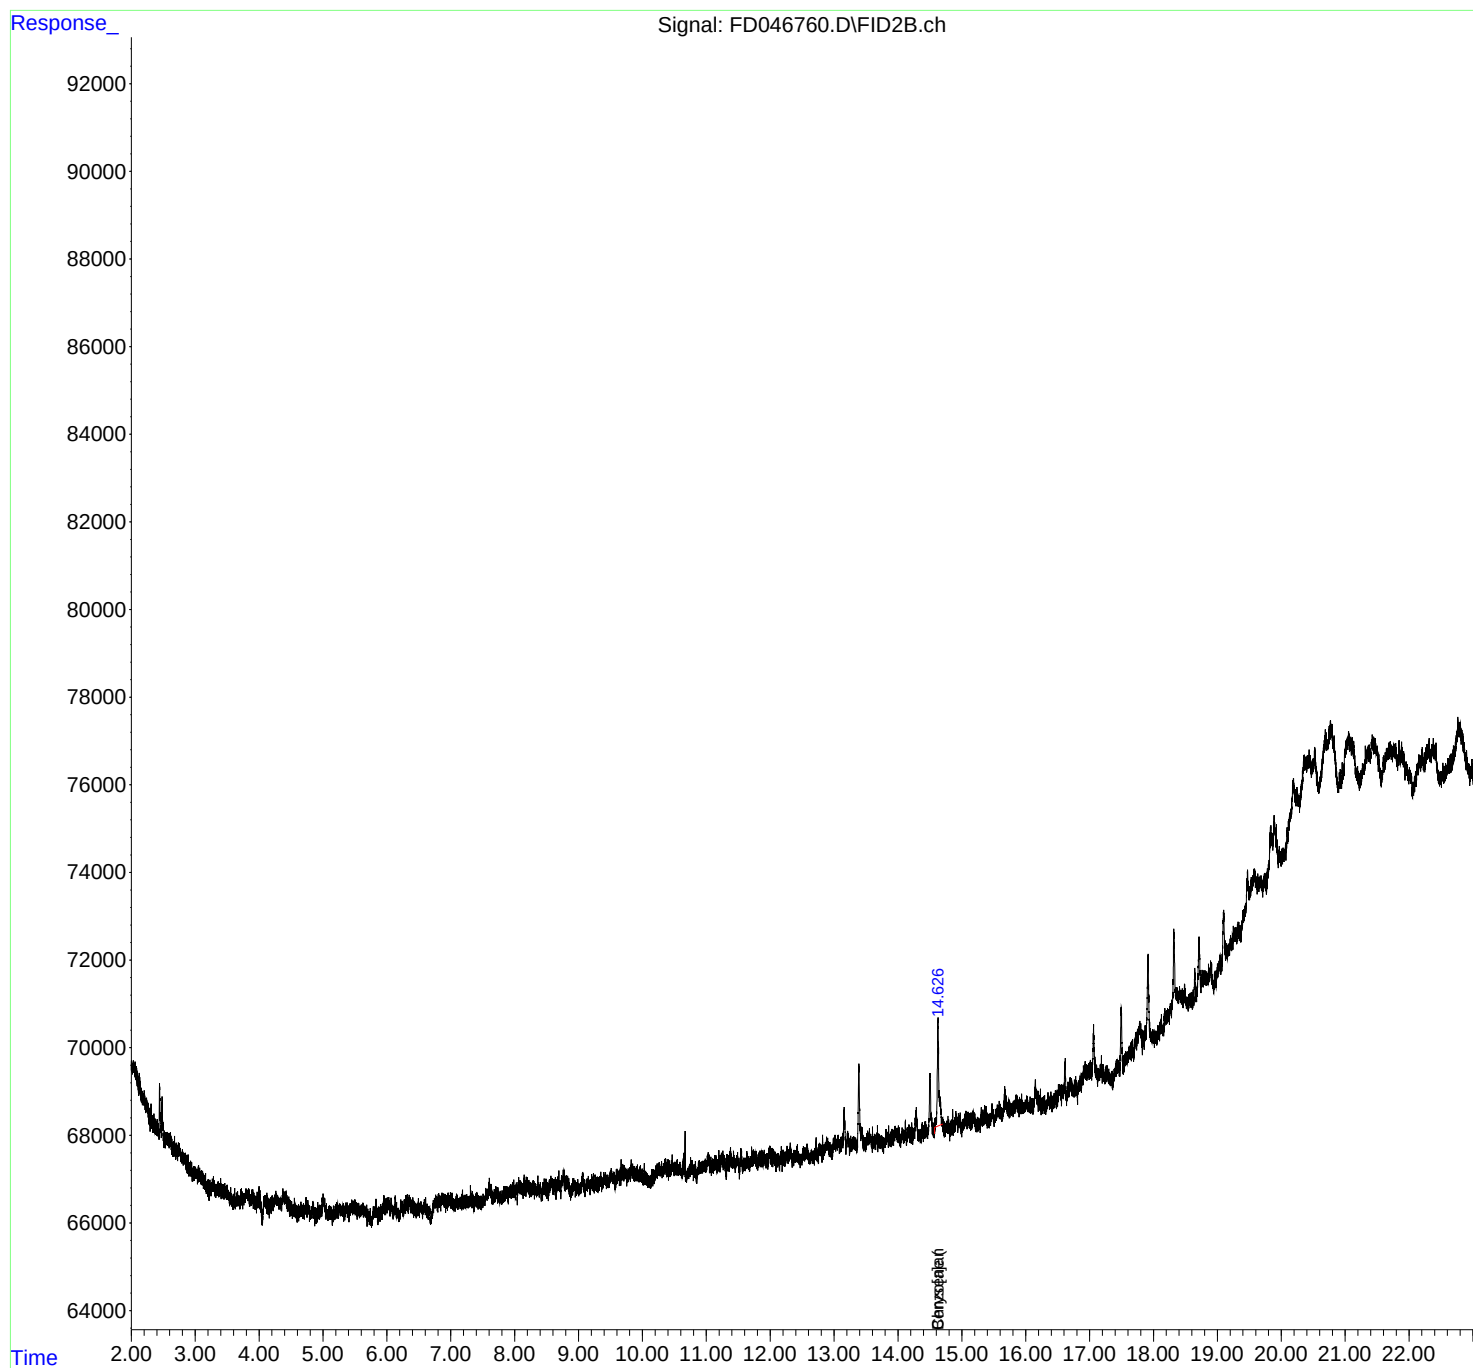


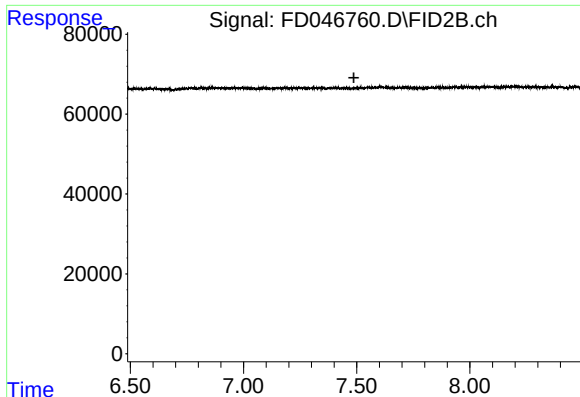

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T.: 7.488 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

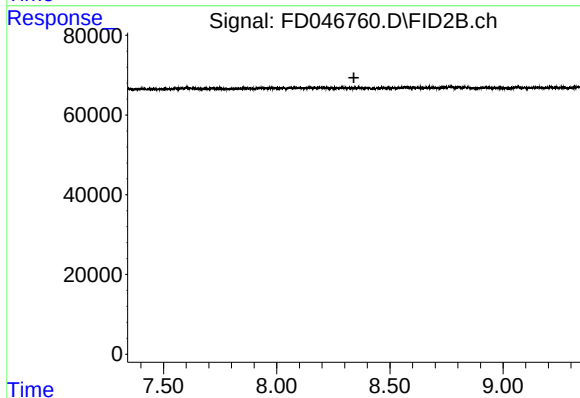


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 8.341 min
Response: 0
Conc: N.D.

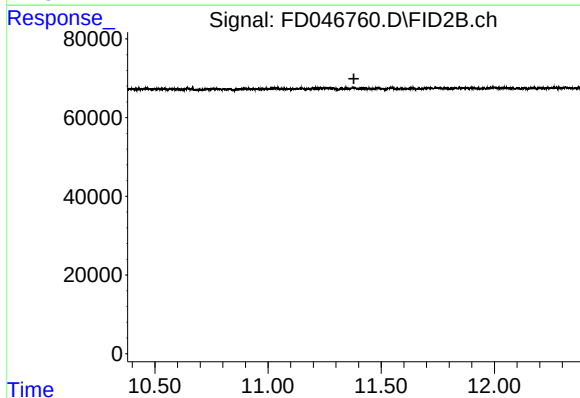


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.379 min
Response: 0
Conc: N.D.

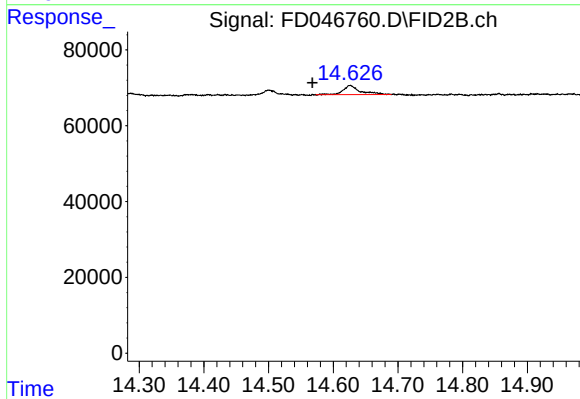

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.626 min
Delta R.T.: 0.059 min
Response: 43769
Conc: 0.30 ug/ml

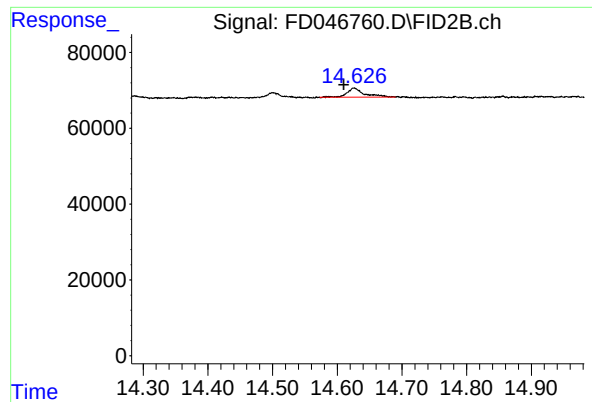

#15 Chrysene (C27.41)

R.T.: 14.626 min
Delta R.T.: 0.016 min
Response: 43769
Conc: 0.27 ug/ml

Instrument :

FID_D

ClientSampleId :