

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110420AL\
 Data File : FD035310.D
 Signal(s) : FID2B.CH
 Acq On : 04 Nov 2020 15:23
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 00:36:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 11:48:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	13.718	103144	0.836 ug/ml
14) T	n-Tetracosane (C24)	14.816	242203	1.958 ug/ml
15) T	n-Hexacosane (C26)	15.832	289659	2.353 ug/ml
16) T	n-Octacosane (C28)	16.778	303933	2.469 ug/ml
17) T	n-Tricontane (C30)	17.660	274412	2.271 ug/ml
18) T	n-Dotriacontane (C32)	18.488	244805	2.177 ug/ml
19) T	n-Tetratriacontane (C34)	19.267	87153	0.830 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110420AL\
Data File : FD035310.D
Signal(s) : FID2B.CH
Acq On : 04 Nov 2020 15:23
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 00:36:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 11:48:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

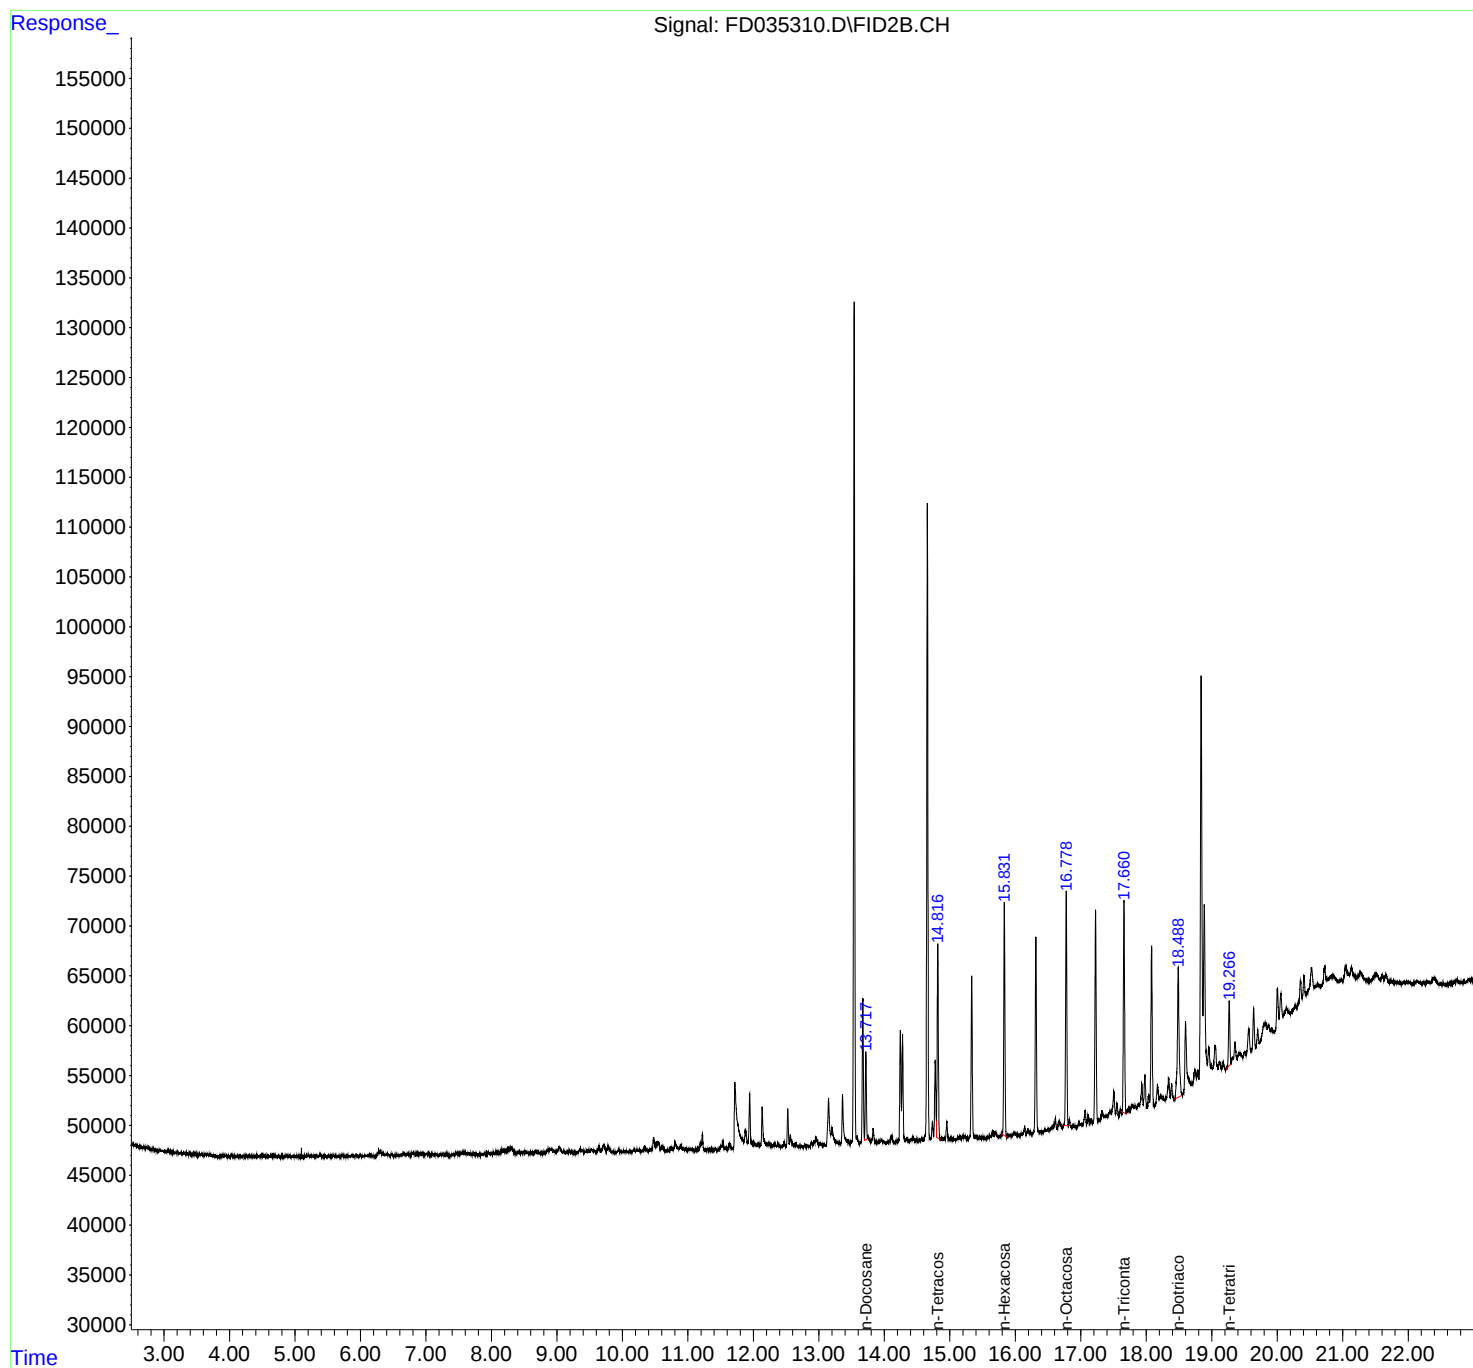


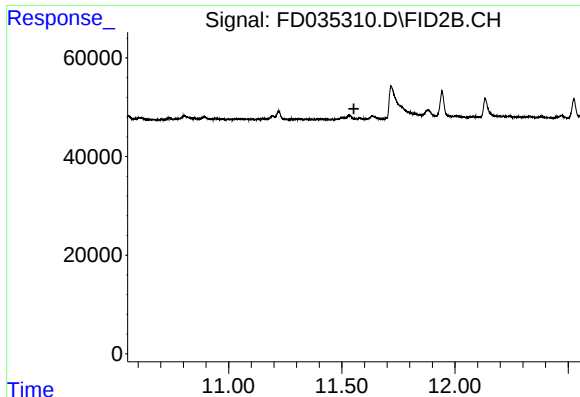

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.553 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

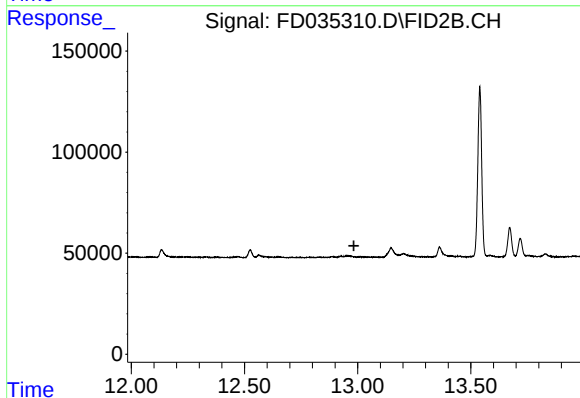


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.983 min
Response: 0
Conc: N.D.

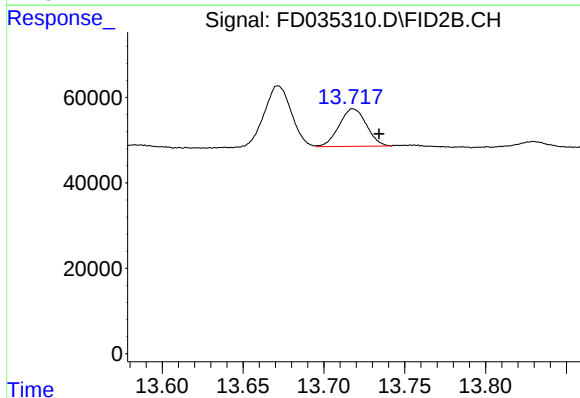


#13 n-Docosane (C22)

R.T.: 13.718 min
Delta R.T.: -0.016 min
Response: 103144
Conc: 0.84 ug/ml

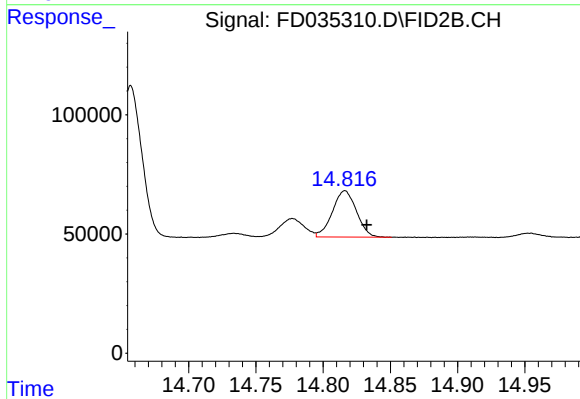

#14 n-Tetracosane (C24)


R.T.: 14.816 min
Delta R.T.: -0.016 min
Response: 242203
Conc: 1.96 ug/ml

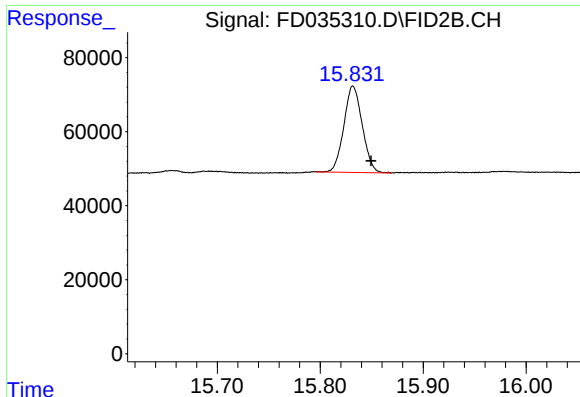

#15 n-Hexacosane (C26)


R.T.: 15.832 min
Delta R.T.: -0.018 min
Response: 289659
Conc: 2.35 ug/ml

Instrument :
FID_D
ClientSampleId :

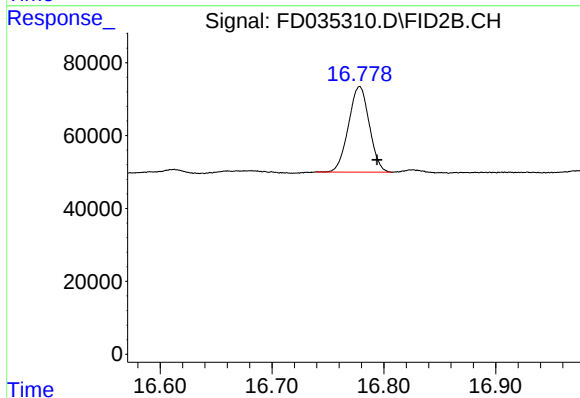


#16 n-Octacosane (C28)

R.T.: 16.778 min
Delta R.T.: -0.016 min
Response: 303933
Conc: 2.47 ug/ml

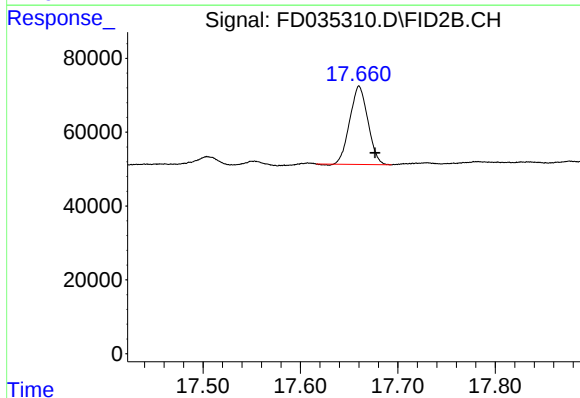


#17 n-Tricontane (C30)

R.T.: 17.660 min
Delta R.T.: -0.016 min
Response: 274412
Conc: 2.27 ug/ml

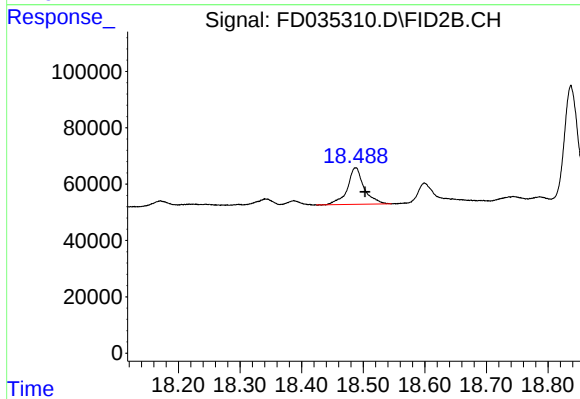

#18 n-Dotriacontane (C32)

R.T.: 18.488 min
Delta R.T.: -0.015 min
Response: 244805
Conc: 2.18 ug/ml

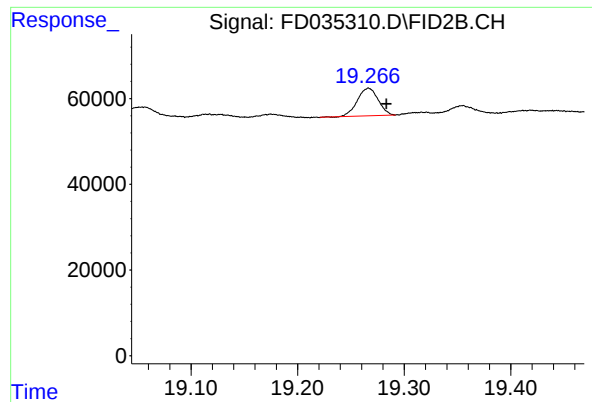

#19 n-Tetratriacontane (C34)

R.T.: 19.267 min
Delta R.T.: -0.017 min
Response: 87153
Conc: 0.83 ug/ml

Instrument :
FID_D
ClientSampleId :