

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110420AL\
 Data File : FD035311.D
 Signal(s) : FID2B.CH
 Acq On : 04 Nov 2020 16:00
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 00:36:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 11:48:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	13.720	101028	0.819 ug/ml
14) T	n-Tetracosane (C24)	14.817	241066	1.949 ug/ml
15) T	n-Hexacosane (C26)	15.834	292844	2.379 ug/ml
16) T	n-Octacosane (C28)	16.778	307781	2.500 ug/ml
17) T	n-Tricontane (C30)	17.660	280144	2.318 ug/ml
18) T	n-Dotriacontane (C32)	18.489	230578	2.051 ug/ml
19) T	n-Tetratriacontane (C34)	19.266	88372	0.842 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110420AL\
Data File : FD035311.D
Signal(s) : FID2B.CH
Acq On : 04 Nov 2020 16:00
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 00:36:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 11:48:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

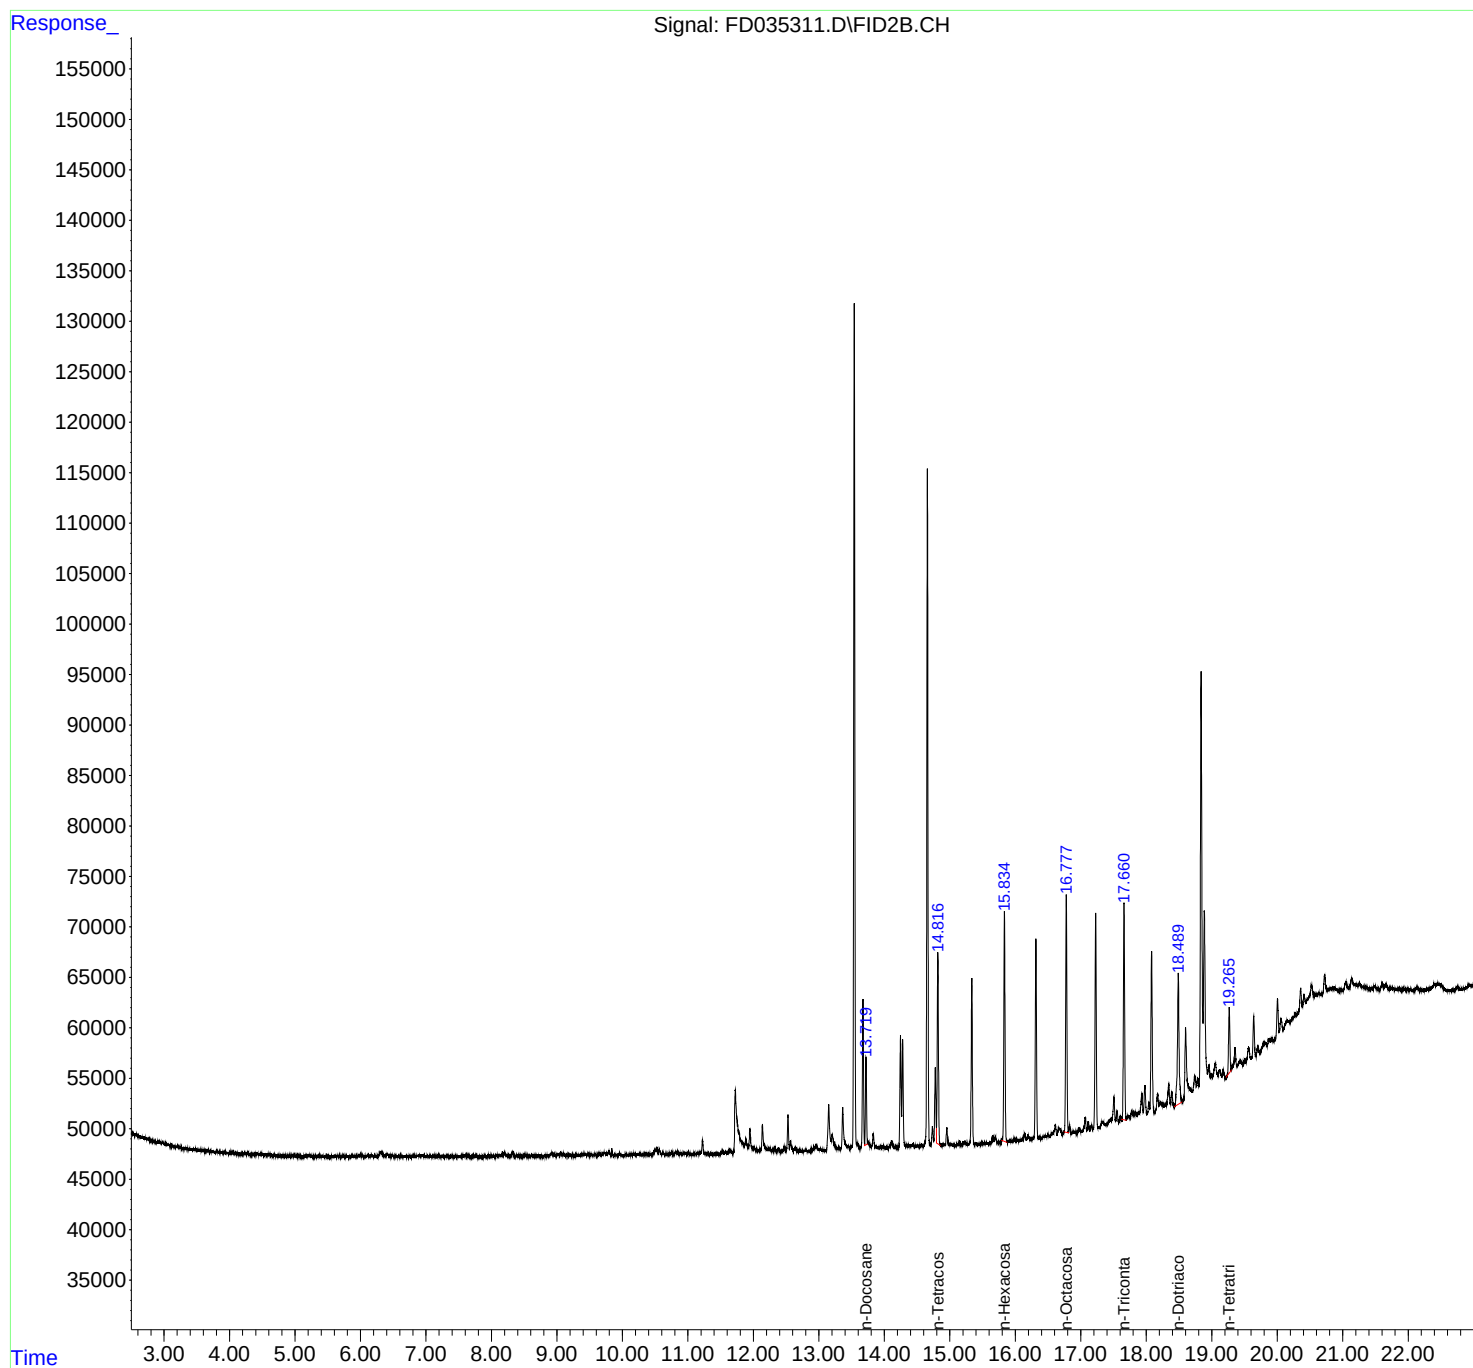


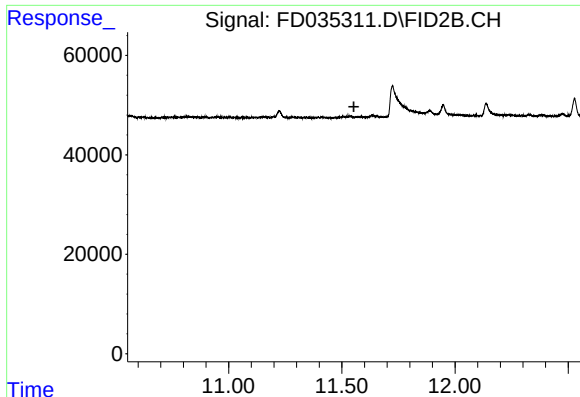

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.553 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

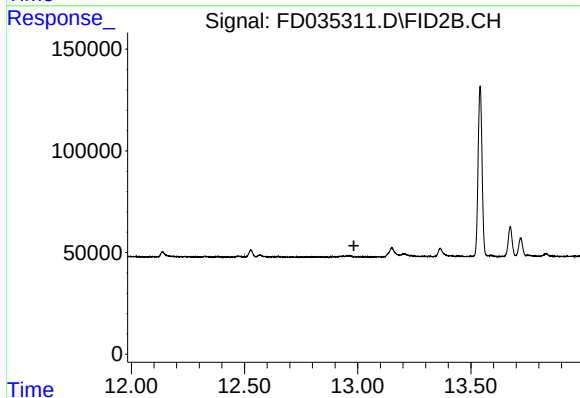


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.983 min
Response: 0
Conc: N.D.

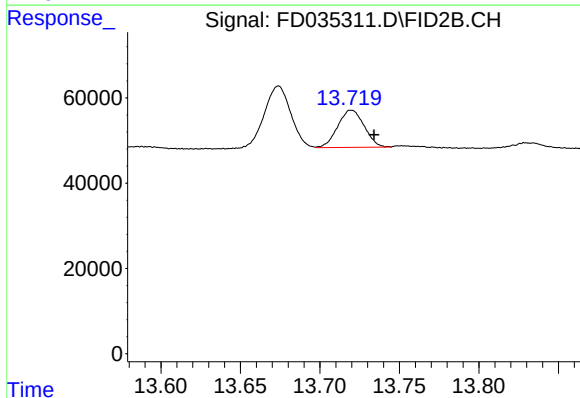


#13 n-Docosane (C22)

R.T.: 13.720 min
Delta R.T.: -0.014 min
Response: 101028
Conc: 0.82 ug/ml

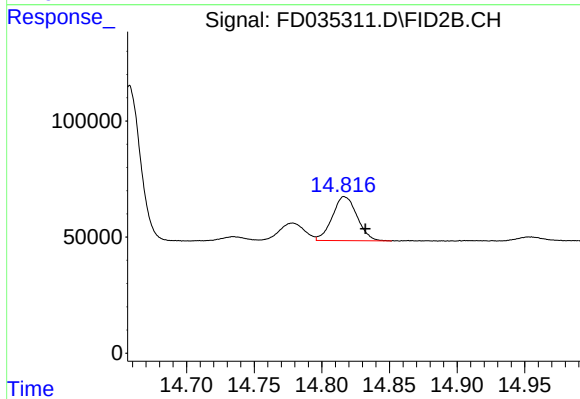

#14 n-Tetracosane (C24)


R.T.: 14.817 min
Delta R.T.: -0.016 min
Response: 241066
Conc: 1.95 ug/ml

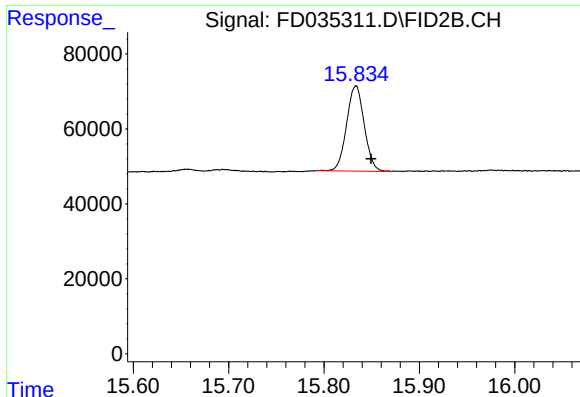

#15 n-Hexacosane (C26)


R.T.: 15.834 min
Delta R.T.: -0.016 min
Response: 292844
Conc: 2.38 ug/ml

Instrument :
FID_D
ClientSampleId :

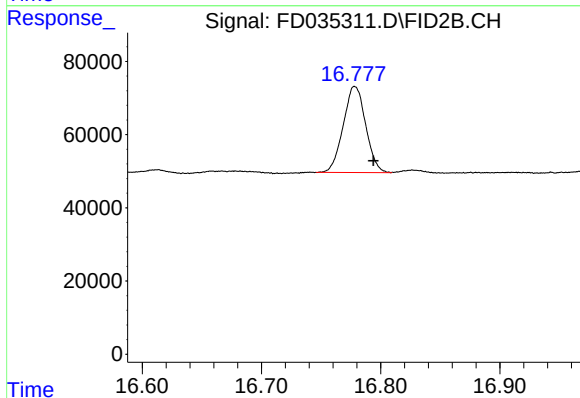


#16 n-Octacosane (C28)

R.T.: 16.778 min
Delta R.T.: -0.016 min
Response: 307781
Conc: 2.50 ug/ml

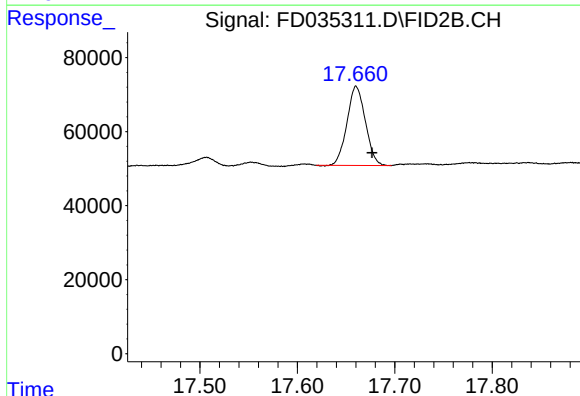


#17 n-Tricontane (C30)

R.T.: 17.660 min
Delta R.T.: -0.016 min
Response: 280144
Conc: 2.32 ug/ml

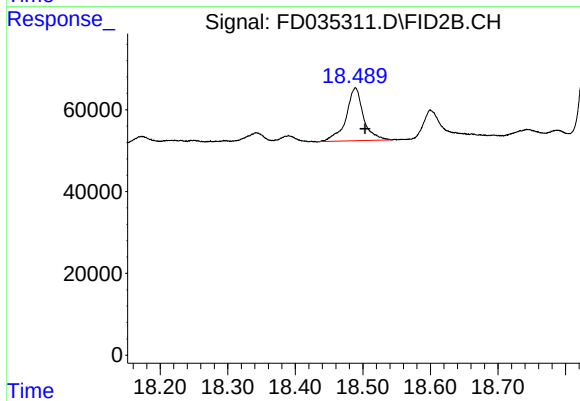

#18 n-Dotriacontane (C32)

R.T.: 18.489 min
Delta R.T.: -0.014 min
Response: 230578
Conc: 2.05 ug/ml

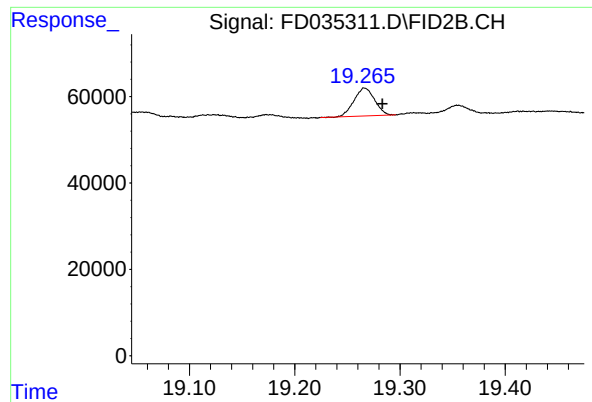

#19 n-Tetratriacontane (C34)

R.T.: 19.266 min
Delta R.T.: -0.017 min
Response: 88372
Conc: 0.84 ug/ml

Instrument :
FID_D
ClientSampleId :