

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110424AR\
 Data File : FD048656.D
 Signal(s) : FID2B.ch
 Acq On : 05 Nov 2024 01:46
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 03:11:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 102324.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 23 18:14:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T Indeno[1,2,3-cd]pyren...	17.807f	54575	0.418 ug/ml
20) T Dibenz[a,h]anthracene...	17.807	54575	0.335 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110424AR\
 Data File : FD048656.D
 Signal(s) : FID2B.ch
 Acq On : 05 Nov 2024 01:46
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 03:11:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 102324.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 23 18:14:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

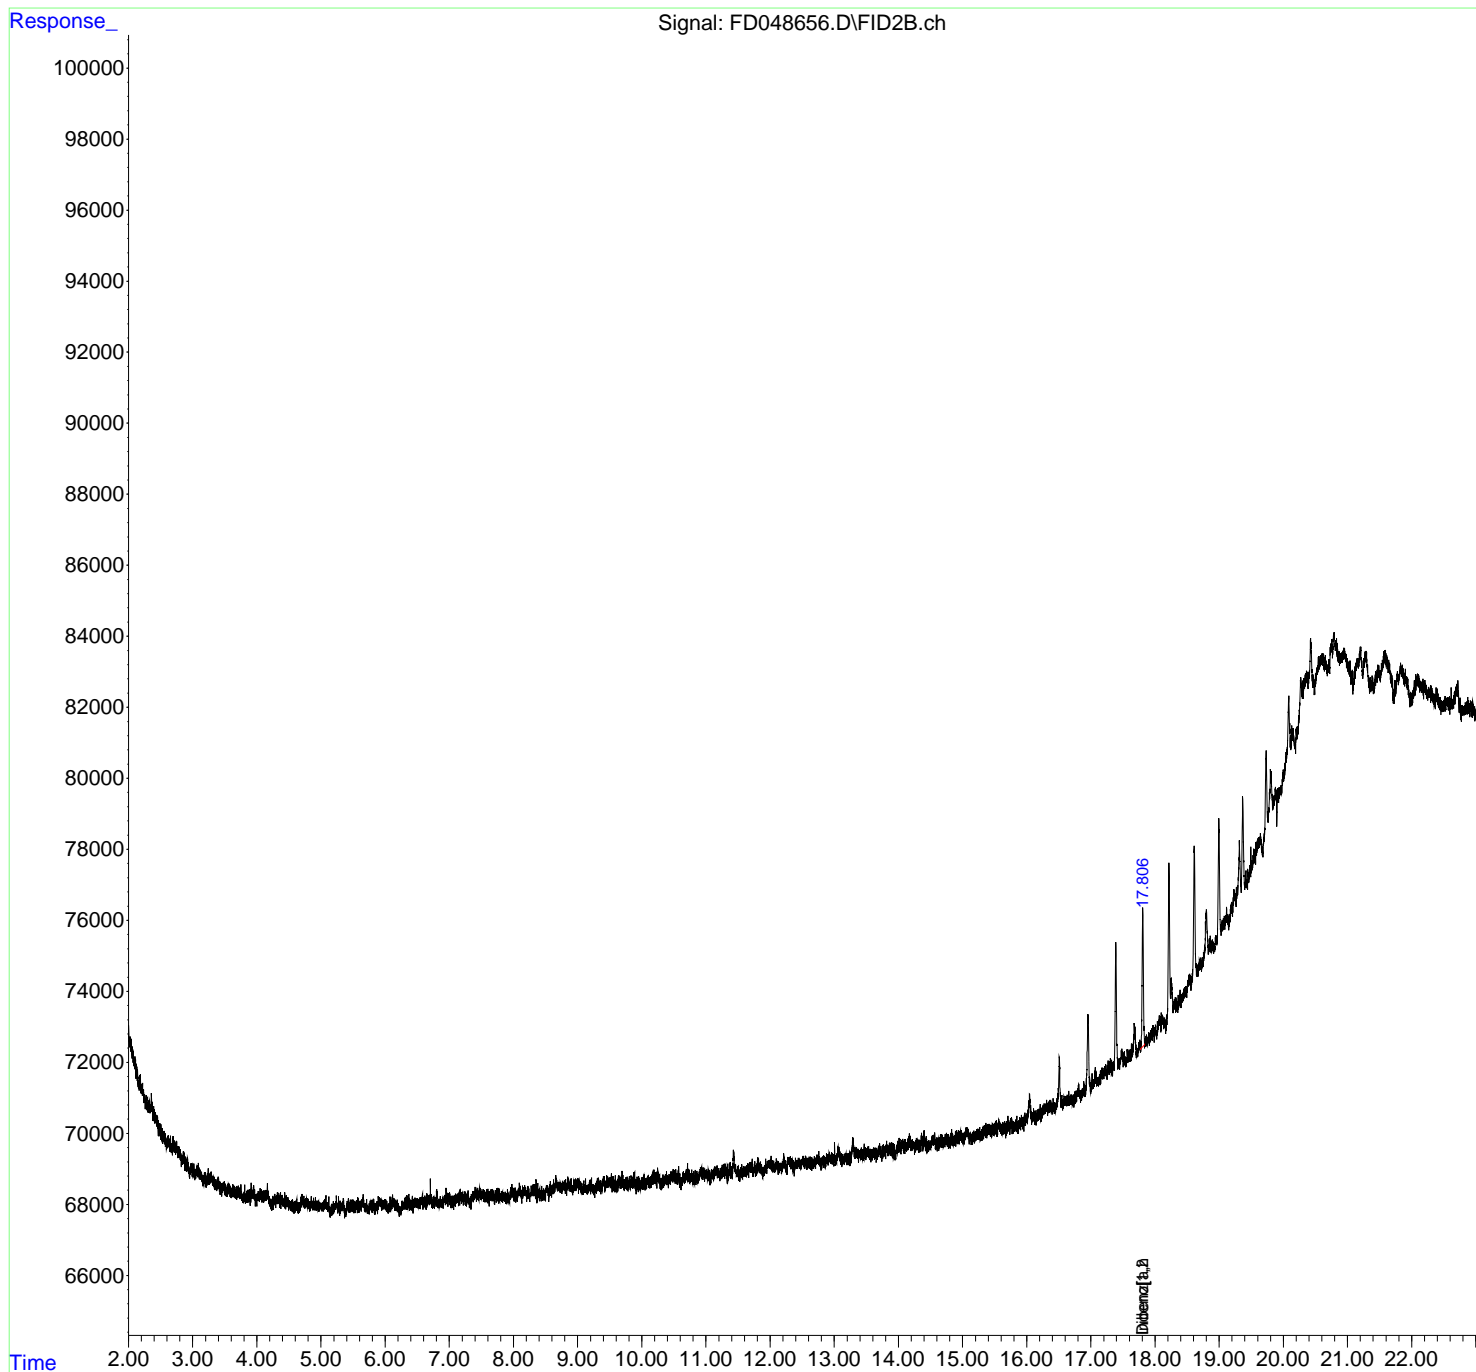


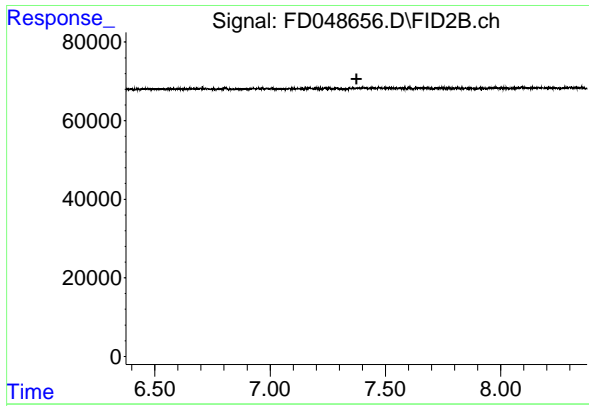

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
 Exp R.T.: 7.375 min
 Response: 0
 Conc: N.D.

Instrument : FID_D
 ClientSampleId :

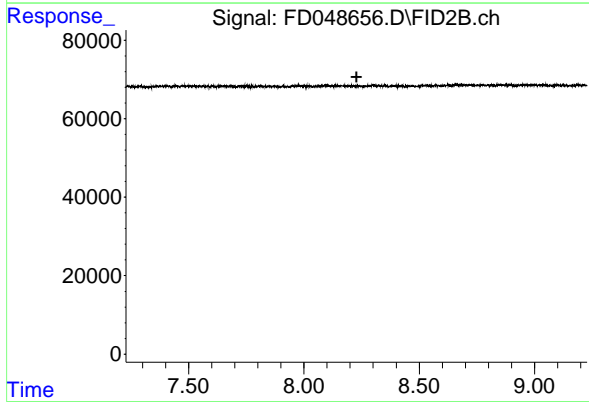


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
 Exp R.T.: 8.228 min
 Response: 0
 Conc: N.D.

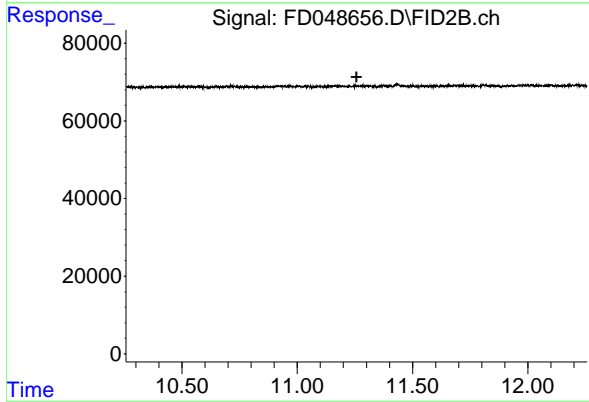


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
 Exp R.T.: 11.257 min
 Response: 0
 Conc: N.D.

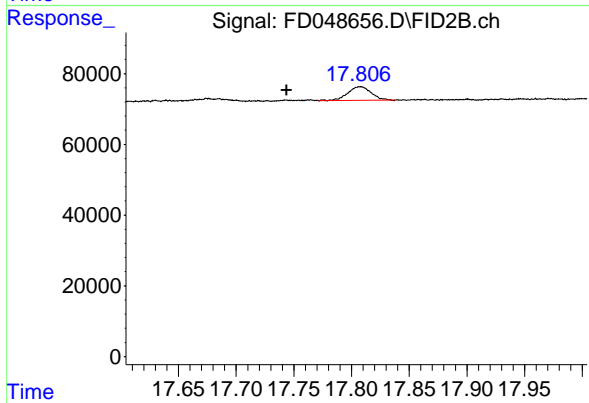

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.807 min
 Delta R.T.: 0.064 min
 Response: 54575
 Conc: 0.42 ug/ml

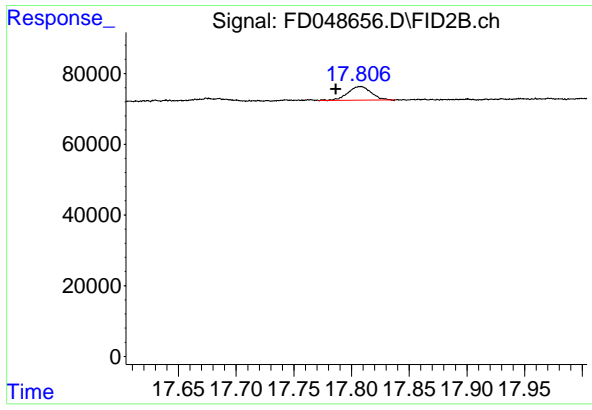

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.807 min
Delta R.T.: 0.021 min
Response: 54575
Conc: 0.34 ug/ml

Instrument :
FID_D
ClientSampleId :