

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110824AR\
Data File : FD048667.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2024 10:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 01:06:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:14:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	Benzo[a]pyrene (C31.34)	16.412	68641	0.456 ug/ml
19) T	Indeno[1,2,3-cd]pyren...	17.681f	94793	0.727 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD110824AR\
Data File : FD048667.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2024 10:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 01:06:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:14:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

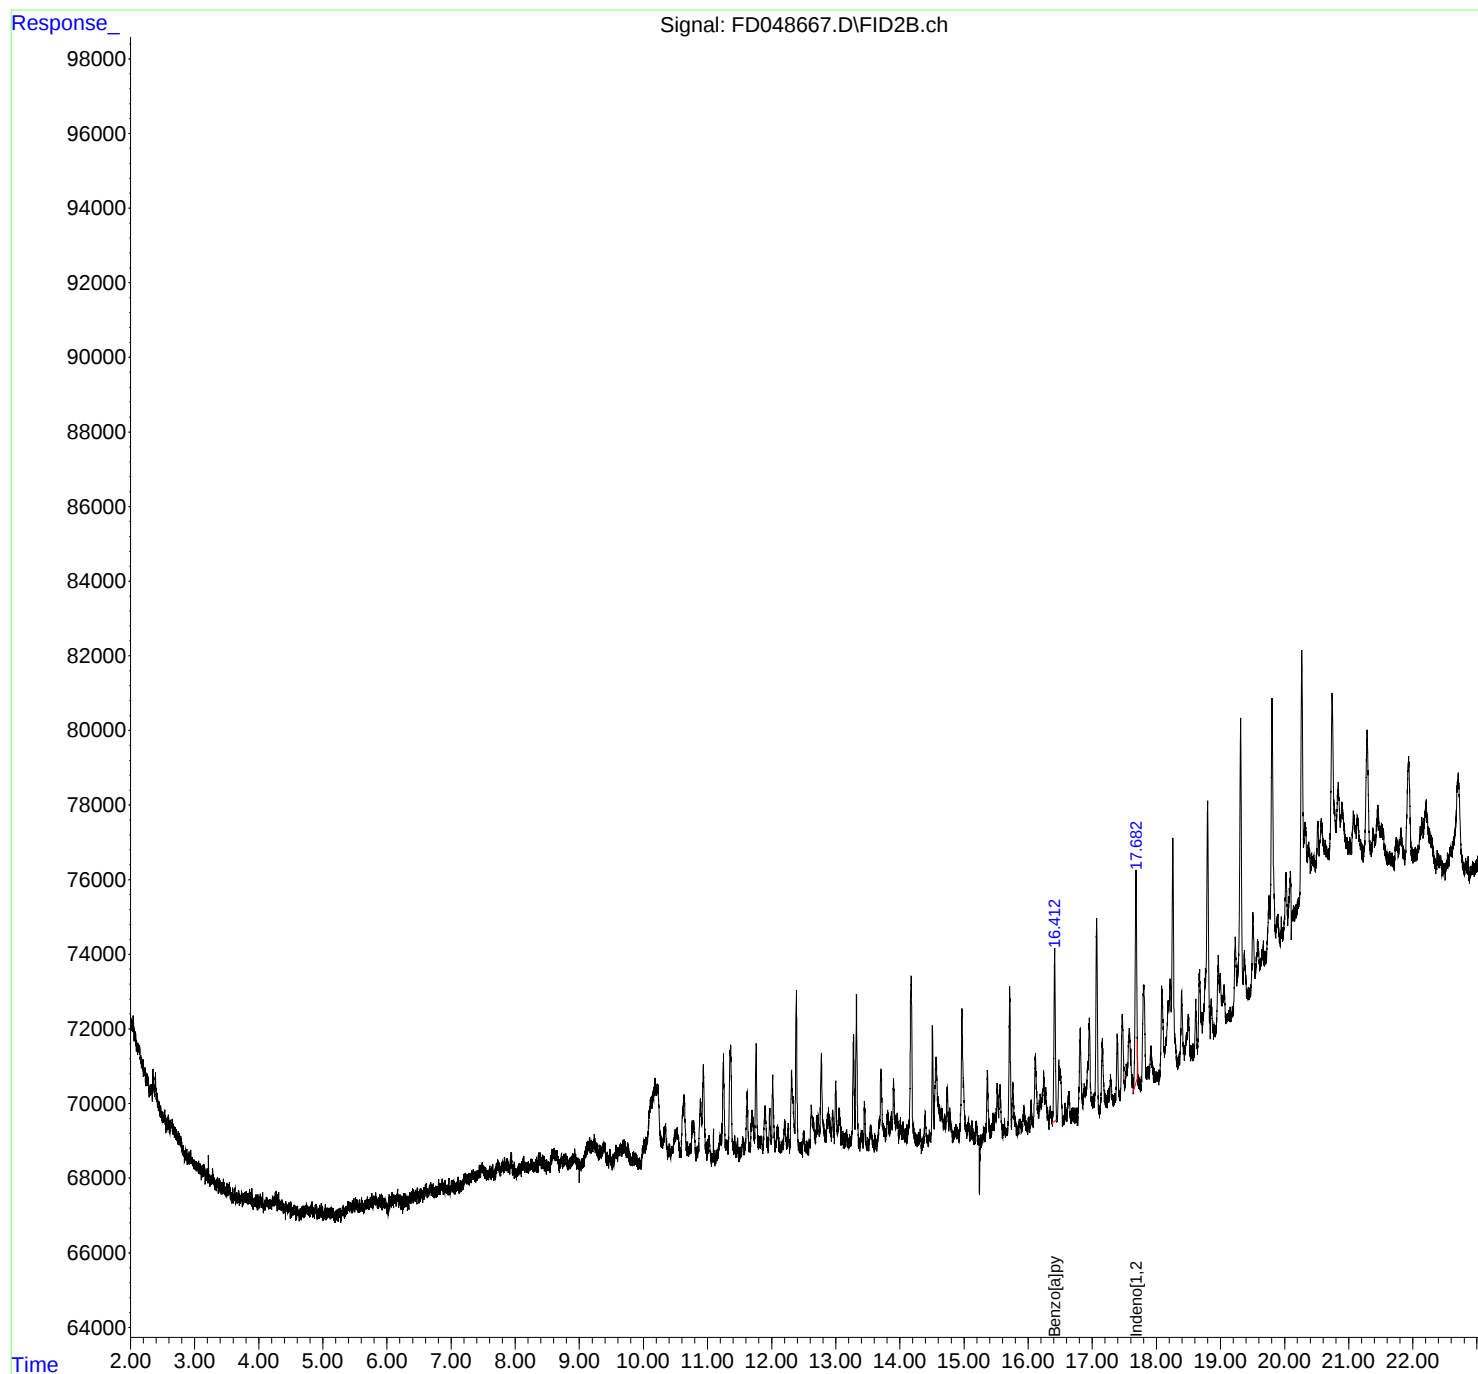


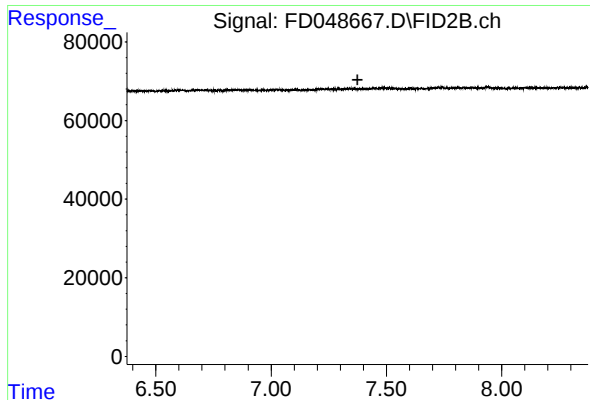

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.375 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

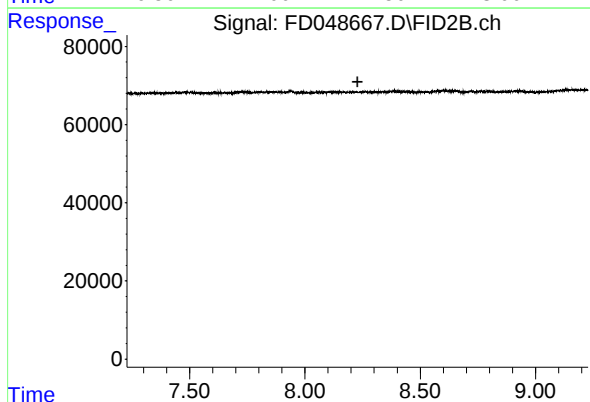


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.228 min
Response: 0
Conc: N.D.

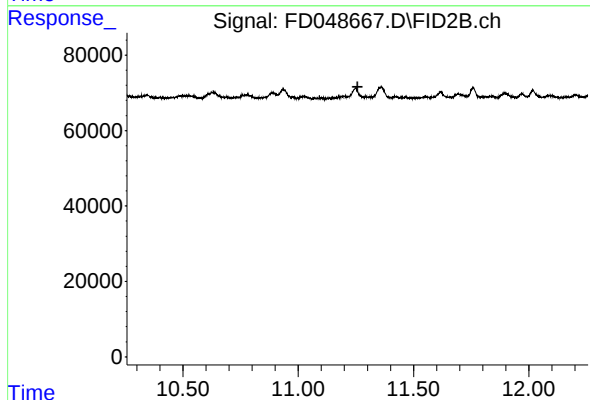


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.257 min
Response: 0
Conc: N.D.

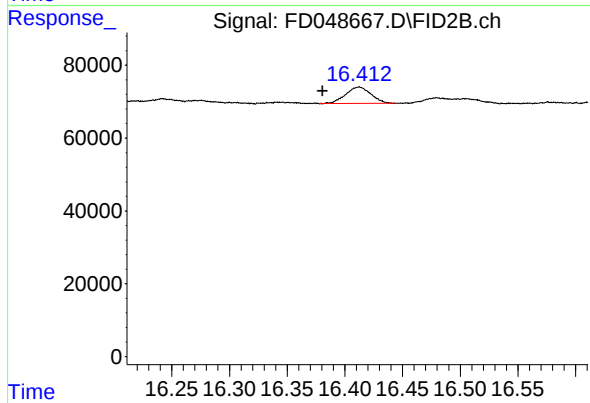

#18 Benzo[a]pyrene (C31.34)

R.T.: 16.412 min
Delta R.T.: 0.031 min
Response: 68641
Conc: 0.46 ug/ml

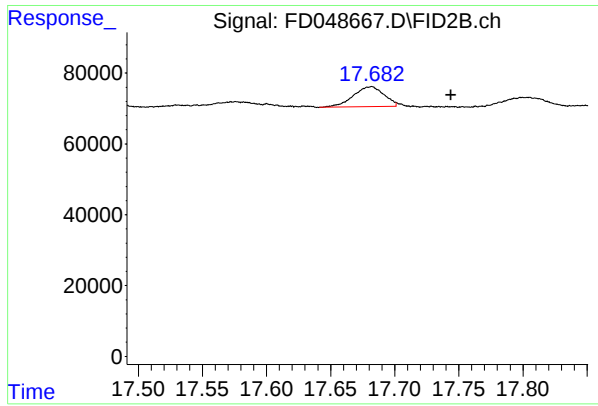

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.681 min

Delta R.T.: -0.063 min

Response: 94793

Conc: 0.73 ug/ml

Instrument :

FID_D

ClientSampleId :