

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111124AL\
 Data File : FC067689.D
 Signal(s) : FID1A.ch
 Acq On : 11 Nov 2024 11:02
 Operator : YP/AJ
 Sample : P4721-01DL2 200X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 11 20:43:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 23 18:12:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) T A~Naphthalene (C11.7)	5.874	227056	1.532 ug/ml
4) T n-Dodecane (C12)	6.370	120127	0.887 ug/ml
5) T A~2-methylnaphthalene...	6.962	75118	0.532 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111124AL\
Data File : FC067689.D
Signal(s) : FID1A.ch
Acq On : 11 Nov 2024 11:02
Operator : YP/AJ
Sample : P4721-01DL2 200X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 11 20:43:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

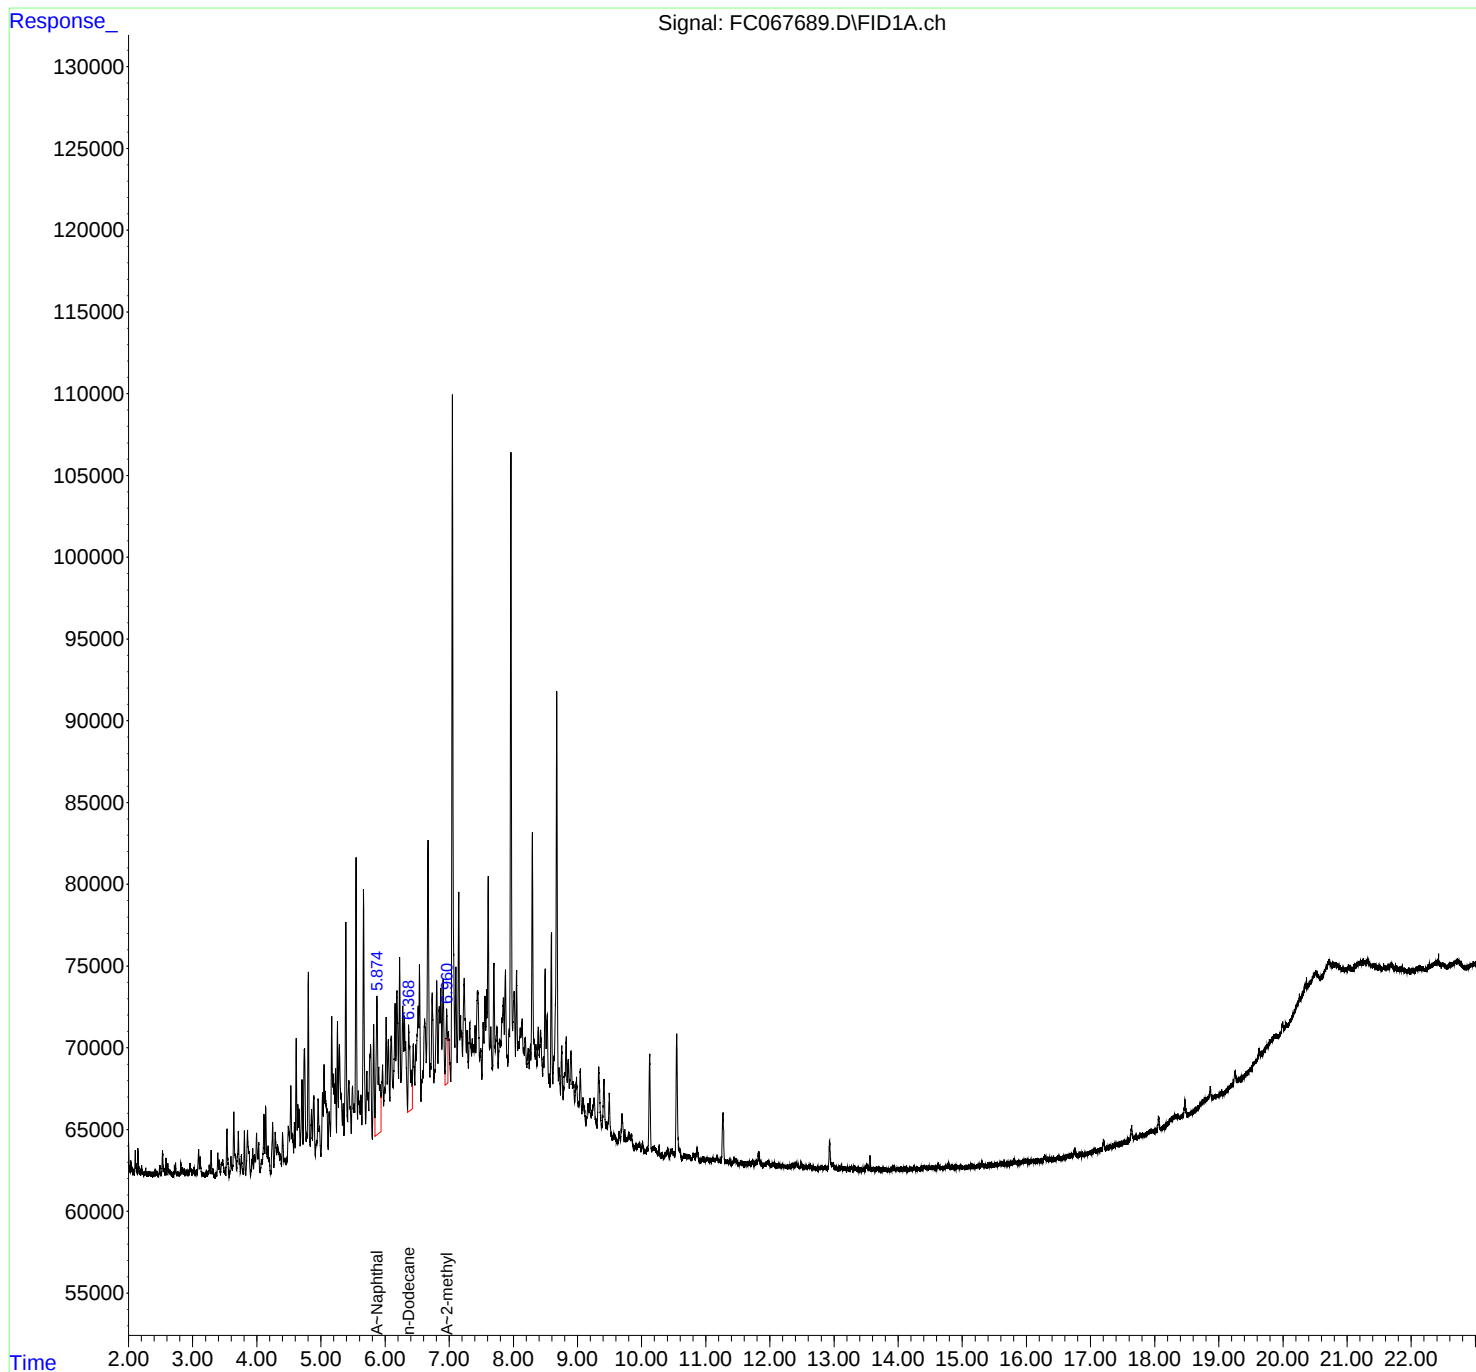


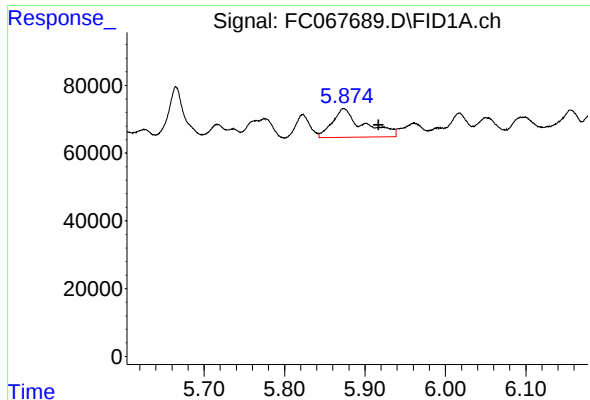

#3 A~Naphthalene (C11.7)


R.T.: 5.874 min
Delta R.T.: -0.043 min
Response: 227056
Conc: 1.53 ug/ml

Instrument :
FID_D
ClientSampleId :

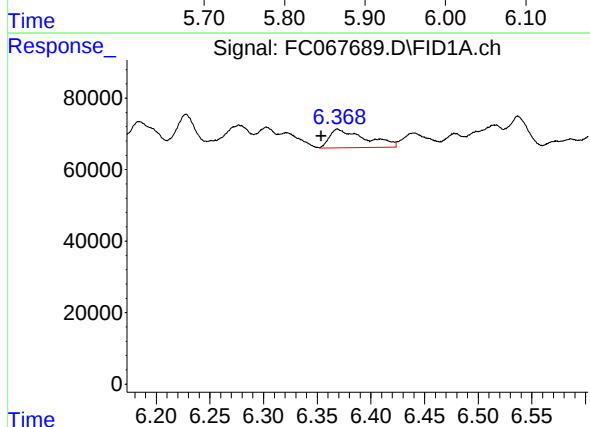


#4 n-Dodecane (C12)

R.T.: 6.370 min
Delta R.T.: 0.016 min
Response: 120127
Conc: 0.89 ug/ml

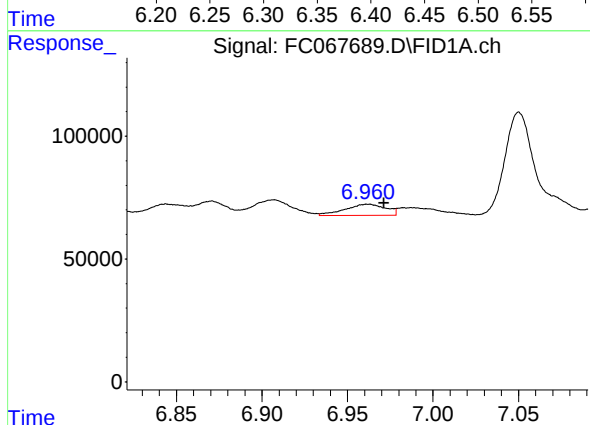


#5 A~2-methylnaphthalene (C12.89)

R.T.: 6.962 min
Delta R.T.: -0.009 min
Response: 75118
Conc: 0.53 ug/ml

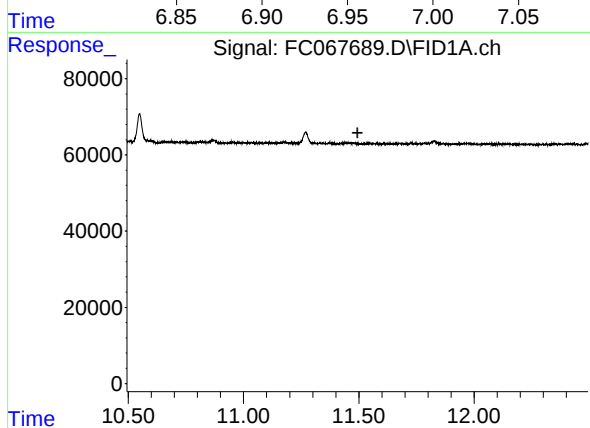

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.494 min
Response: 0
Conc: N.D.

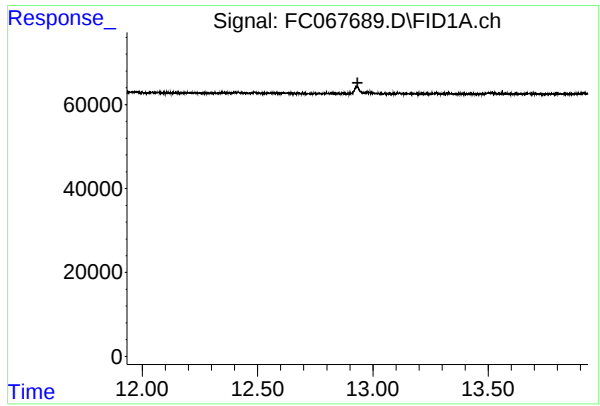

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.933 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :