

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111224AL\
Data File : FC067703.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2024 08:45
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 23:53:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
20) T	n-Hexatriacontane (C36)	20.047f	15160	0.167 ug/ml
21) T	n-Octatriacontane (C38)	20.655f	199483	2.303 ug/ml
22) T	n-Tetracontane (C40)	21.583	702951	8.269 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111224AL\
Data File : FC067703.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2024 08:45
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 23:53:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

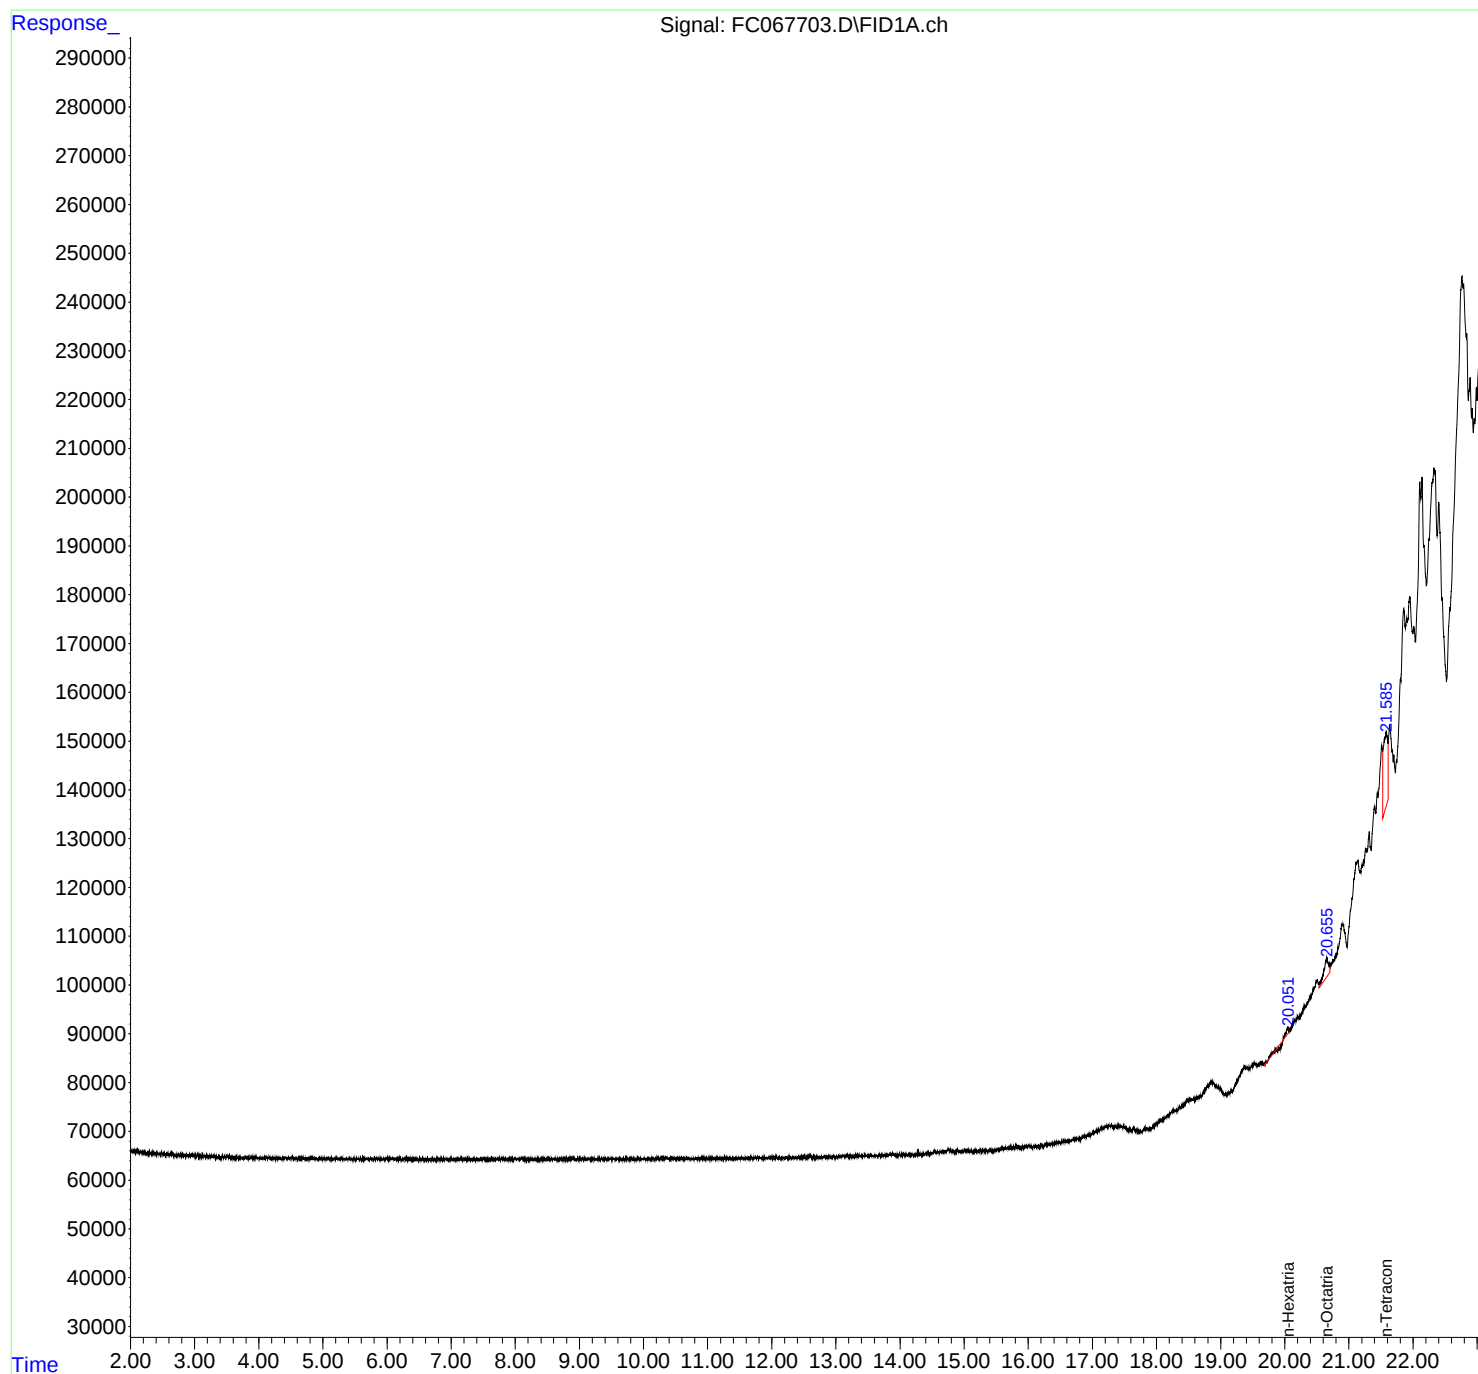


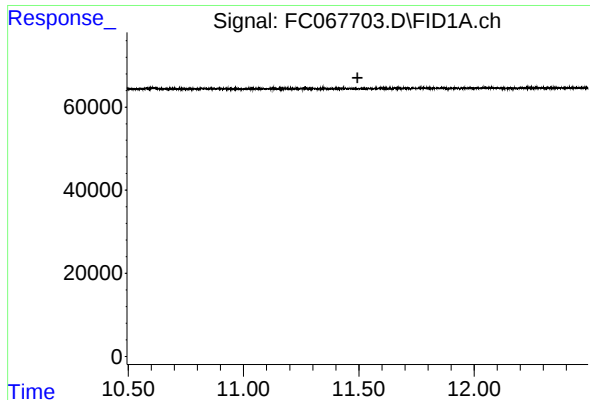

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.494 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

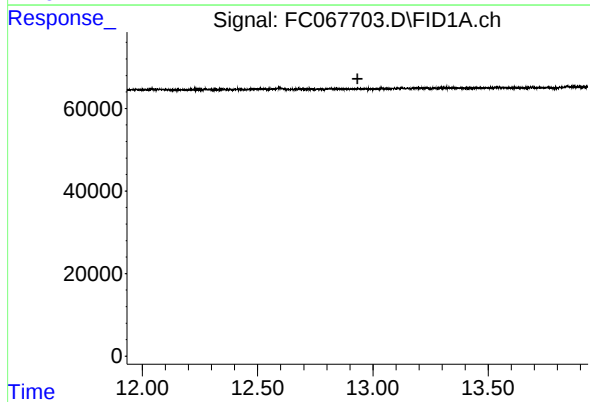


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.933 min
Response: 0
Conc: N.D.

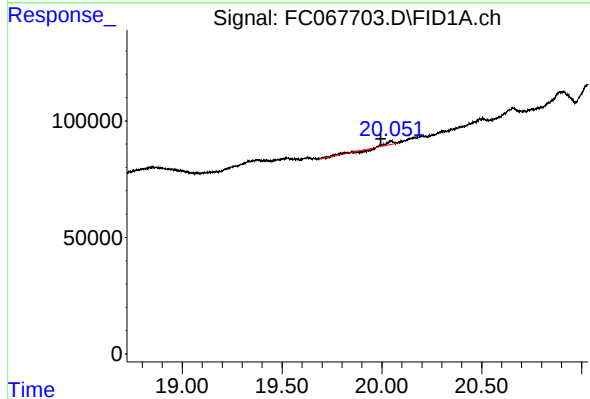


#20 n-Hexatriacontane (C36)

R.T.: 20.047 min
Delta R.T.: 0.053 min
Response: 15160
Conc: 0.17 ug/ml

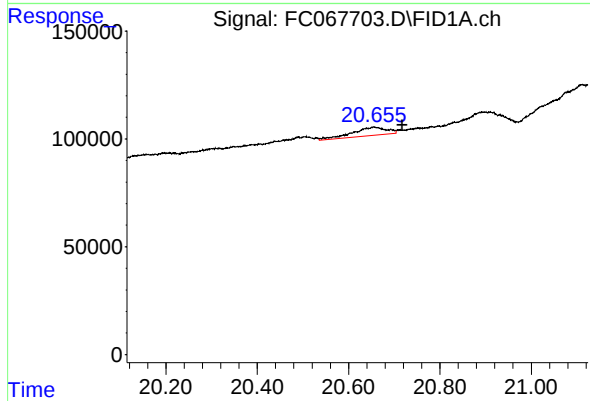

#21 n-Octatriacontane (C38)

R.T.: 20.655 min
Delta R.T.: -0.063 min
Response: 199483
Conc: 2.30 ug/ml

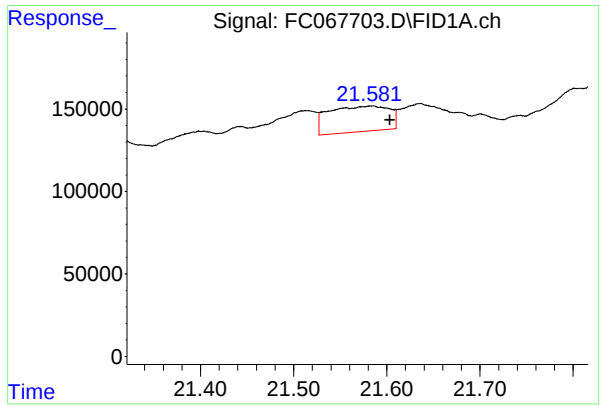

#22 n-Tetracontane (C40)

R.T.: 21.583 min
Delta R.T.: -0.020 min
Response: 702951
Conc: 8.27 ug/ml

Instrument :

FID_D

ClientSampleId :