

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111324AR\
 Data File : FF015009.D
 Signal(s) : FID2B.ch
 Acq On : 13 Nov 2024 13:22
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 02:58:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 110724.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 08 08:49:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T Indeno[1,2,3-cd]pyren...	18.497	29969	0.218 ug/ml
20) T Dibenz[a,h]anthracene...	18.497	29969	0.203 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111324AR\
Data File : FF015009.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2024 13:22
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 02:58:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 110724.M
Quant Title : GC Extractables
QLast Update : Fri Nov 08 08:49:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

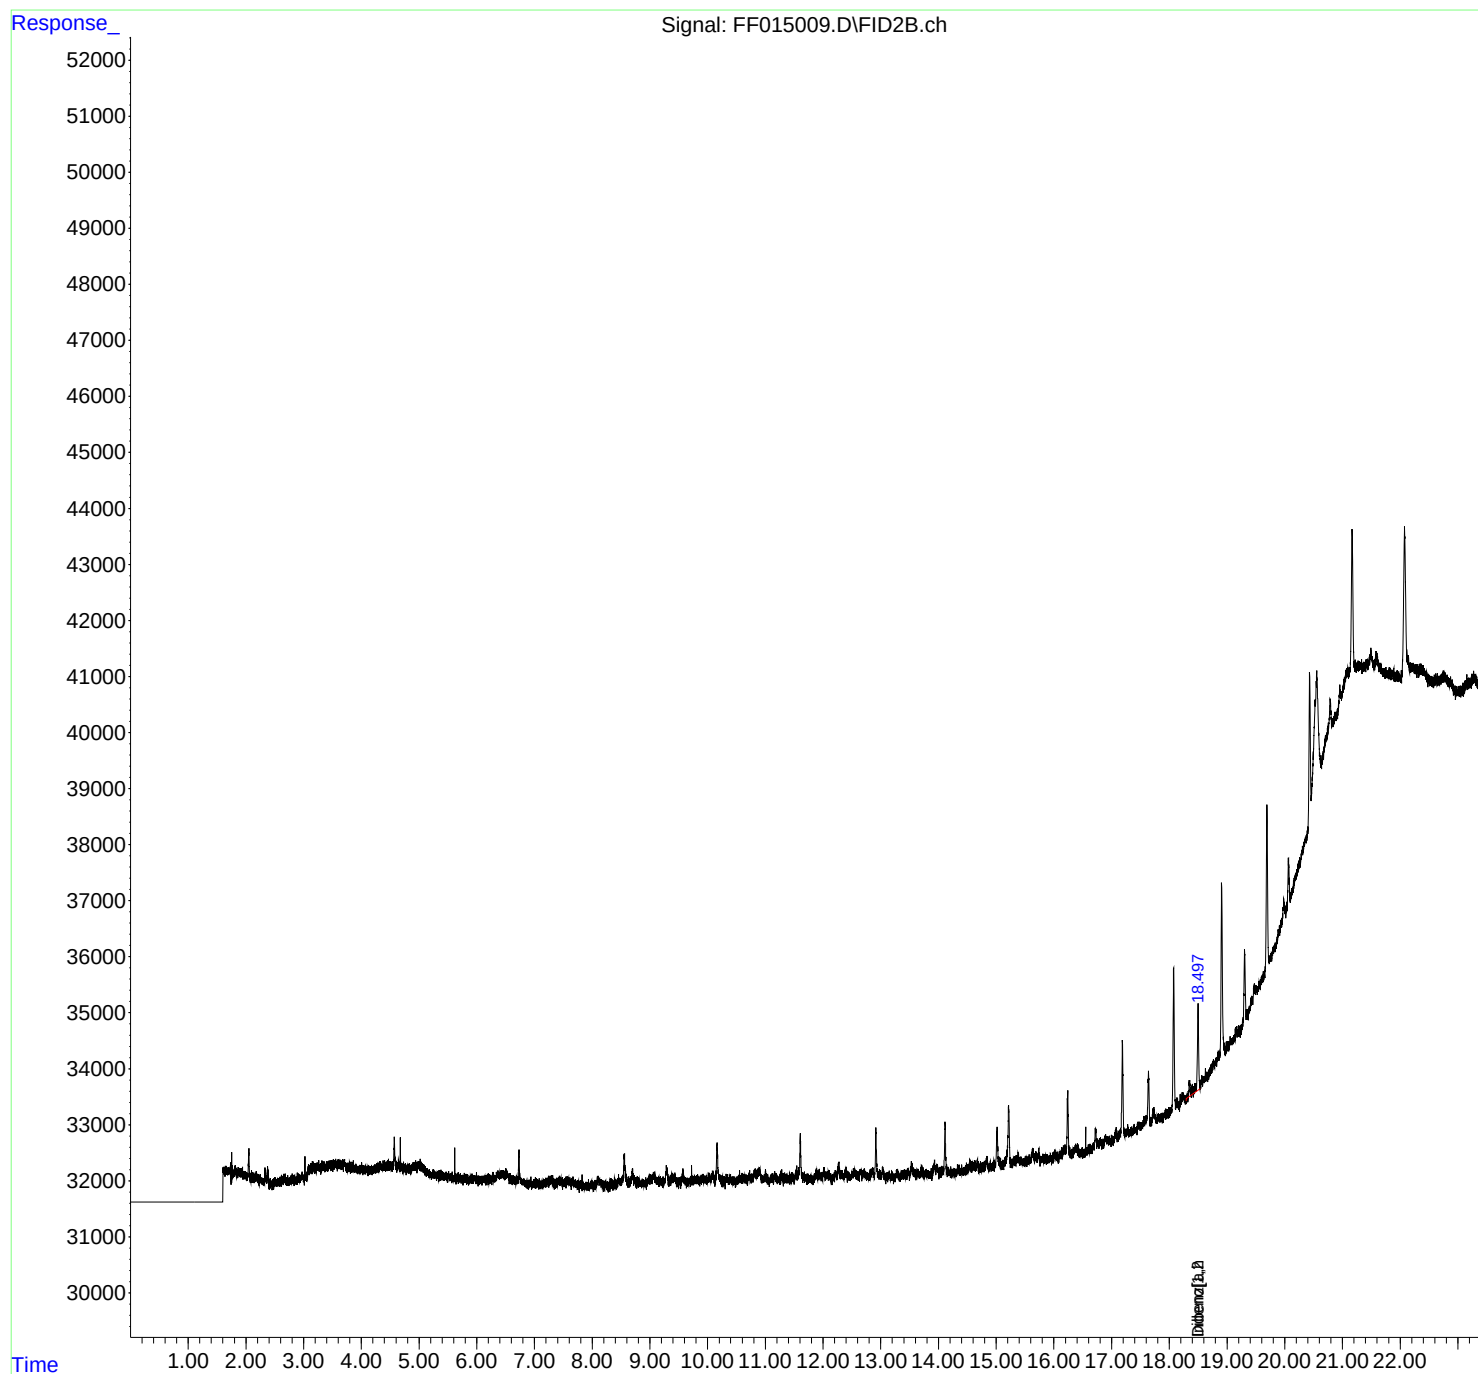


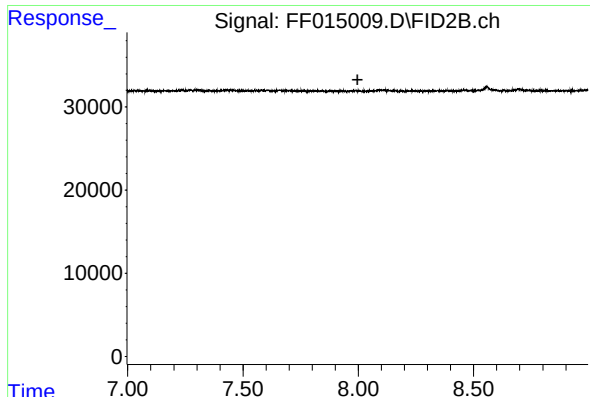

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.997 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

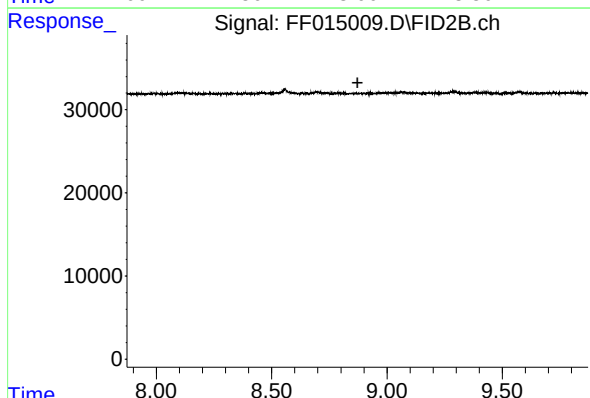


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

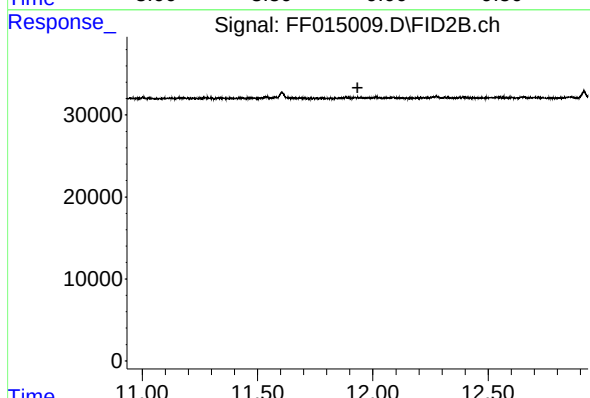


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.933 min
Response: 0
Conc: N.D.

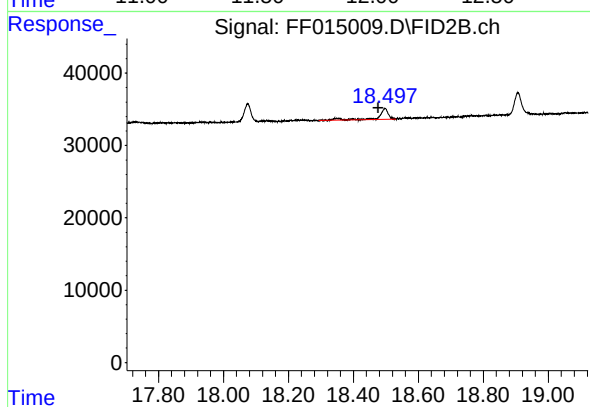

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.497 min
Delta R.T.: 0.021 min
Response: 29969
Conc: 0.22 ug/ml

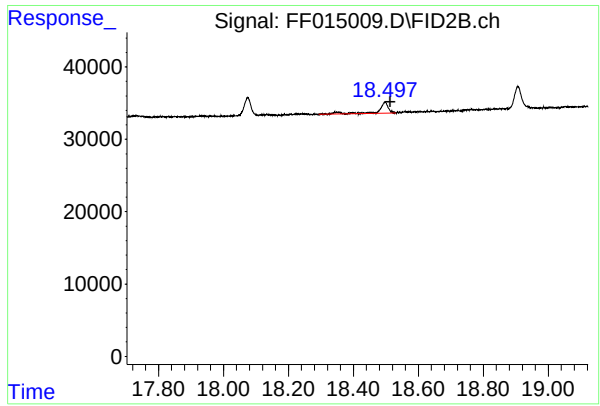

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.497 min
Delta R.T.: -0.017 min
Response: 29969
Conc: 0.20 ug/ml

Instrument :
FID_D
ClientSampleId :