

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD111620AL\
 Data File : FD035556.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2020 6:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 17 08:06:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 11:48:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	13.676f	101039	0.819 ug/ml
14) T n-Tetracosane (C24)	14.823	118401	0.957 ug/ml
15) T n-Hexacosane (C26)	15.840	138343	1.124 ug/ml
16) T n-Octacosane (C28)	16.787	161673	1.313 ug/ml
17) T n-Tricontane (C30)	17.671	524638	4.341 ug/ml
18) T n-Dotriacontane (C32)	18.498	117863	1.048 ug/ml
19) T n-Tetratriacontane (C34)	19.288	227342	2.166 ug/ml
20) T n-Hexatriacontane (C36)	20.012	662910	6.920 ug/ml
21) T n-Octatriacontane (C38)	20.736	1633715	18.392 ug/ml
22) T n-Tetracontane (C40)	21.609	443015	5.048 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD111620AL\
Data File : FD035556.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2020 6:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 17 08:06:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 11:48:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

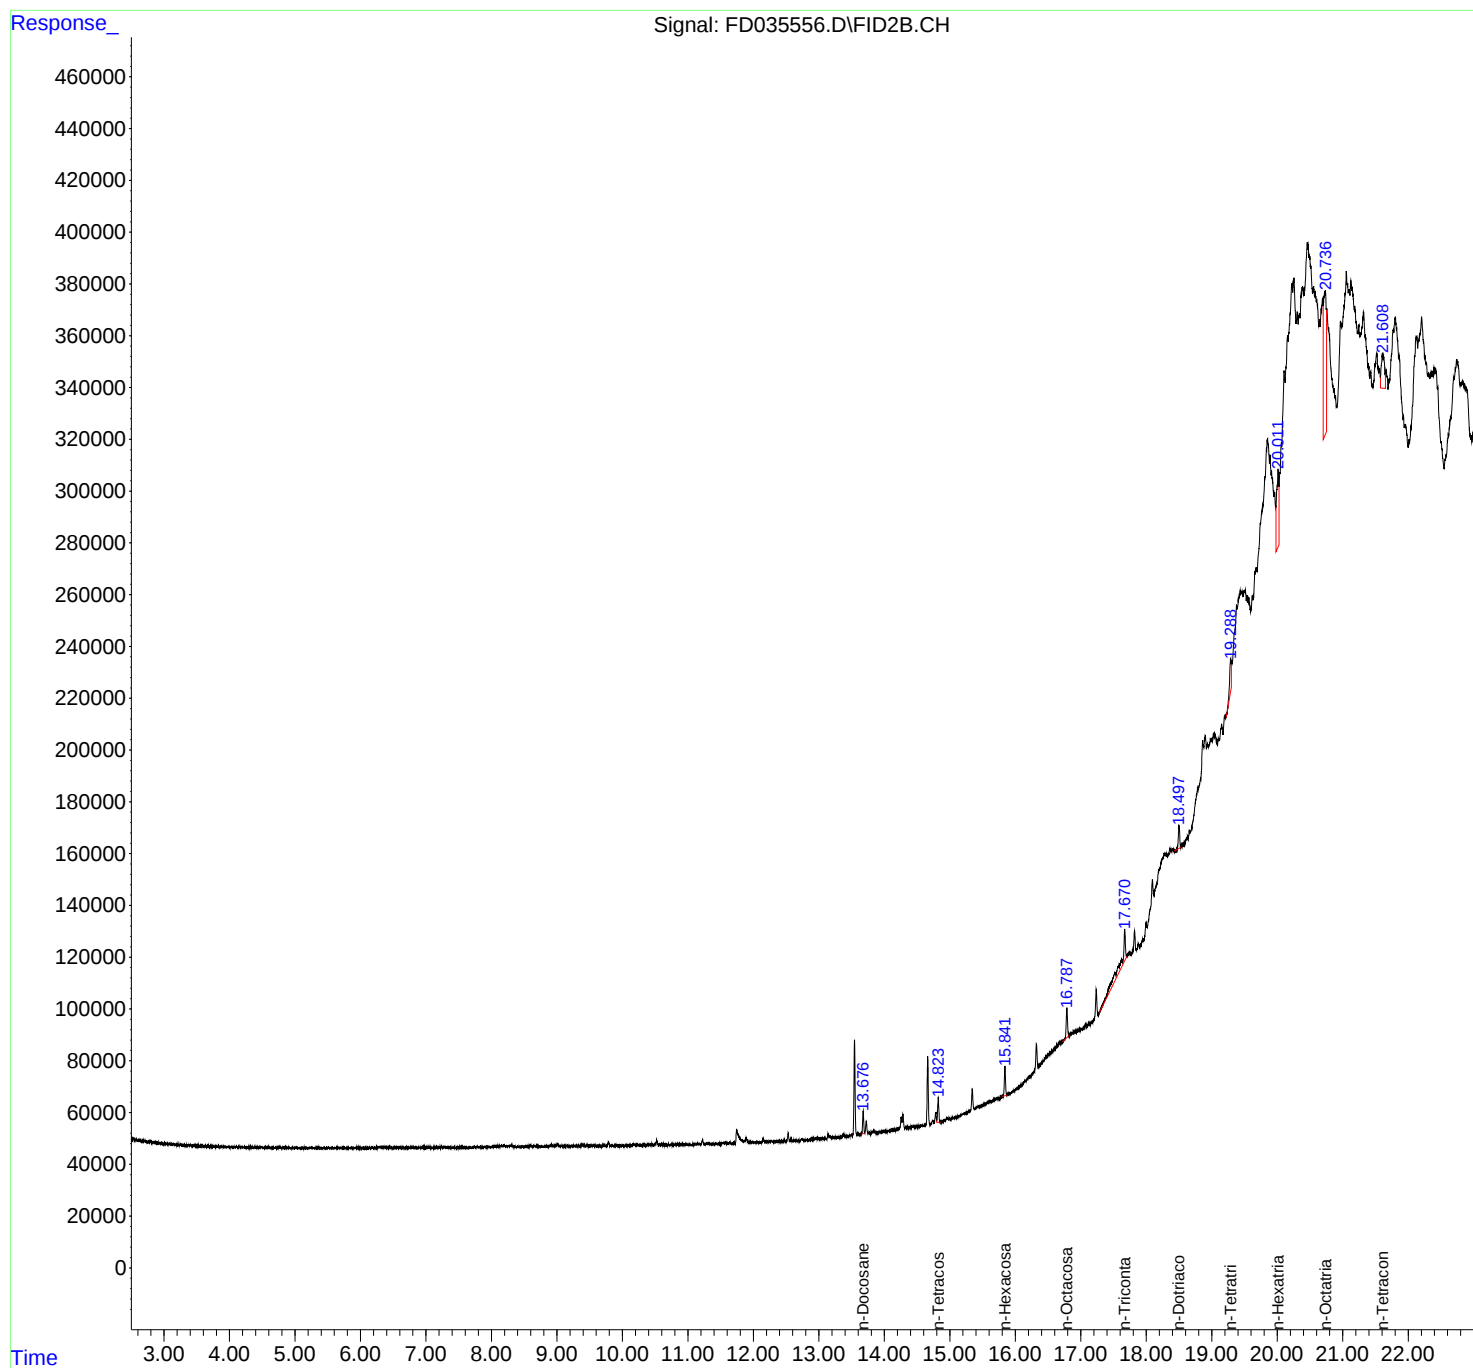


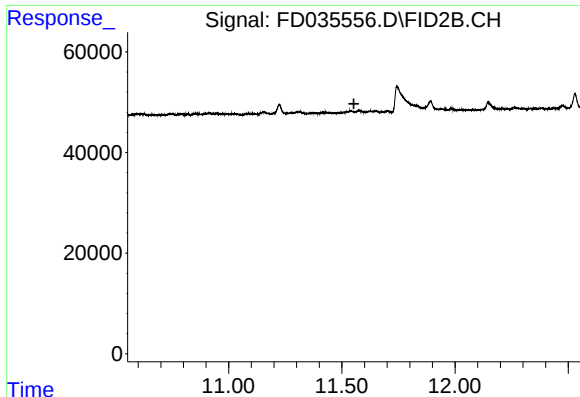

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.553 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

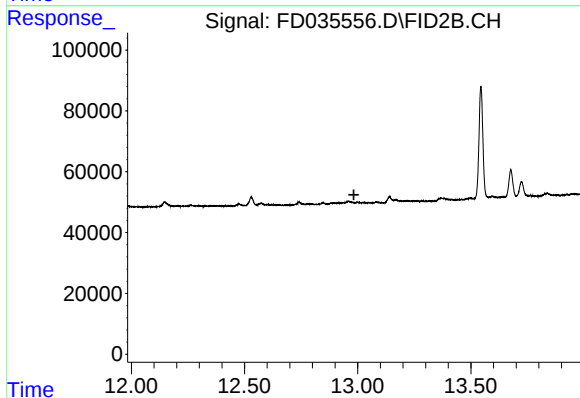


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.983 min
Response: 0
Conc: N.D.

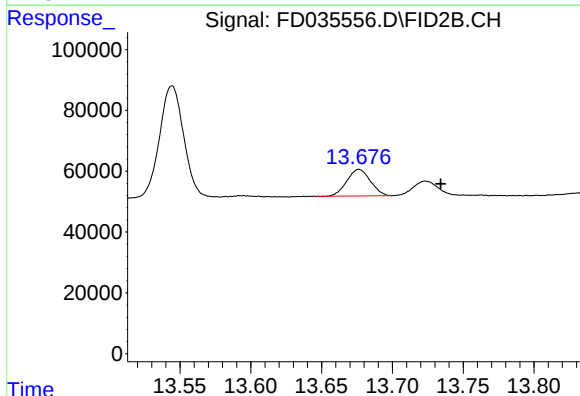


#13 n-Docosane (C22)

R.T.: 13.676 min
Delta R.T.: -0.058 min
Response: 101039
Conc: 0.82 ug/ml

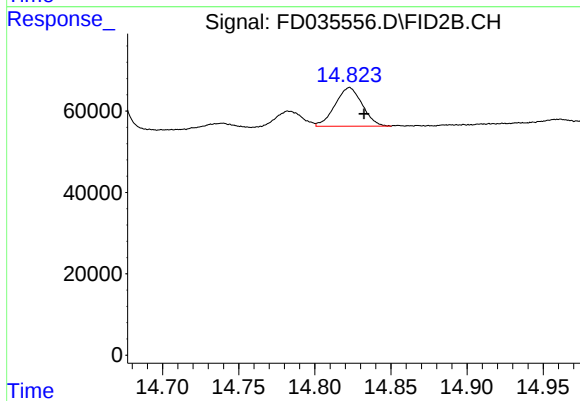

#14 n-Tetracosane (C24)


R.T.: 14.823 min
Delta R.T.: -0.009 min
Response: 118401
Conc: 0.96 ug/ml

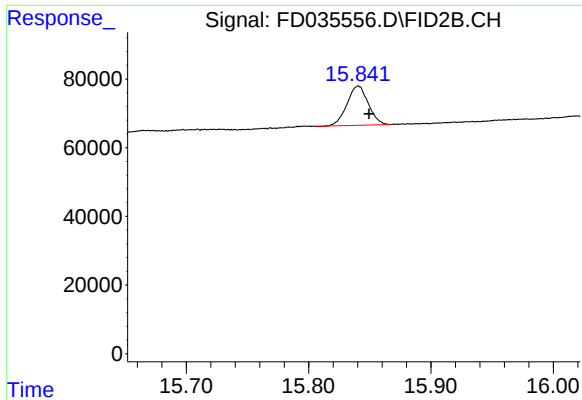

#15 n-Hexacosane (C26)


R.T.: 15.840 min
Delta R.T.: -0.009 min
Response: 138343
Conc: 1.12 ug/ml

Instrument :
FID_D
ClientSampleId :

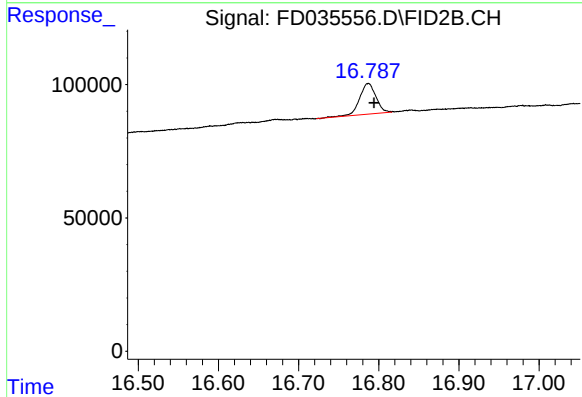


#16 n-Octacosane (C28)

R.T.: 16.787 min
Delta R.T.: -0.007 min
Response: 161673
Conc: 1.31 ug/ml

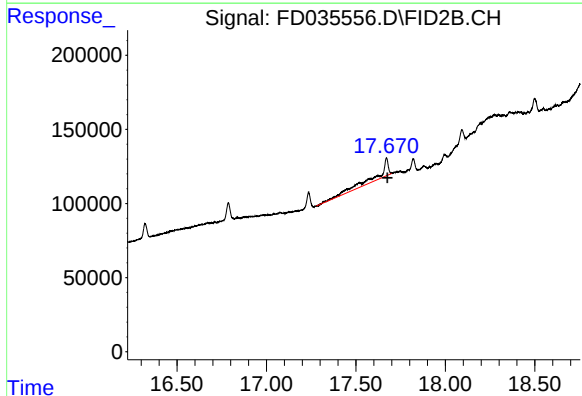


#17 n-Tricontane (C30)

R.T.: 17.671 min
Delta R.T.: -0.006 min
Response: 524638
Conc: 4.34 ug/ml

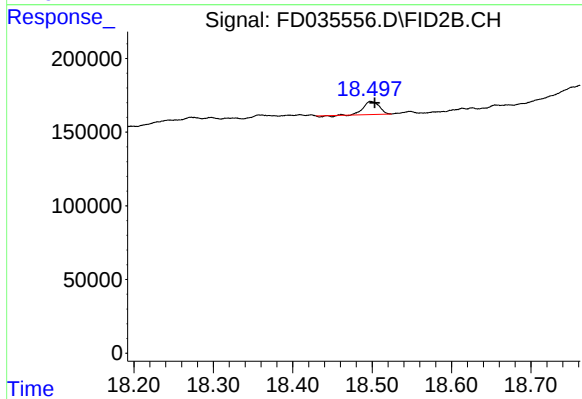

#18 n-Dotriacontane (C32)


R.T.: 18.498 min
Delta R.T.: -0.005 min
Response: 117863
Conc: 1.05 ug/ml

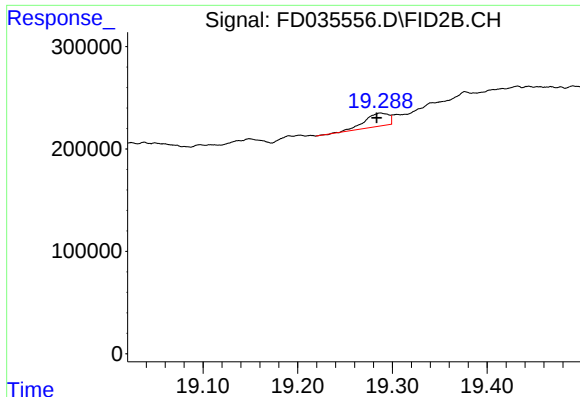

#19 n-Tetratriacontane (C34)


R.T.: 19.288 min
Delta R.T.: 0.004 min
Response: 227342
Conc: 2.17 ug/ml

Instrument :
FID_D
ClientSampleId :

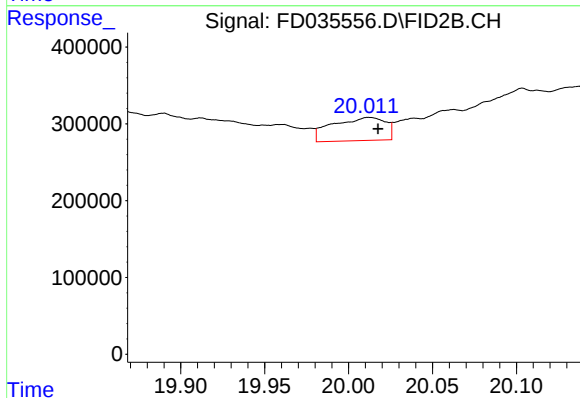


#20 n-Hexatriacontane (C36)

R.T.: 20.012 min
Delta R.T.: -0.005 min
Response: 662910
Conc: 6.92 ug/ml

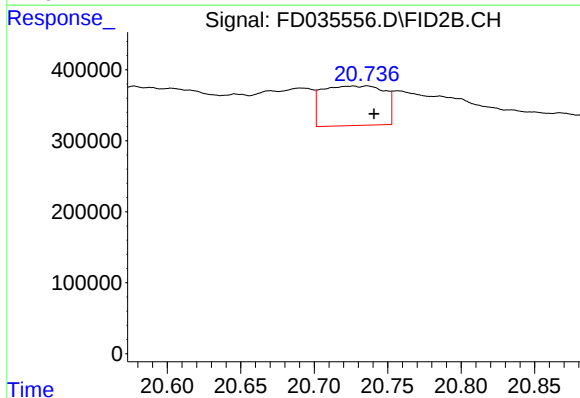

#21 n-Octatriacontane (C38)

R.T.: 20.736 min
Delta R.T.: -0.005 min
Response: 1633715
Conc: 18.39 ug/ml

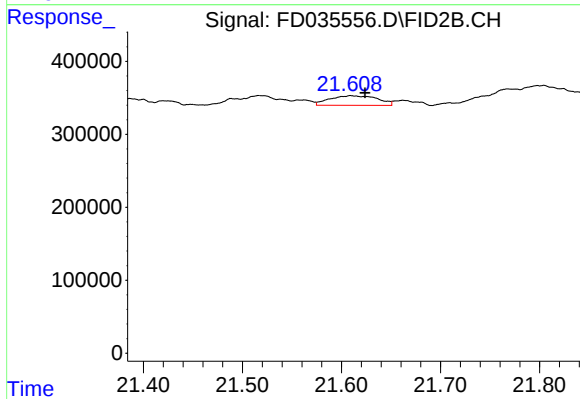

#22 n-Tetracontane (C40)

R.T.: 21.609 min
Delta R.T.: -0.015 min
Response: 443015
Conc: 5.05 ug/ml