

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD111722AR\
Data File : FD044445.D
Signal(s) : FID2B.ch
Acq On : 17 Nov 2022 06:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Nov 18 03:12:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 110322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 08:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T Benzo[a]anthracene (C...	14.812	34433	0.246 ug/ml
15) T Chrysene (C27.41)	14.812	34433	0.235 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD111722AR\
Data File : FD044445.D
Signal(s) : FID2B.ch
Acq On : 17 Nov 2022 06:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Nov 18 03:12:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 110322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 08:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

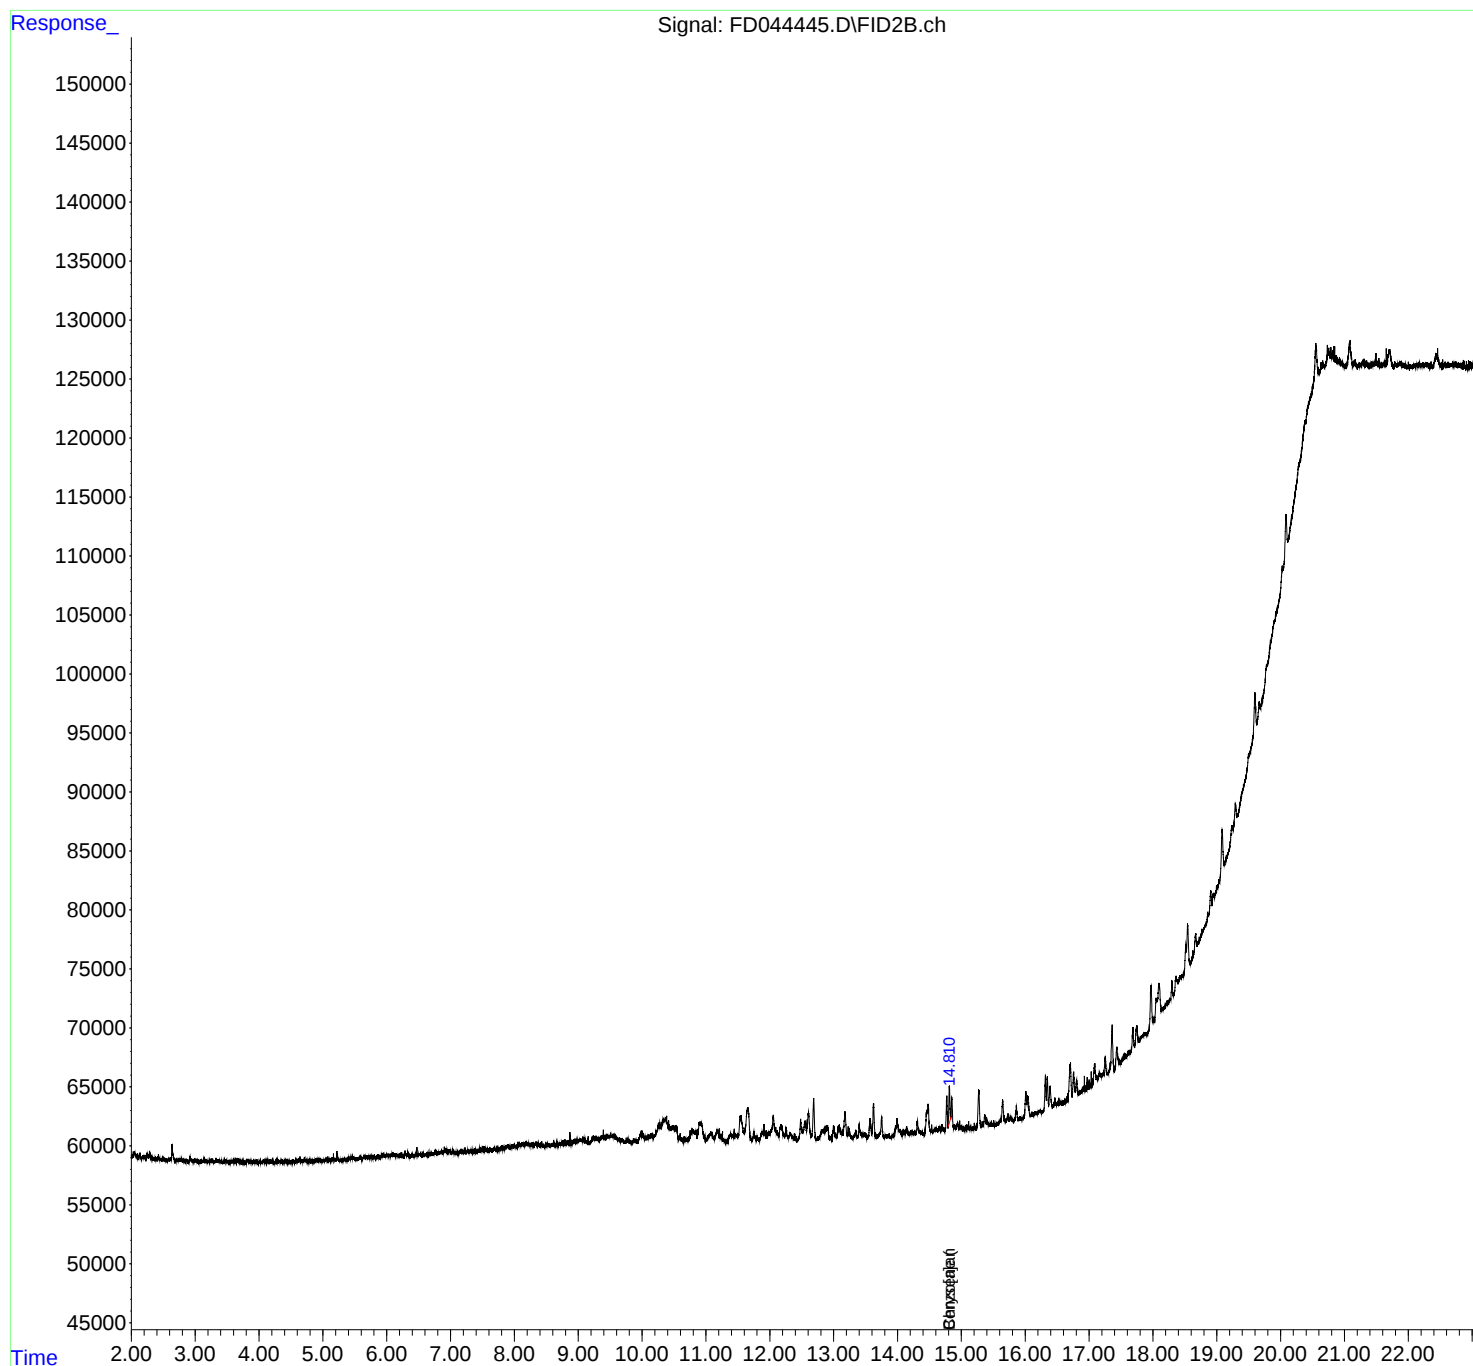


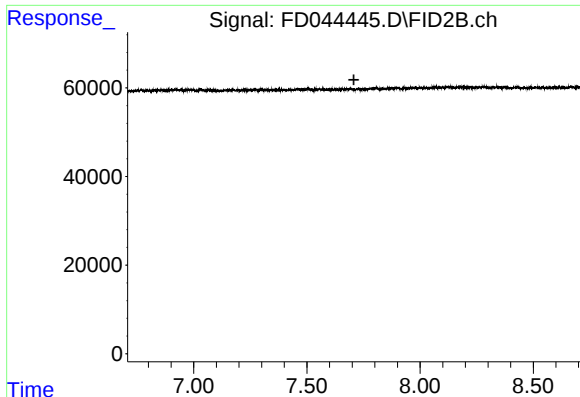

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T.: 7.708 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
MECL2

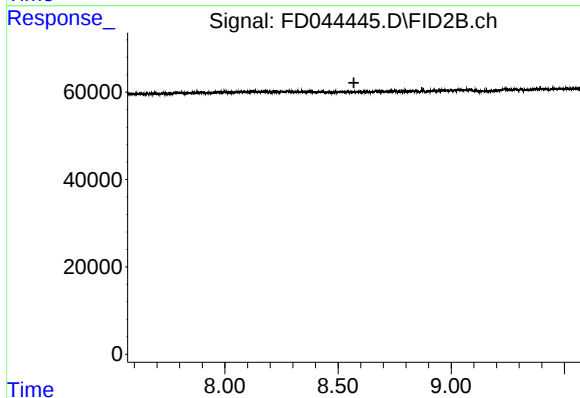


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 8.570 min
Response: 0
Conc: N.D.

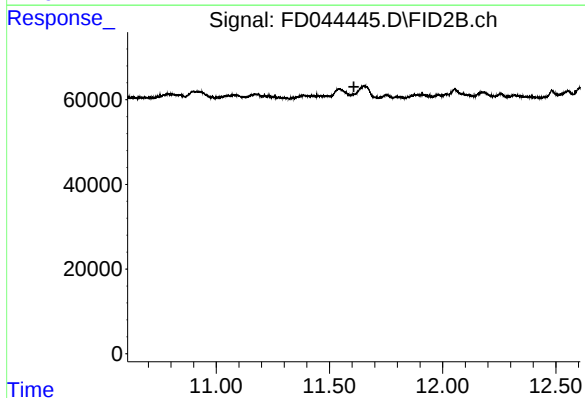


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.608 min
Response: 0
Conc: N.D.

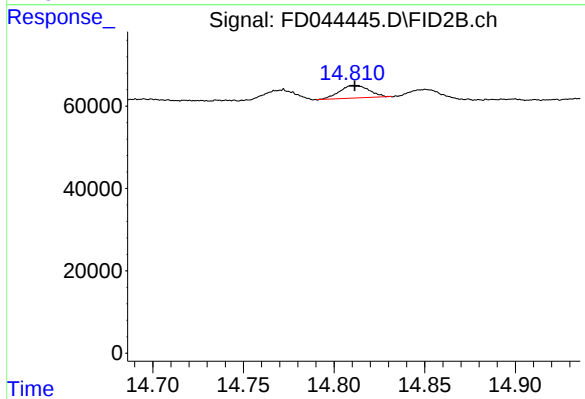

#14 Benzo[a]anthracene (C26.37)

R.T.: 14.812 min
Delta R.T.: 0.000 min
Response: 34433
Conc: 0.25 ug/ml

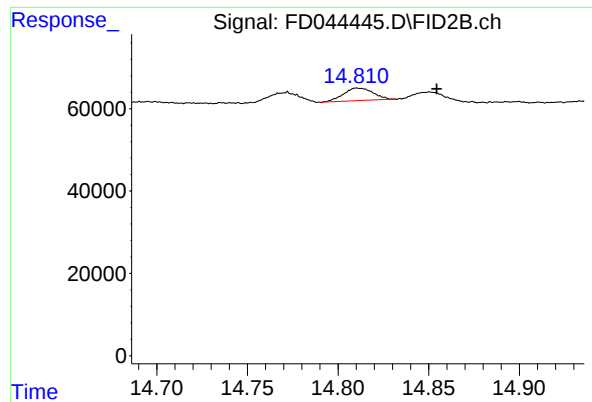

#15 Chrysene (C27.41)

R.T.: 14.812 min
Delta R.T.: -0.043 min
Response: 34433
Conc: 0.24 ug/ml

Instrument :
FID_D
ClientSampleId :
MECL2