

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD111821AL\  
 Data File : FD039520.D  
 Signal(s) : FID2B.CH  
 Acq On : 19 Nov 2021 7:29  
 Operator : AJ\MA  
 Sample : M4744-10  
 Misc :  
 ALS Vial : 73 Sample Multiplier: 1

Instrument :  
 FID\_D  
 ClientSampleId :  
 B-5-4

Manual Integrations  
 APPROVED

Reviewed By :Ankita Jodhani 11/19/2021  
 Supervised By :Sohil Jodhani 11/22/2021

Integration File: autoint1.e  
 Quant Time: Nov 19 08:32:15 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102621.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Oct 27 04:49:08 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 11.665 | 3493993    | 27.385 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 54.77%        |
| 12) S 1-chlorooctadecane (S... | 13.094 | 3016771    | 29.028 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 58.06%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD111821AL\  
Data File : FD039520.D  
Signal(s) : FID2B.CH  
Acq On : 19 Nov 2021 7:29  
Operator : AJ\MA  
Sample : M4744-10  
Misc :  
ALS Vial : 73 Sample Multiplier: 1


Instrument :  
FID\_D  
ClientSampleId :  
B-5-4


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021  
Supervised By :Sohil Jodhani 11/22/2021

Integration File: autoint1.e  
Quant Time: Nov 19 08:32:15 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102621.M  
Quant Title : GC Extractables  
QLast Update : Wed Oct 27 04:49:08 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

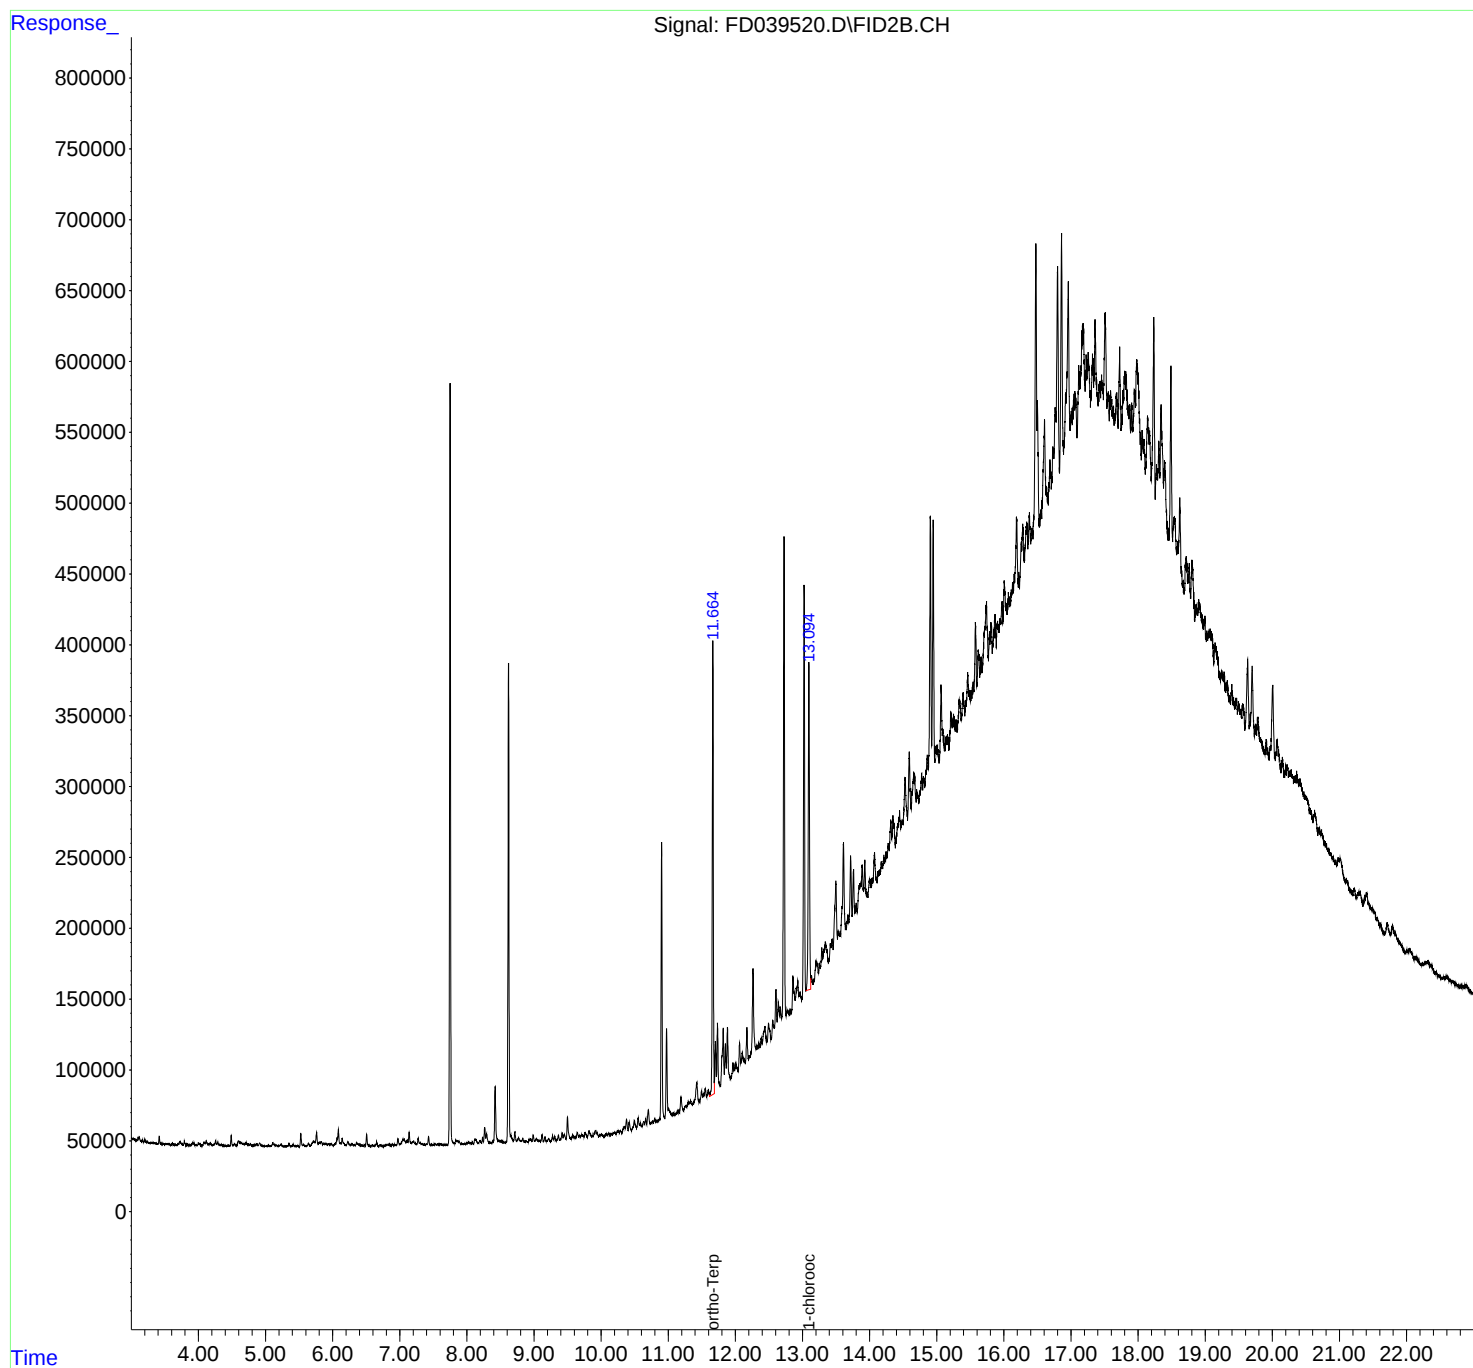

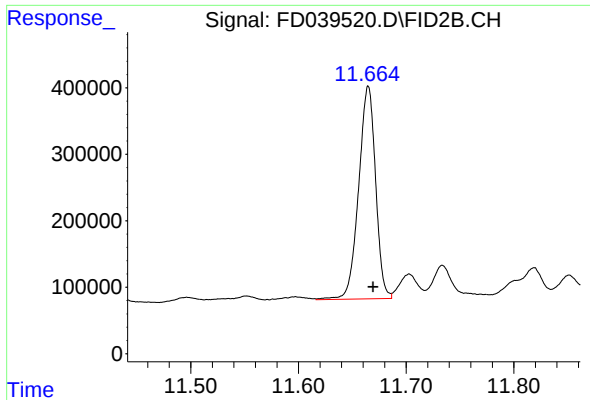


#9 ortho-Terphenyl (SURR)

R.T.: 11.665 min  
Delta R.T.: -0.005 min  
Response: 3493993  
Conc: 27.38 ug/ml

Instrument :  
FID\_D  
ClientSampleId :  
B-5-4

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021  
Supervised By :Sohil Jodhani 11/22/2021

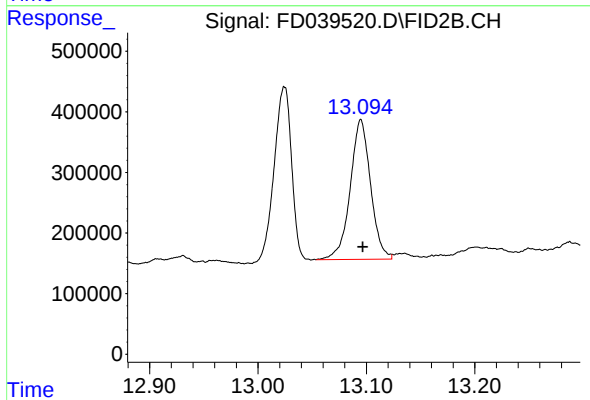

#12 1-chlorooctadecane (SURR)

R.T.: 13.094 min  
Delta R.T.: -0.002 min  
Response: 3016771  
Conc: 29.03 ug/ml m