

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD112221AL\  
 Data File : FD039602.D  
 Signal(s) : FID2B.CH  
 Acq On : 23 Nov 2021 7:28  
 Operator : AJ\MA  
 Sample : M4758-36  
 Misc :  
 ALS Vial : 78 Sample Multiplier: 1

Instrument :  
 FID\_D  
 ClientSampleId :  
 TP18-B

Manual Integrations  
 APPROVED

Reviewed By :Ankita Jodhani 11/23/2021  
 Supervised By :Sohil Jodhani 11/23/2021

Integration File: autoint1.e  
 Quant Time: Nov 23 08:31:09 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102621.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Oct 27 04:49:08 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 11.661 | 5327724    | 41.757 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 83.51%        |
| 12) S 1-chlorooctadecane (S... | 13.088 | 4513090    | 43.426 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 86.85%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD112221AL\  
Data File : FD039602.D  
Signal(s) : FID2B.CH  
Acq On : 23 Nov 2021 7:28  
Operator : AJ\MA  
Sample : M4758-36  
Misc :  
ALS Vial : 78 Sample Multiplier: 1


Instrument :  
FID\_D  
ClientSampleId :  
TP18-B


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 11/23/2021  
Supervised By :Sohil Jodhani 11/23/2021

Integration File: autoint1.e  
Quant Time: Nov 23 08:31:09 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102621.M  
Quant Title : GC Extractables  
QLast Update : Wed Oct 27 04:49:08 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

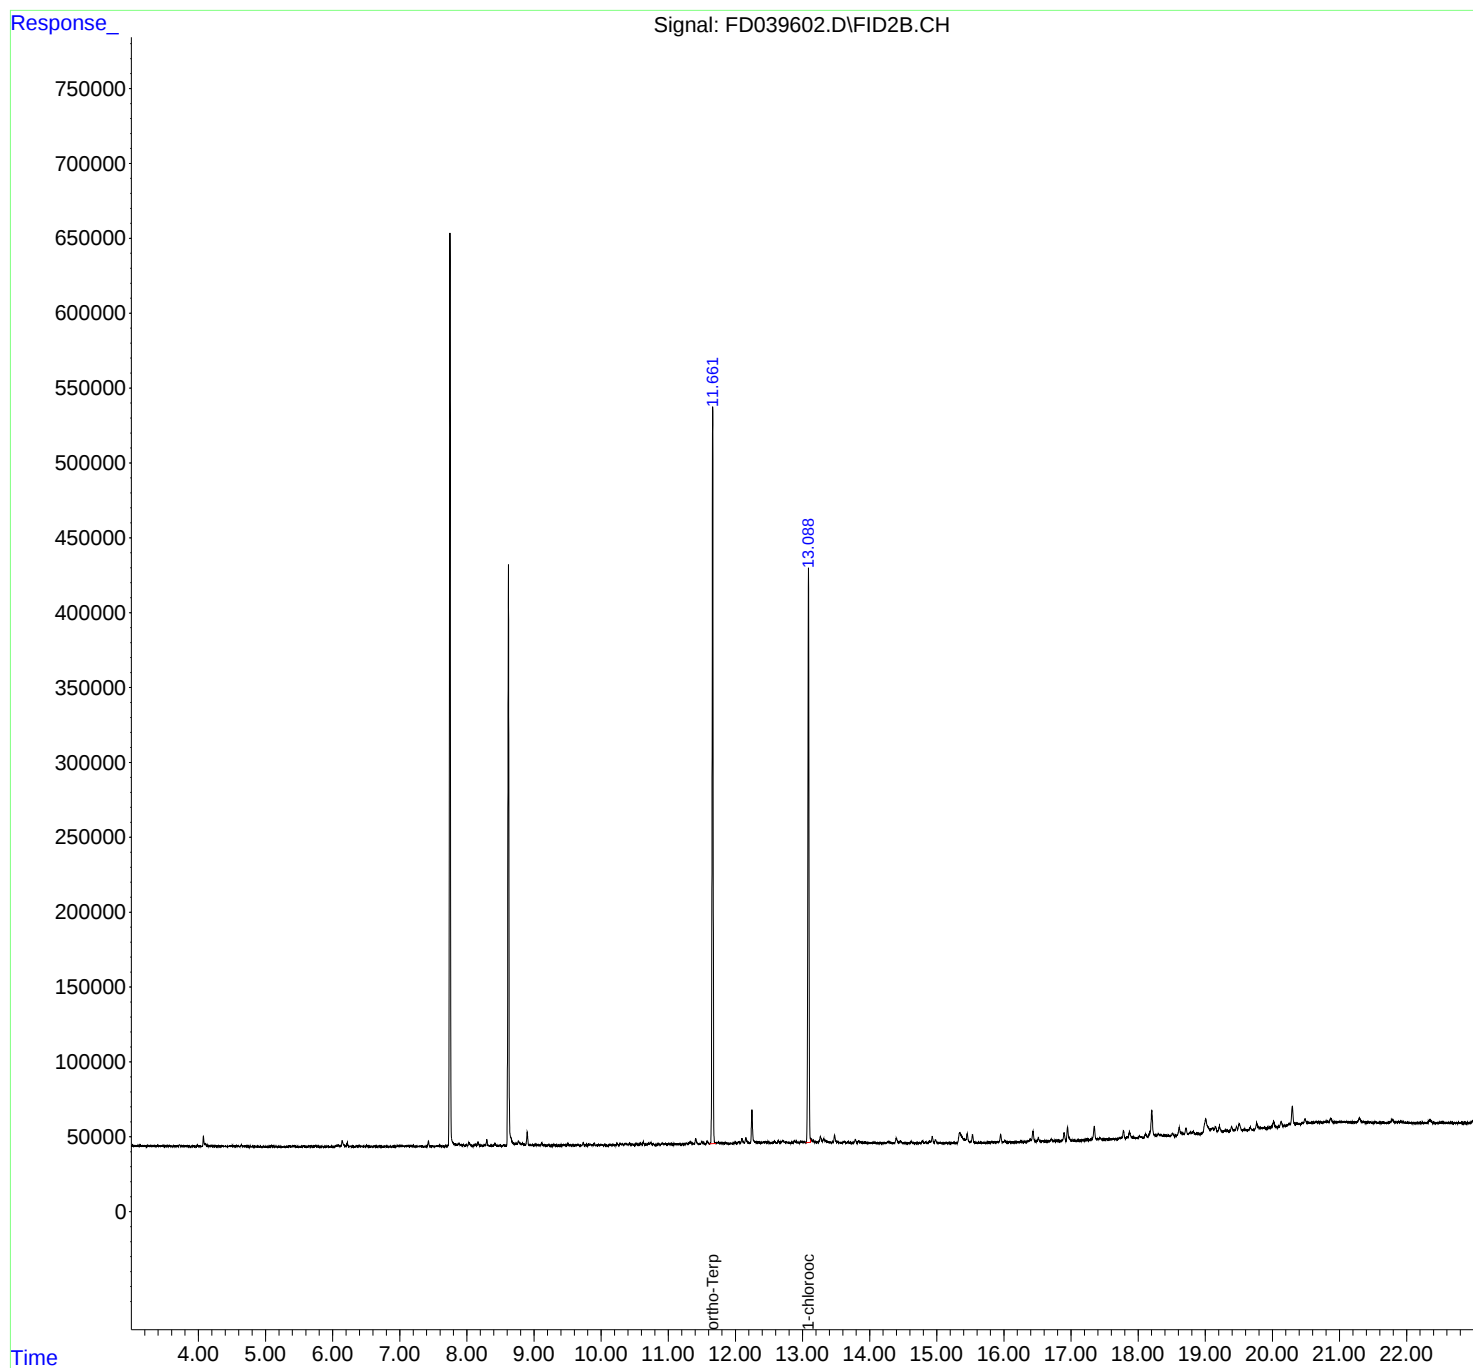

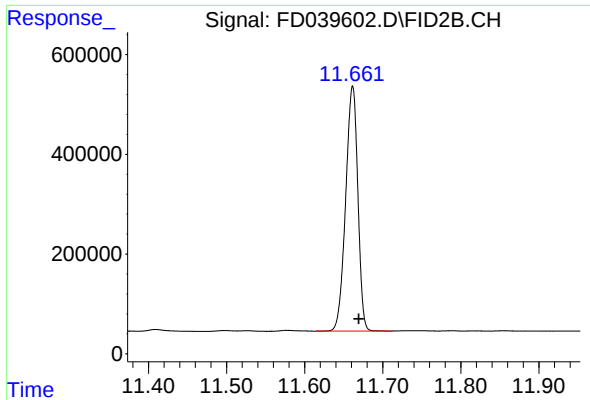


#9 ortho-Terphenyl (SURR)

R.T.: 11.661 min  
Delta R.T.: -0.008 min  
Response: 5327724  
Conc: 41.76 ug/ml

Instrument :  
FID\_D  
ClientSampleId :  
TP18-B

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 11/23/2021  
Supervised By :Sohil Jodhani 11/23/2021

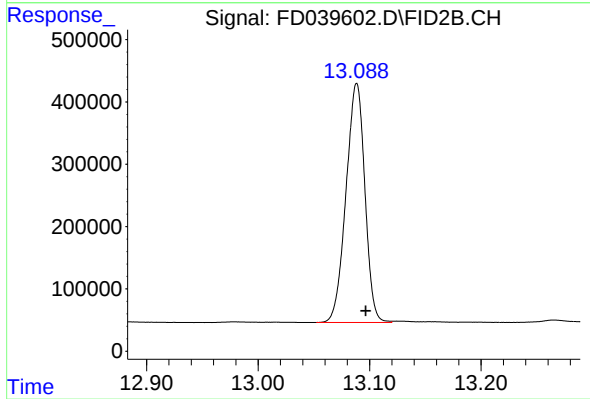

#12 1-chlorooctadecane (SURR)

R.T.: 13.088 min  
Delta R.T.: -0.008 min  
Response: 4513090  
Conc: 43.43 ug/ml m